

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
 Data File : BF128119.D
 Acq On : 06 May 2022 11:38
 Operator : CG\JU
 Sample : N2672-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 09

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.151	483	487	496	rVB	26003	34643	1.09%	0.180%
2	5.534	547	552	555	rBV	2594741	2497043	78.40%	12.961%
3	6.540	717	723	726	rBV	2468468	2635367	82.74%	13.679%
4	6.904	781	785	789	rBV	618677	473751	14.87%	2.459%
5	7.475	876	882	885	rBV	1678694	1788714	56.16%	9.285%
6	8.187	999	1003	1007	rBV	723306	597960	18.77%	3.104%
7	9.263	1181	1186	1189	rBV	3315226	3029468	95.11%	15.725%
8	9.945	1298	1302	1305	rBV	905103	726260	22.80%	3.770%
9	10.739	1432	1437	1440	rBV	2394792	2161355	67.86%	11.219%
10	11.439	1552	1556	1559	rBV	932506	797924	25.05%	4.142%
11	13.027	1821	1826	1829	rBV	3477220	3185169	100.00%	16.533%
12	13.921	1973	1978	1992	rBV3	98873	243552	7.65%	1.264%
13	14.086	2001	2006	2009	rBV	611502	597939	18.77%	3.104%
14	14.921	2145	2148	2153	rVB	41759	43902	1.38%	0.228%
15	15.586	2255	2261	2268	rBV	355570	452210	14.20%	2.347%




Sum of corrected areas: 19265257

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
Data File : BF128119.D
Acq On : 06 May 2022 11:38
Operator : CG\JU
Sample : N2672-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

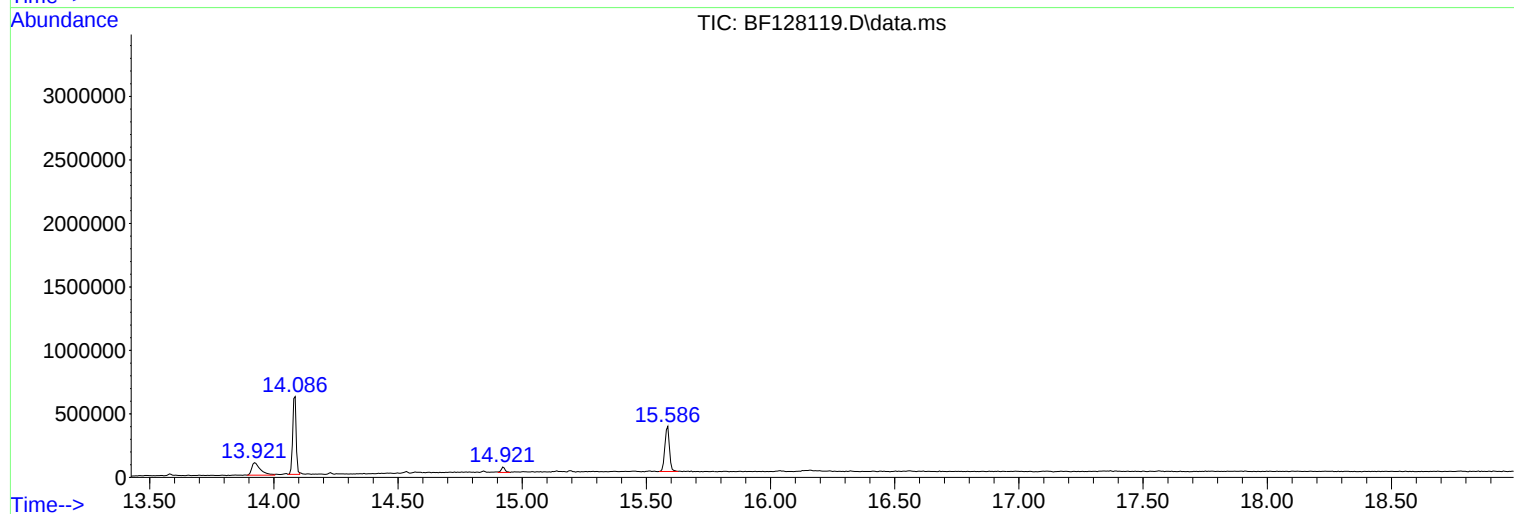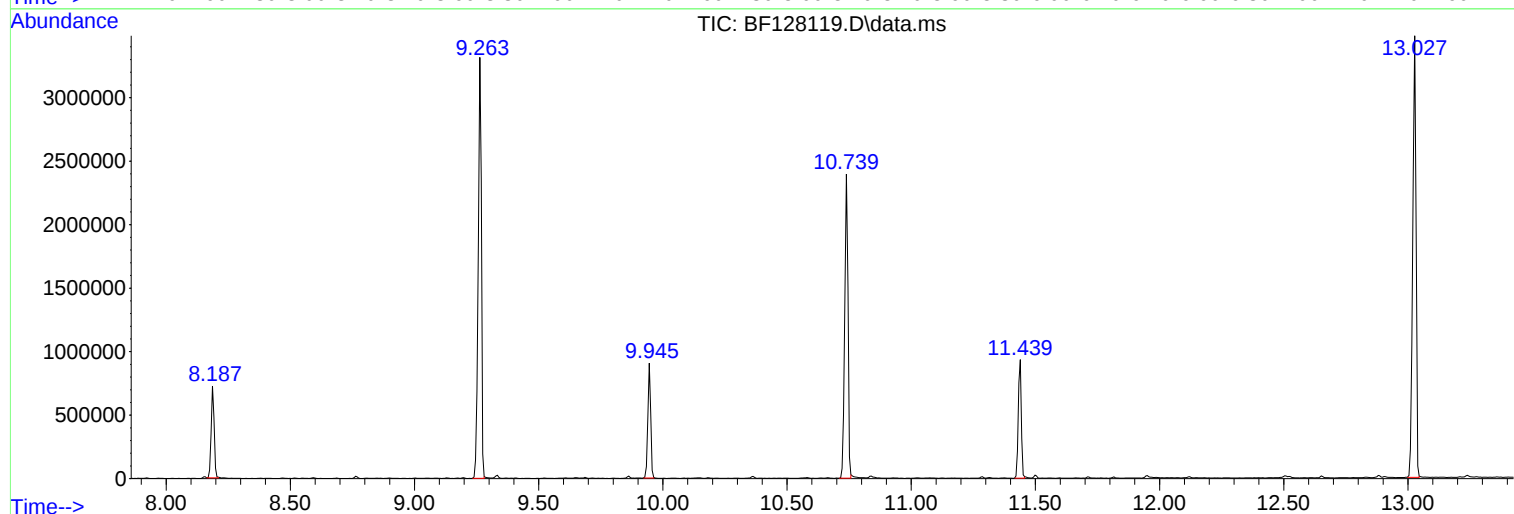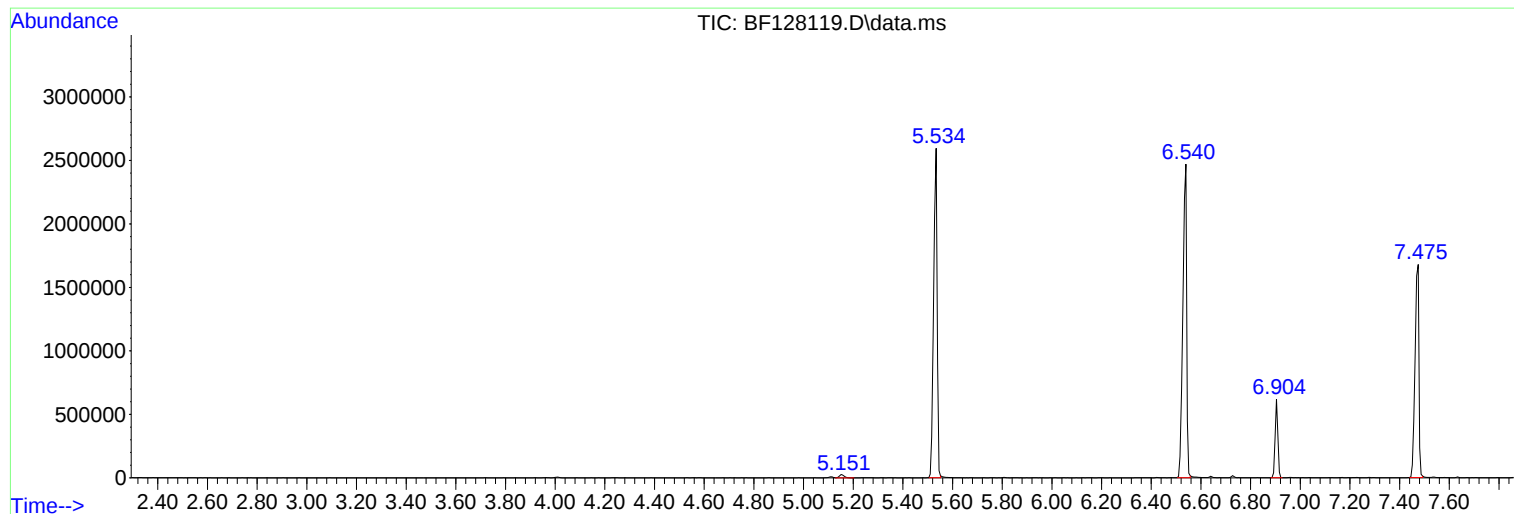

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
Data File : BF128119.D
Acq On : 06 May 2022 11:38
Operator : CG\JU
Sample : N2672-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
09










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Eicosene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.921	8.15 ng	243552	Chrysene-d12	14.086

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Eicosene, (E)-	280	C20H40	074685-33-9	94
2			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94
5			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94

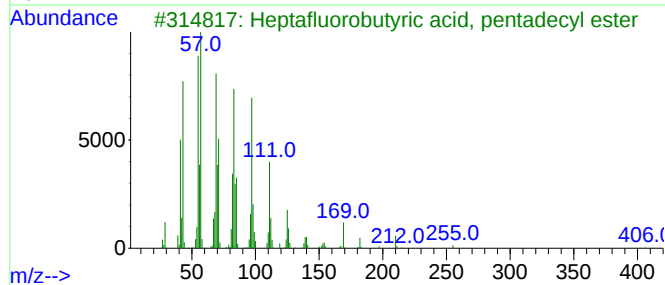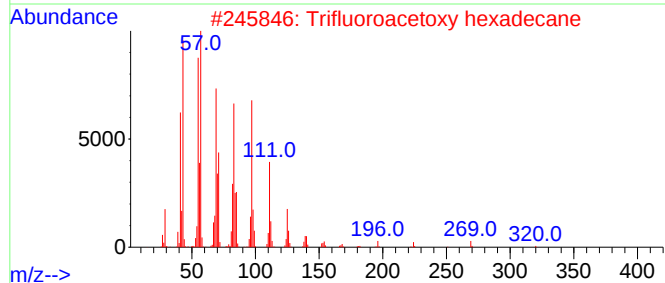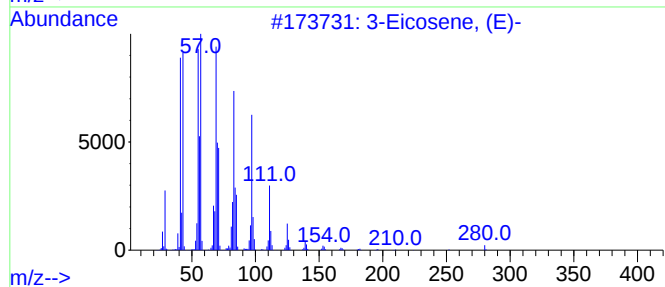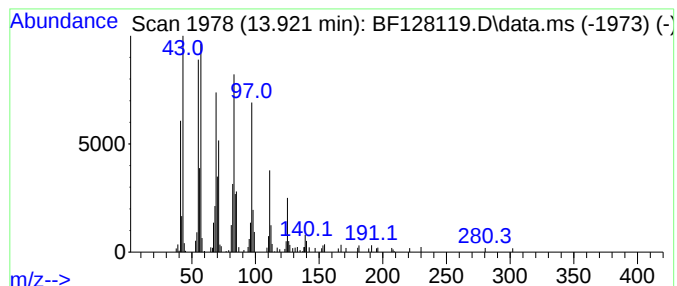

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
Data File : BF128119.D
Acq On : 06 May 2022 11:38
Operator : CG\JU
Sample : N2672-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Eicosene, (E)-	13.921	8.2	ng	243552	5	14.086	597939	20.0