
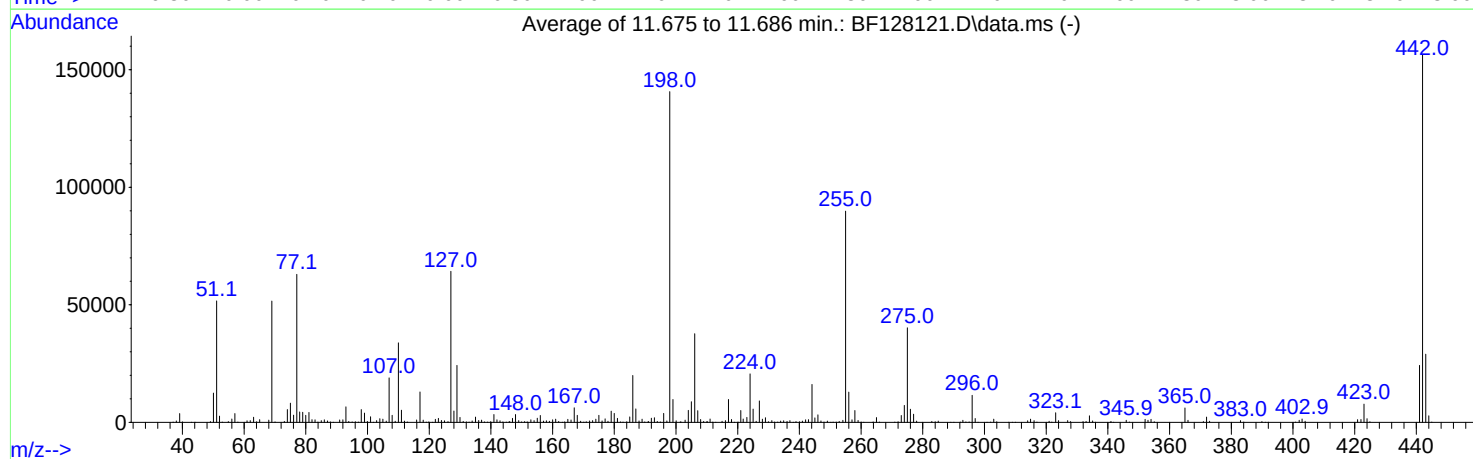


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
 Data File : BF128121.D
 Acq On : 06 May 2022 13:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 17:56:23 2022

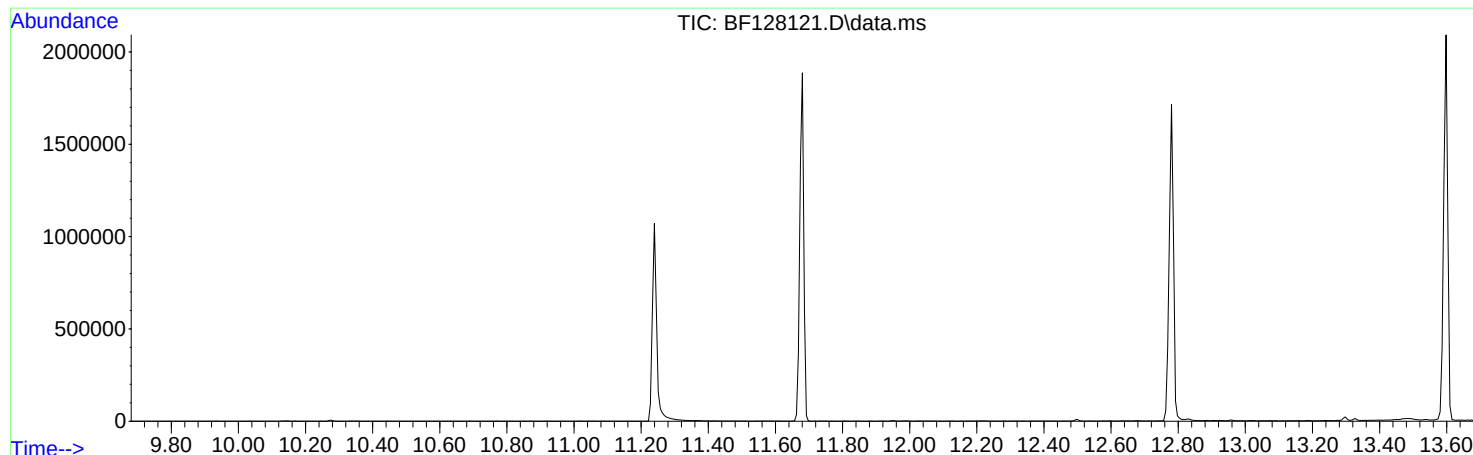




AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	51691	PASS
68	69	0.00	2	1.9	964	PASS
69	198	0.00	100	36.7	51631	PASS
70	69	0.00	2	0.5	244	PASS
127	198	10	80	45.6	64235	PASS
197	198	0.00	2	0.4	630	PASS
198	198	100	100	100.0	140717	PASS
199	198	5	9	6.9	9704	PASS
275	198	10	60	28.6	40232	PASS
365	198	1	100	4.4	6148	PASS
441	198	0.01	100	17.2	24235	PASS
442	442	50	100	100.0	156480	PASS
443	442	15	24	18.5	28973	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
Data File : BF128121.D
Acq On : 06 May 2022 13:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 06 16:20:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 17:56:23 2022
Response via : Initial Calibration

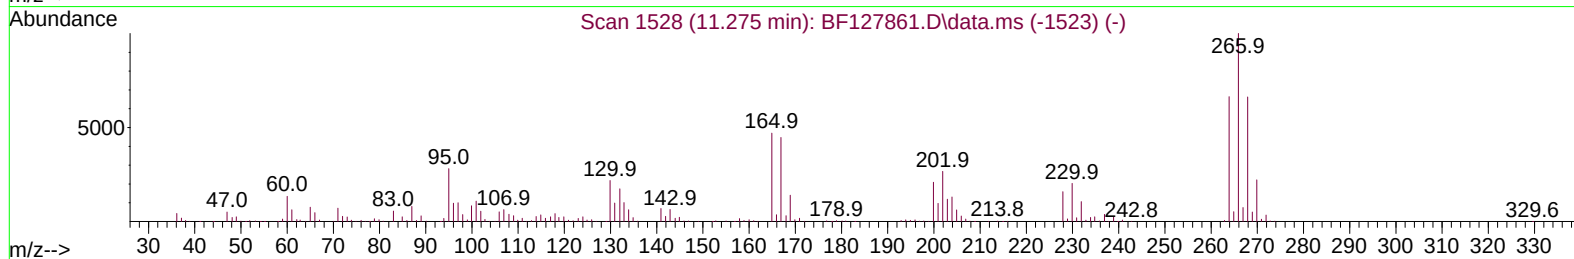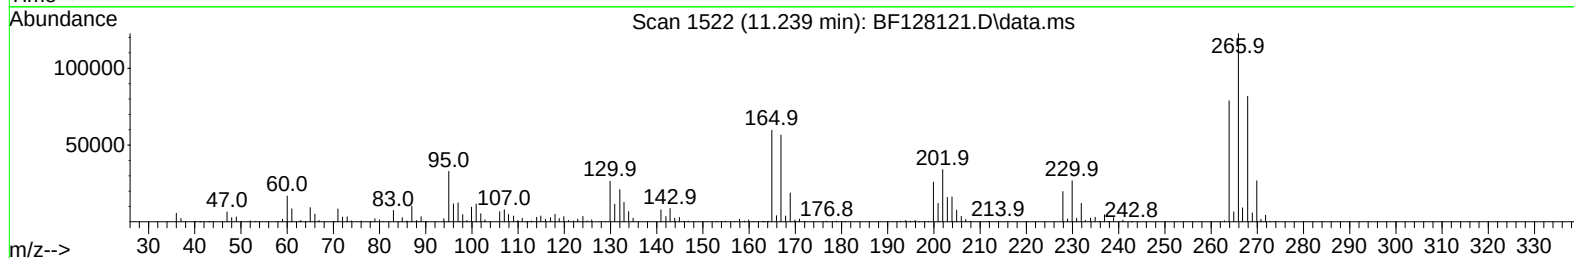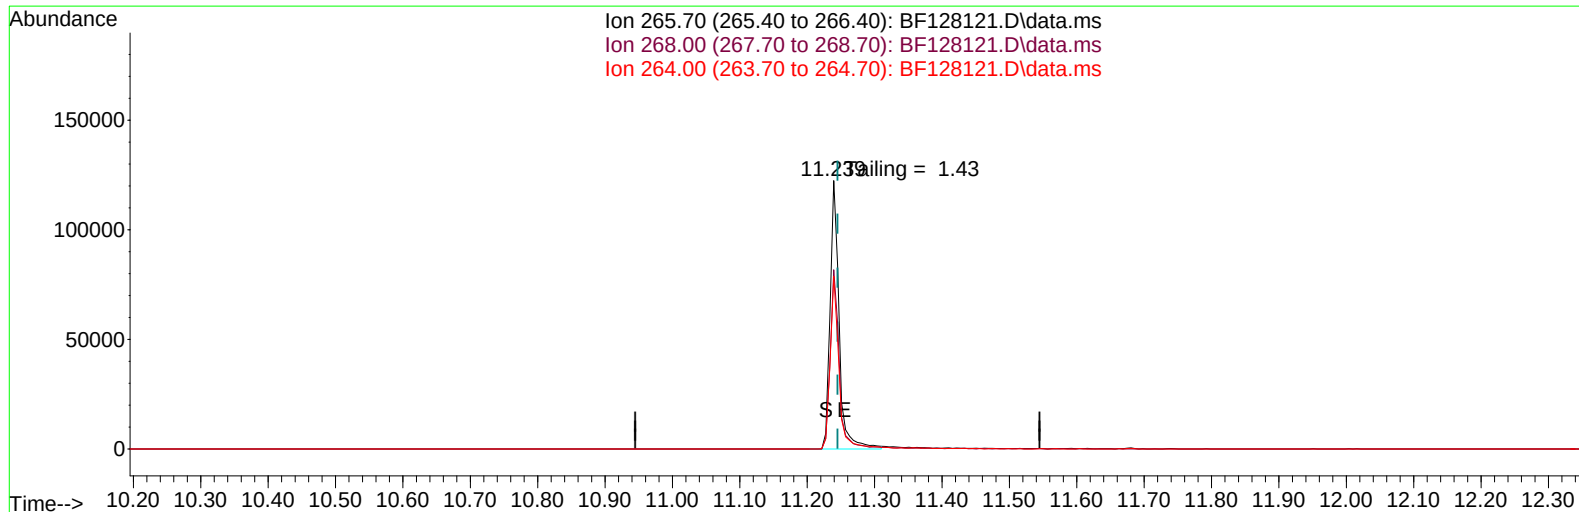

TIC: BF128121.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.006) 22154.29 ng




response 116757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.80
264.00	66.40	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
 Data File : BF128121.D
 Acq On : 06 May 2022 13:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 06 16:20:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 05 17:56:23 2022
 Response via : Initial Calibration

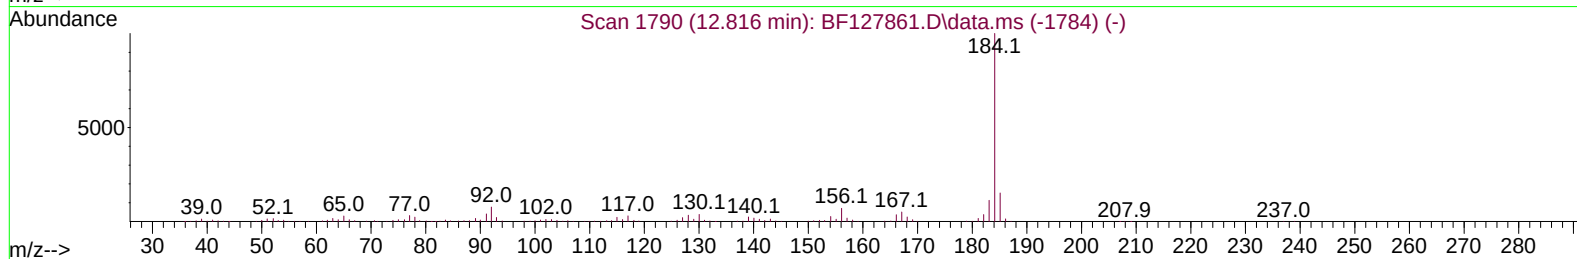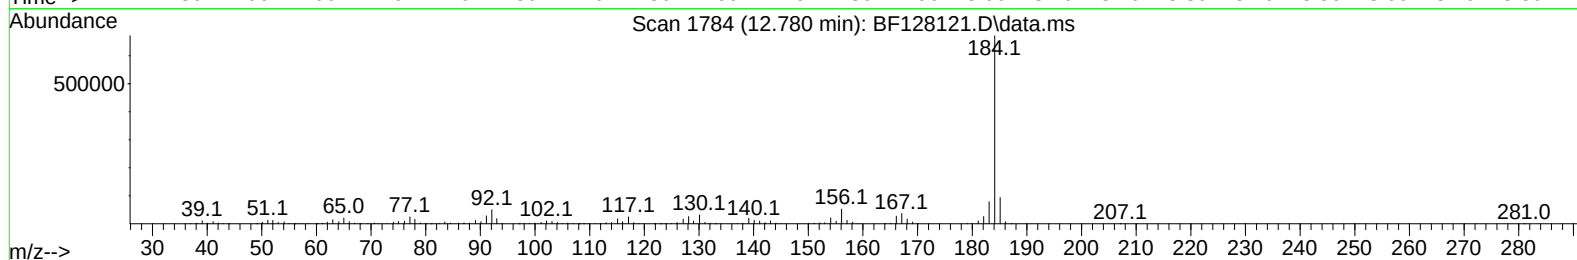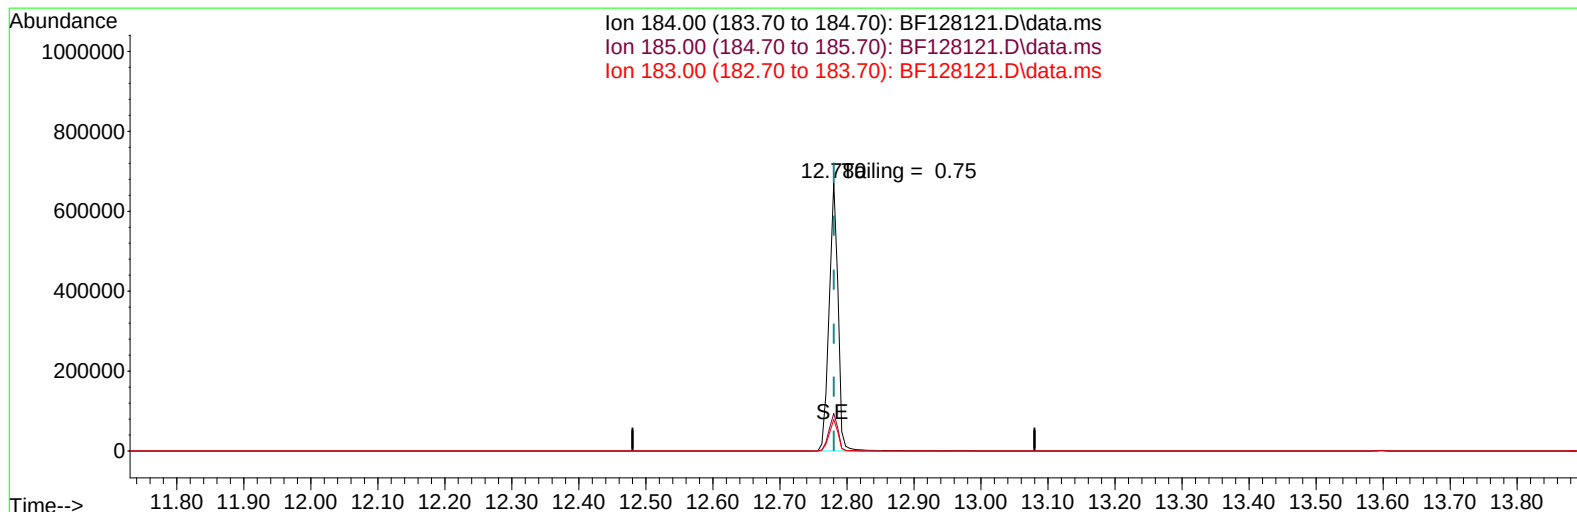

TIC: BF128121.D\data.ms

(77) Benzidine

12.780min (+ 0.000) 0.00 ng

response 620937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.01
183.00	11.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2022	BNA_F	<u>BF128121.D</u>
Compound Name	Response	Retention Time
DDT	339448	13.59
DDD	3642	13.29
DDE	783	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4425	343873	1.29

Instrument :
BNA_F
ClientSampleId :
DFTPP