
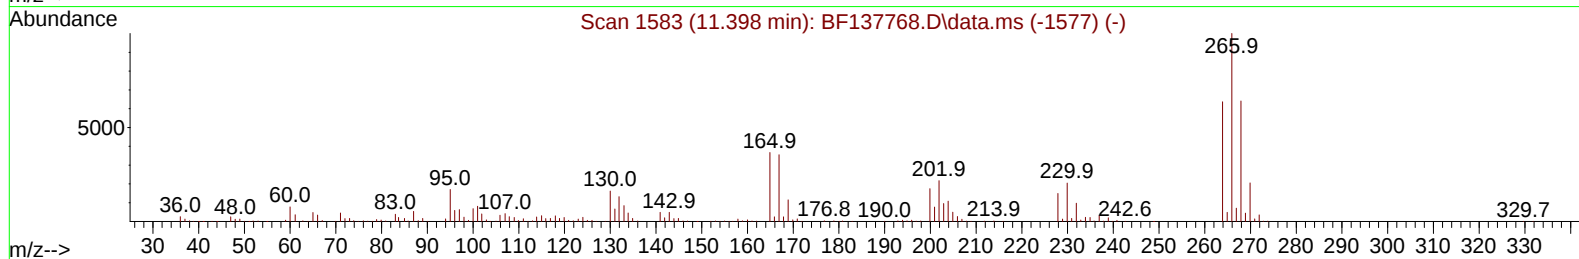
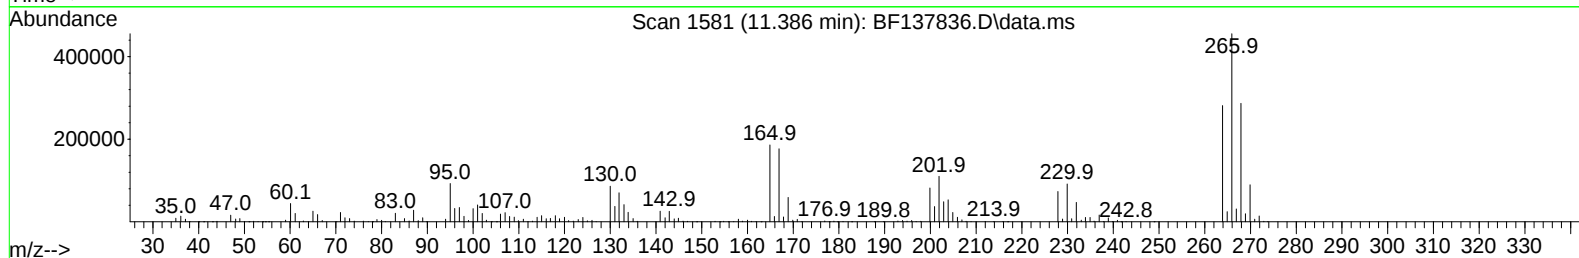


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050624\
Data File : BF137836.D
Acq On : 06 May 2024 11:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:47:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

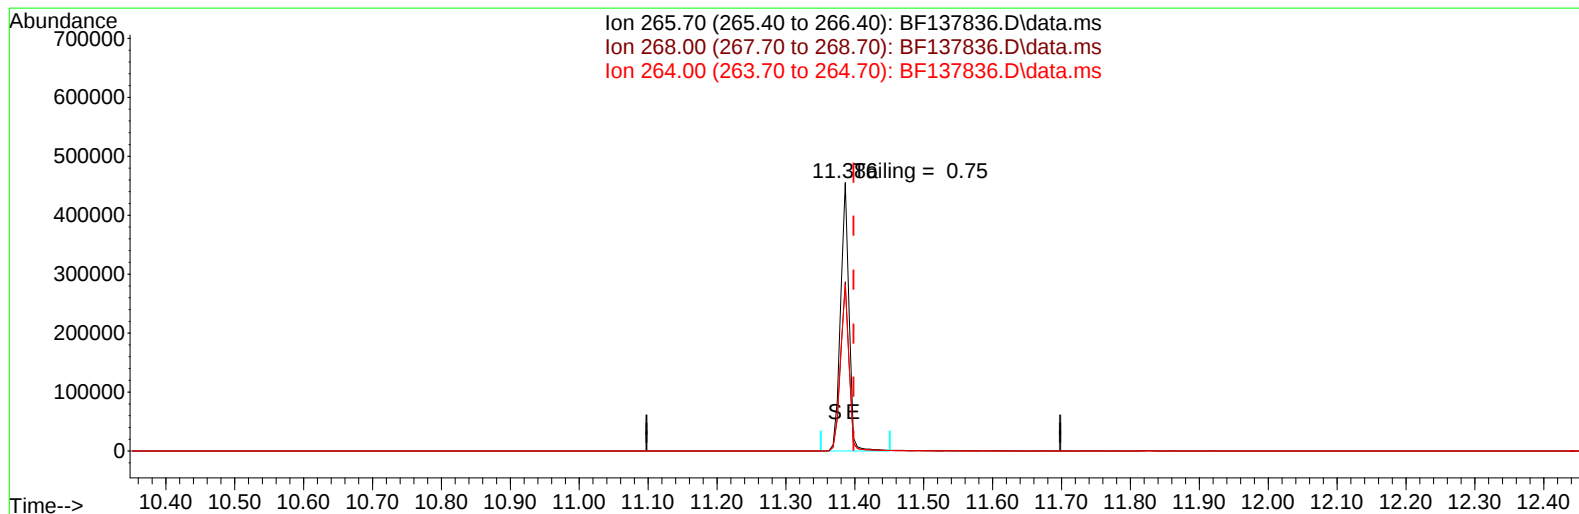

TIC: BF137836.D\data.ms

(70) Pentachlorophenol (C)




11.386min (-0.012) 482458.59 ng

response 391260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.99
264.00	63.70	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050624\
Data File : BF137836.D
Acq On : 06 May 2024 11:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:47:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

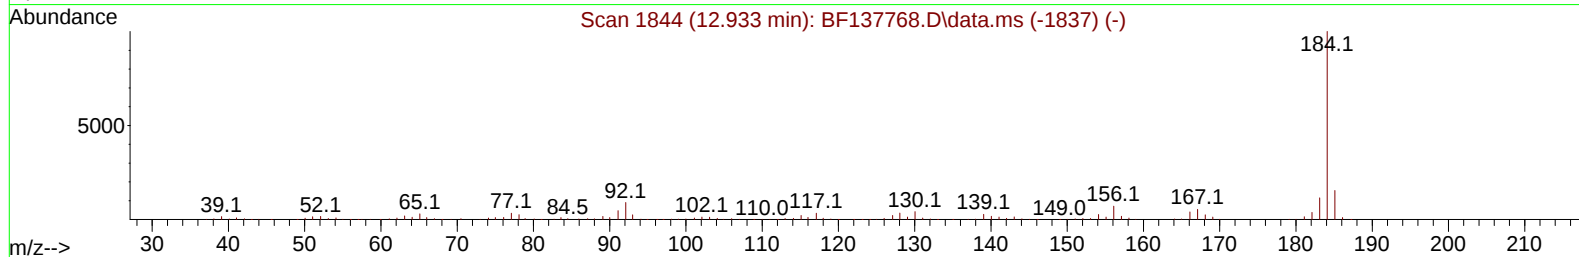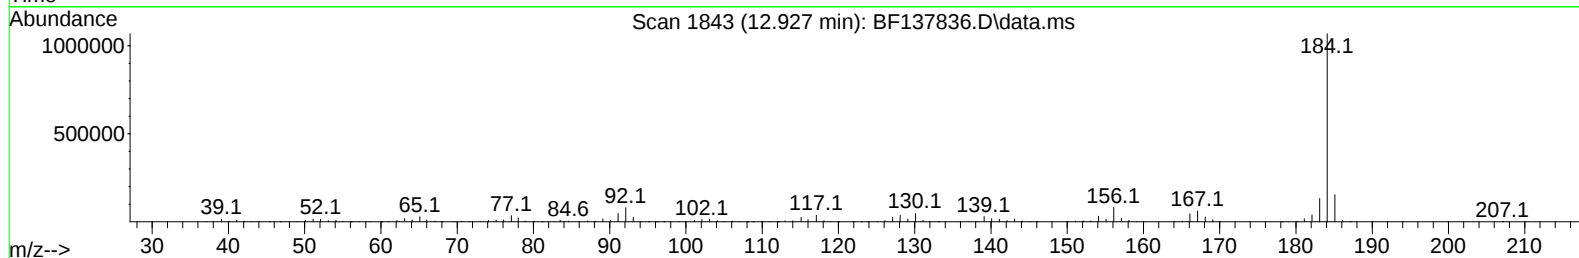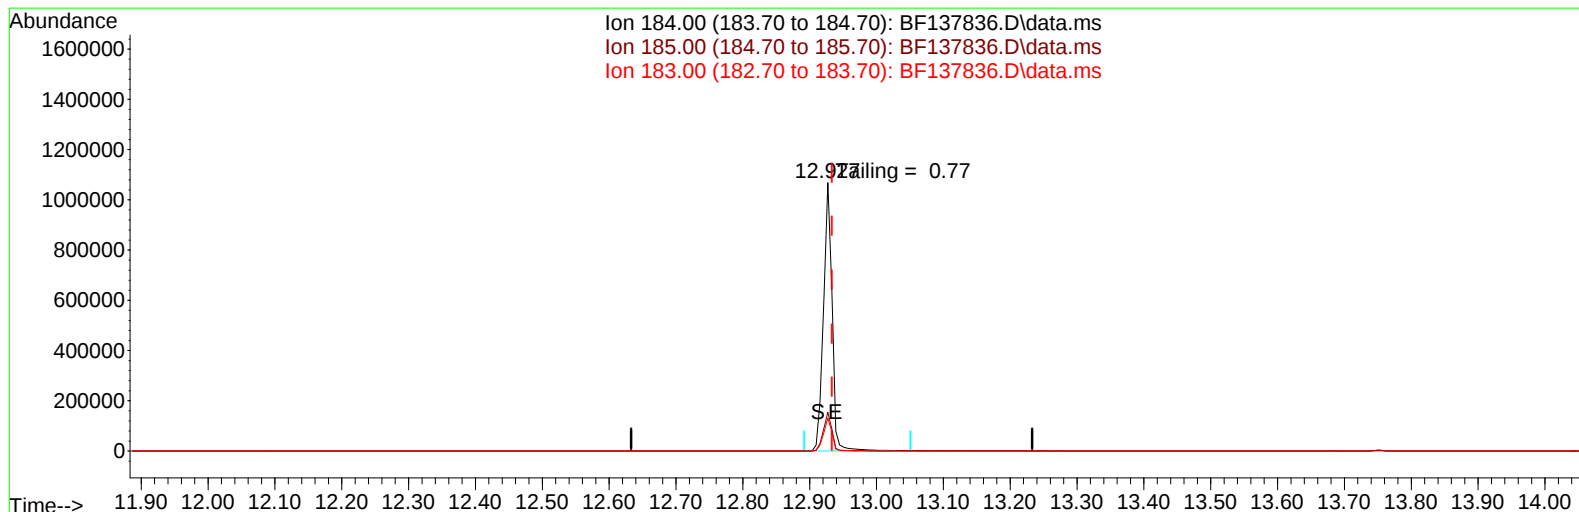

TIC: BF137836.D\data.ms

(77) Benzidine

12.927min (-0.006) 114356.59 ng

response 965354

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.42
183.00	11.50	12.33
0.00	0.00	0.00