


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050624\
Data File : BF137836.D
Acq On : 06 May 2024 11:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

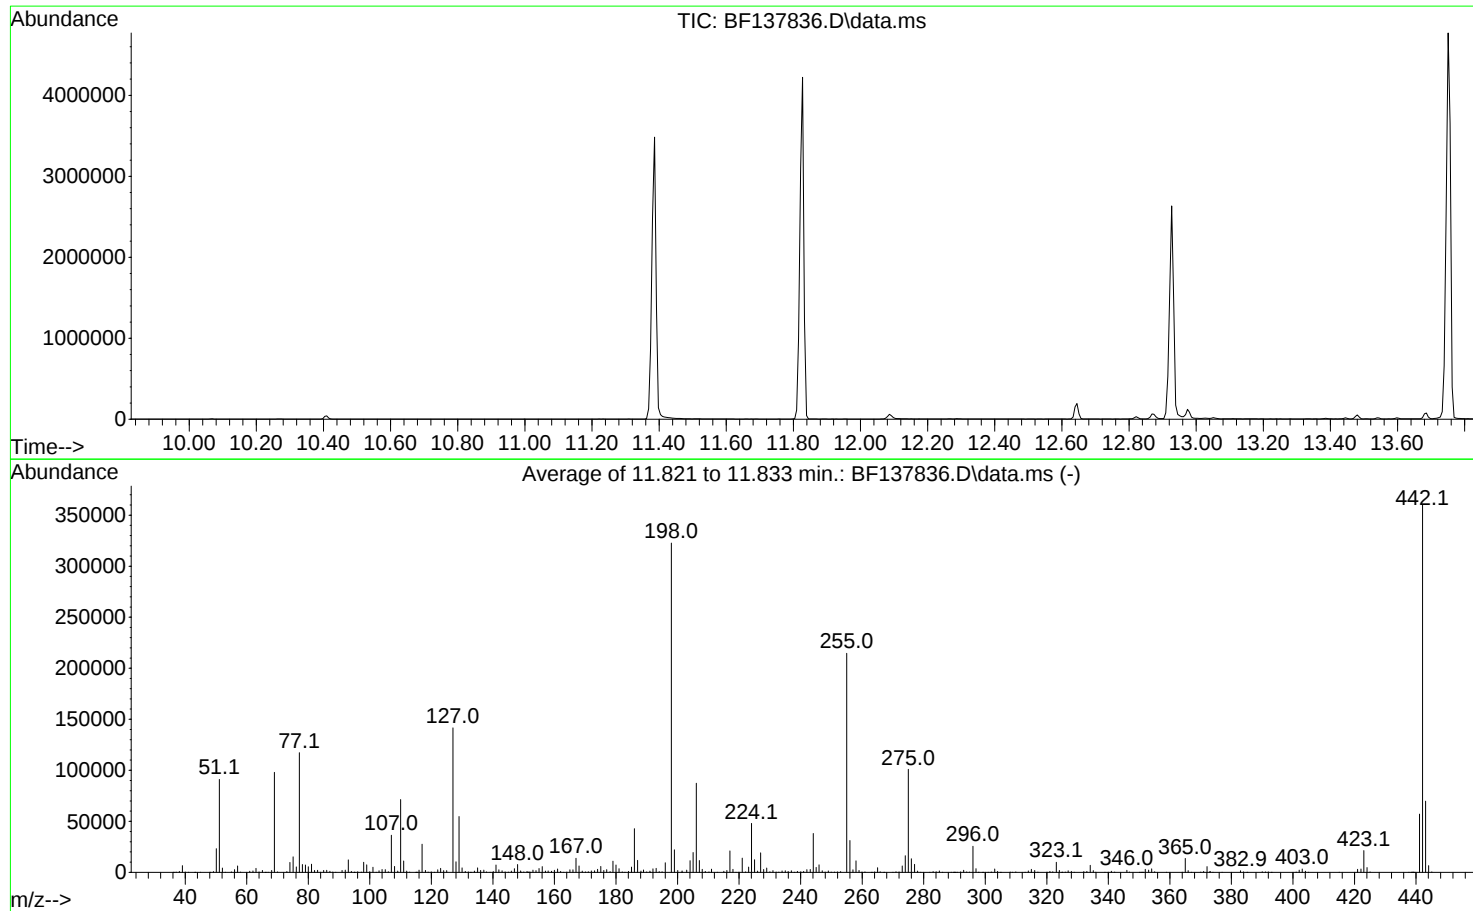




AutoFind: Scans 1655, 1656, 1657; Background Corrected with Scan 1649

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	91155	PASS
68	69	0.00	2	2.0	1941	PASS
69	198	0.00	100	30.4	98003	PASS
70	69	0.00	2	0.6	545	PASS
127	198	10	80	43.9	141656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	322725	PASS
199	198	5	9	6.8	22075	PASS
275	198	10	60	31.3	100923	PASS
365	198	1	100	4.2	13572	PASS
441	198	0.01	100	17.7	57088	PASS
442	442	50	100	100.0	360448	PASS
443	442	15	24	19.3	69744	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050624\
Data File : BF137836.D
Acq On : 06 May 2024 11:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 06 11:47:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

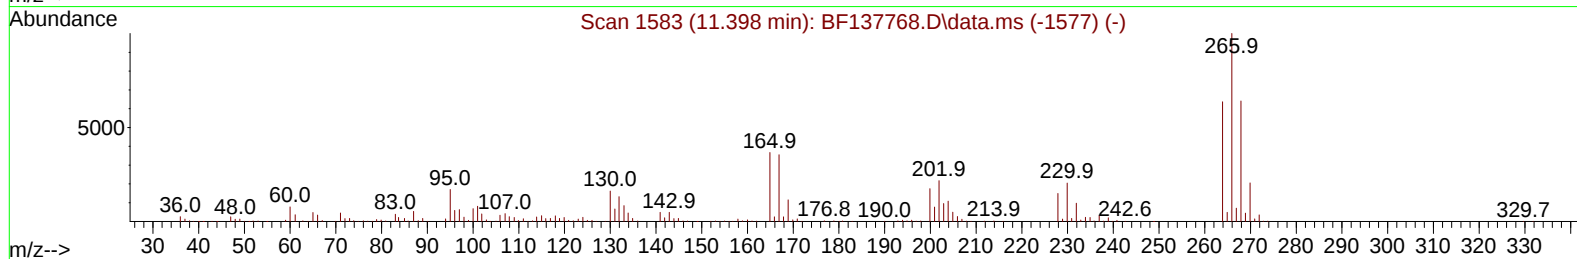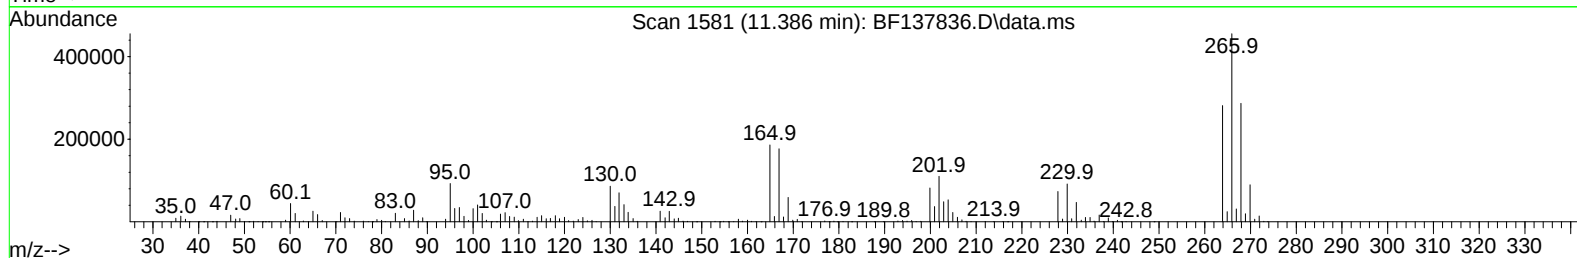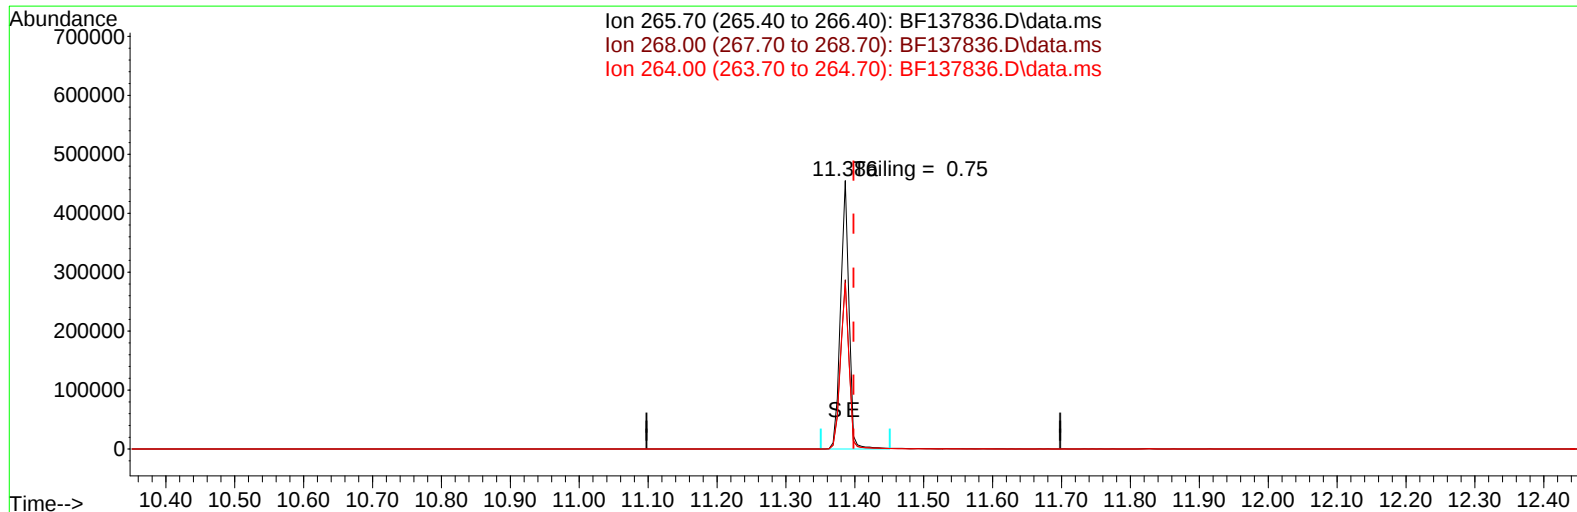

TIC: BF137836.D\data.ms

(70) Pentachlorophenol (C)

11.386min (-0.012) 482458.59 ng




response 391260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.99
264.00	63.70	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050624\
Data File : BF137836.D
Acq On : 06 May 2024 11:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 06 11:47:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

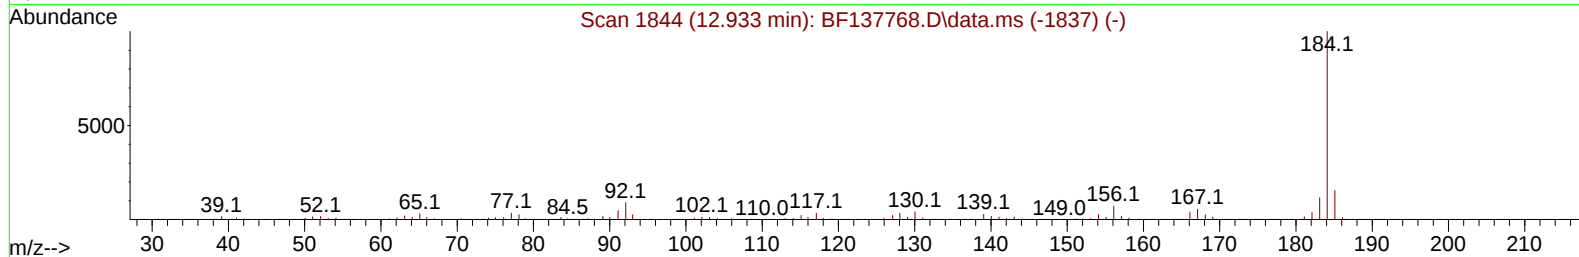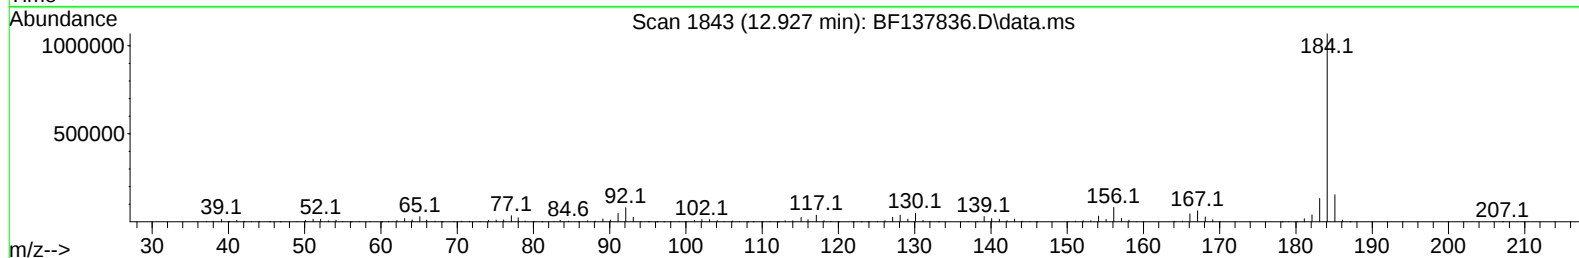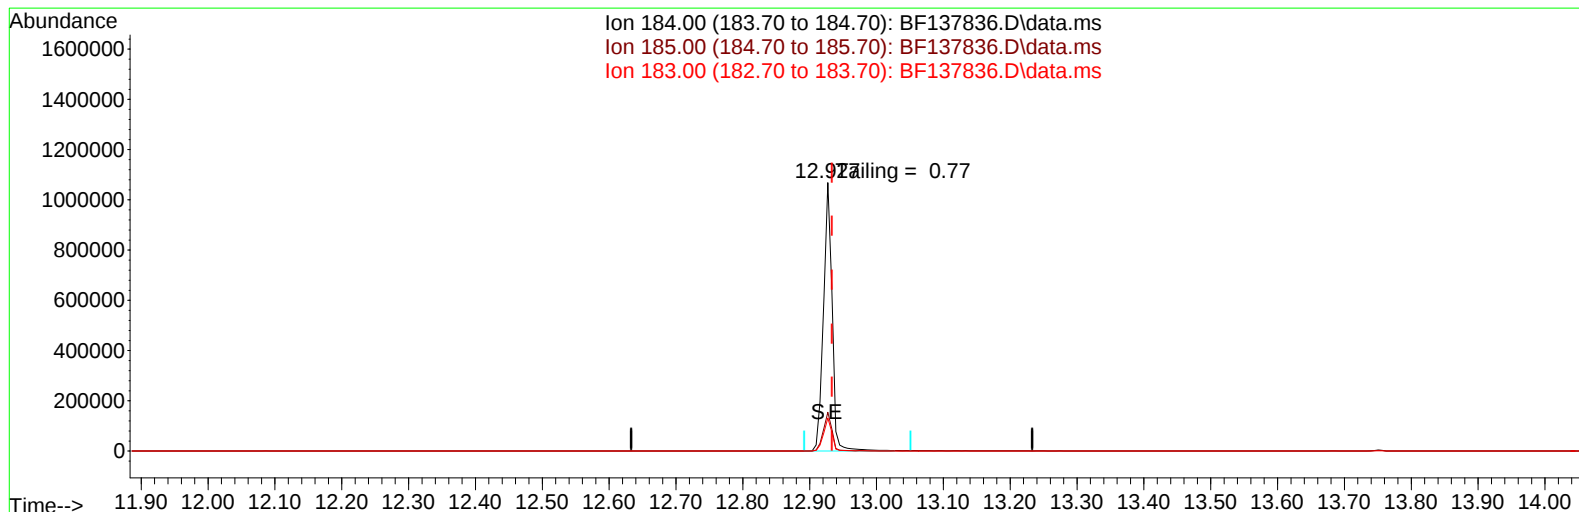

TIC: BF137836.D\data.ms

(77) Benzidine

12.927min (-0.006) 114356.59 ng

response 965354

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.42
183.00	11.50	12.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2024	BNA_F	<u>BF137836.D</u>
Compound Name	Response	Retention Time
DDT	856745	13.751
DDD	9862	13.48
DDE	340	13.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10202	866947	1.18

Instrument :
BNA_F
ClientSampleId :
DFTPP