
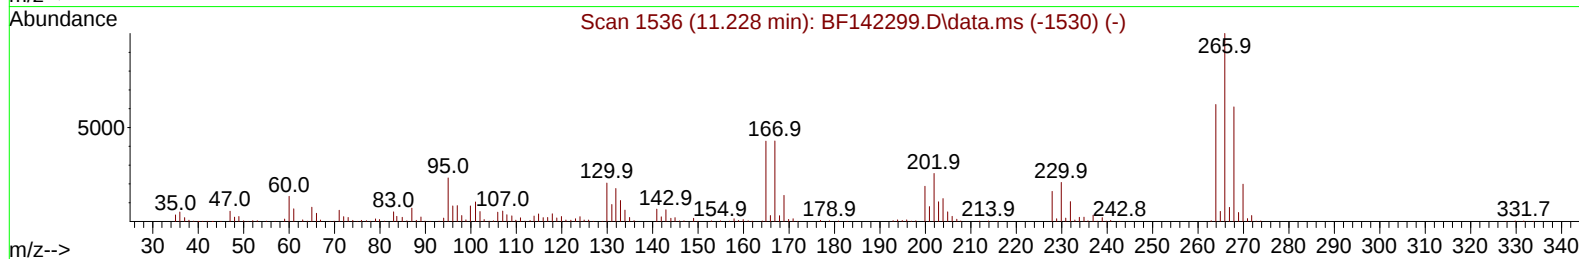
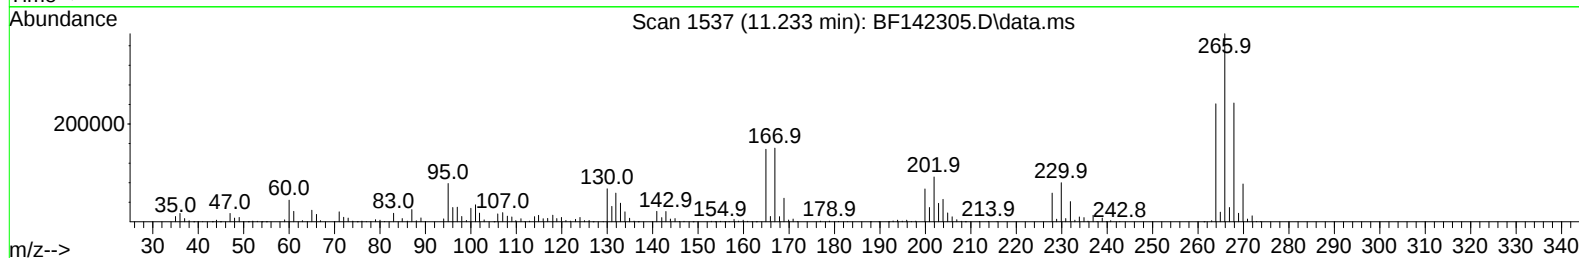


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050625\
Data File : BF142305.D
Acq On : 06 May 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:41:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

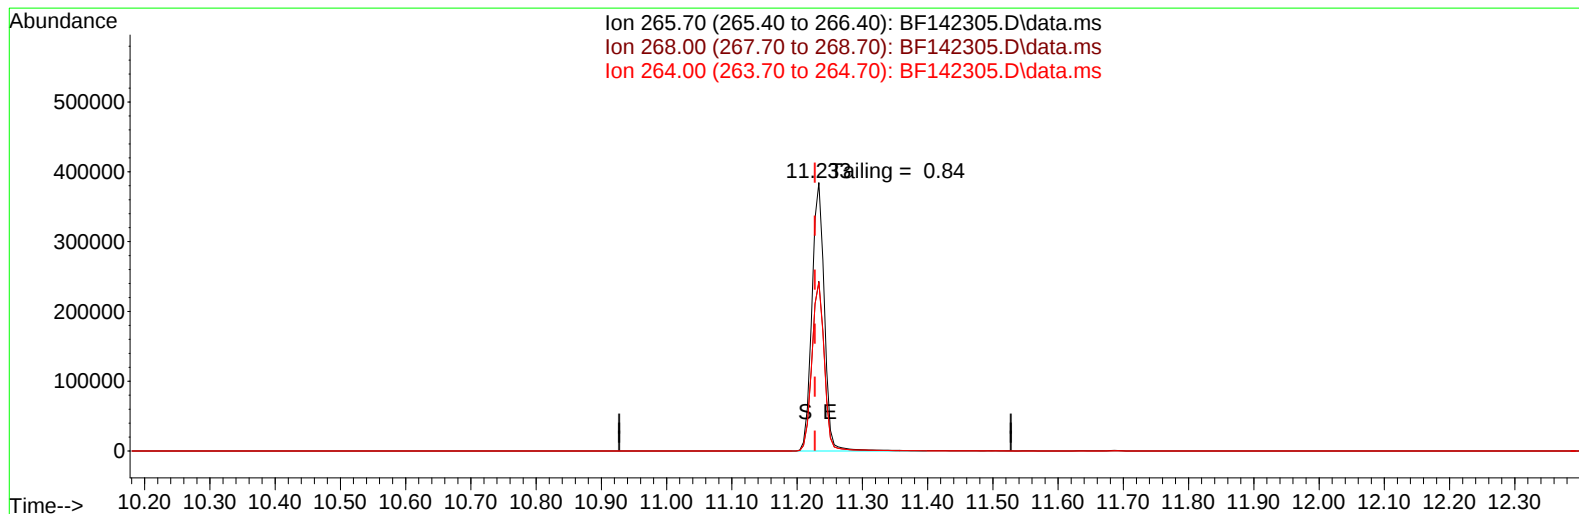

TIC: BF142305.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.006) 53010.55 ng

response 509315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.18
264.00	62.20	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050625\
Data File : BF142305.D
Acq On : 06 May 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:41:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

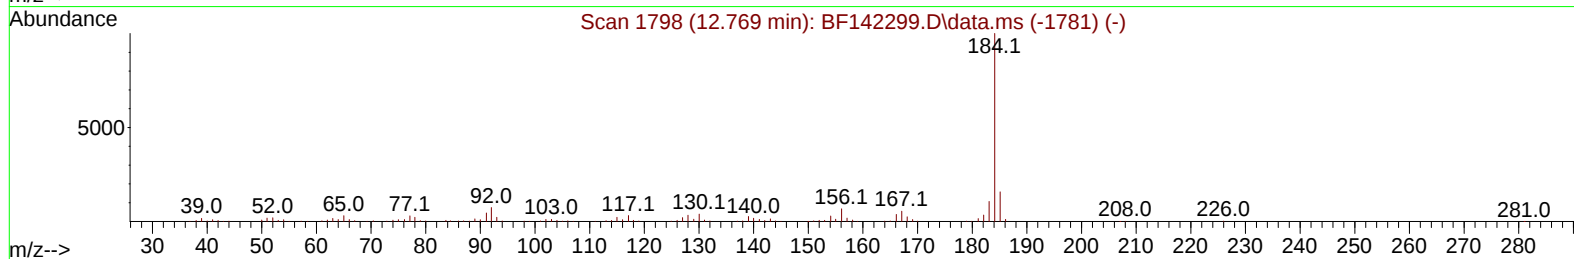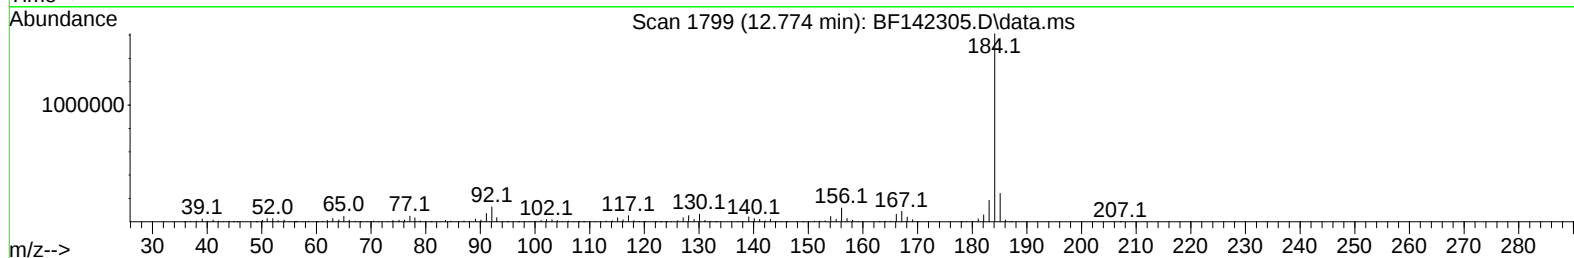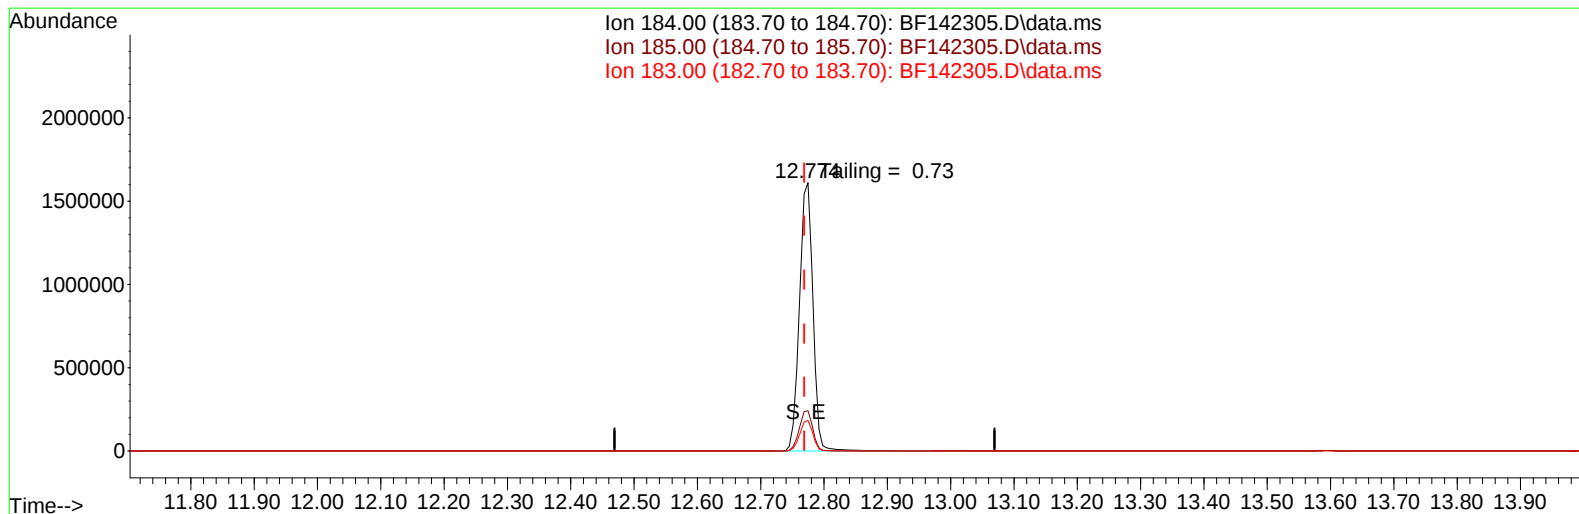

TIC: BF142305.D\data.ms

(77) Benzidine**12.774min (+ 0.005) 45124.90 ng****response 2395357**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	15.07
183.00	10.70	11.43
0.00	0.00	0.00