
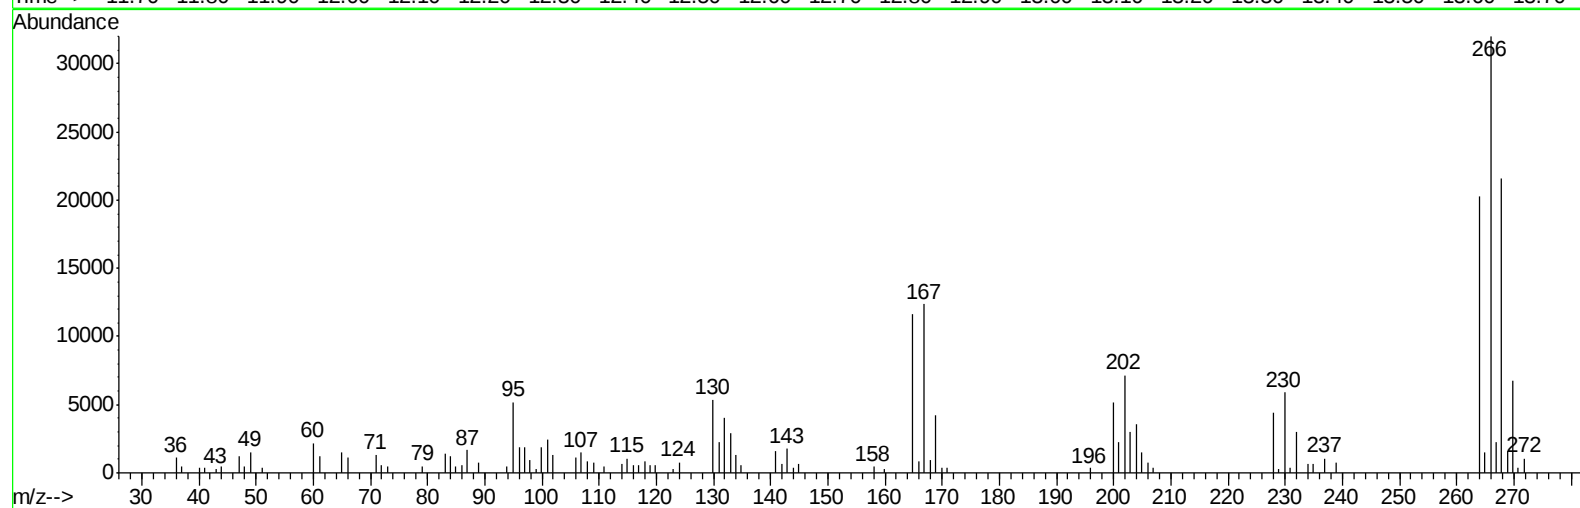


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050715\
Data File : BF079014.D
Acq On : 8 May 2015 1:20
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 06:44:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 08 04:33:44 2015
Response via : Initial Calibration

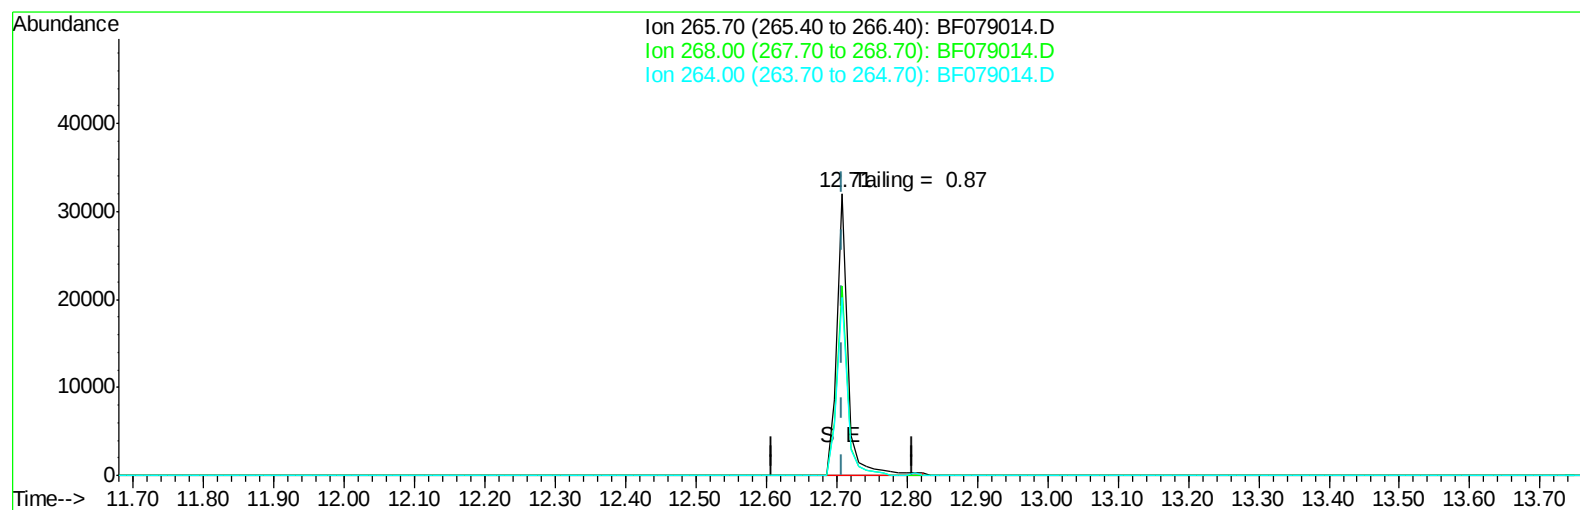

TIC: BF079014.D

(69) Pentachlorophenol (C)



12.708min (-0.000) 0.00ng

response 33510

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.36
264.00	60.20	63.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050715\
Data File : BF079014.D
Acq On : 8 May 2015 1:20
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 06:44:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 08 04:33:44 2015
Response via : Initial Calibration

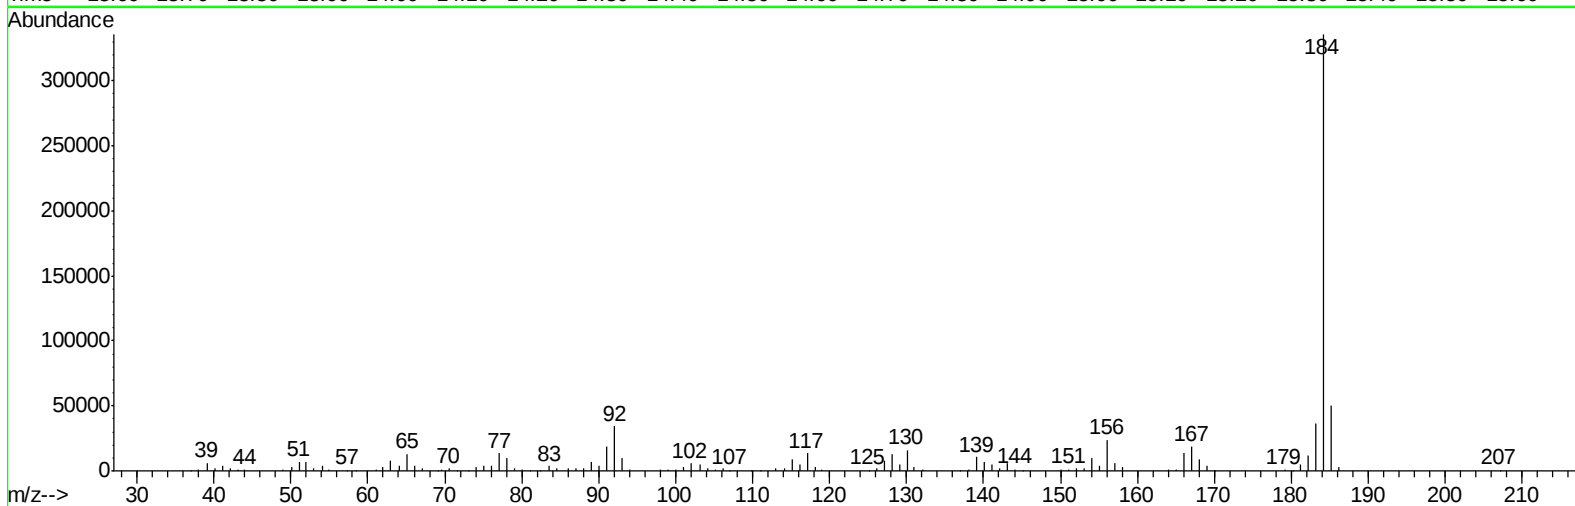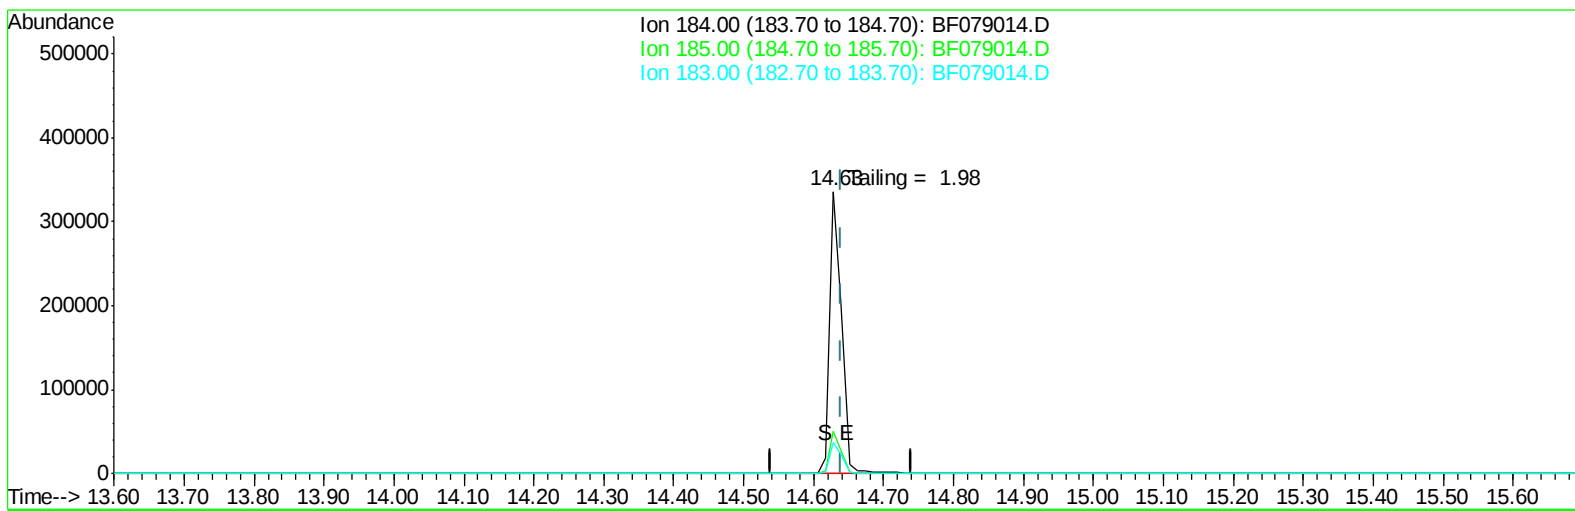

TIC: BF079014.D

(76) Benzidine

14.628min (-0.012) 0.00ng

response 395376

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.00
183.00	10.50	10.86
0.00	0.00	0.00