


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050715\
Data File : BF078990.D
Acq On : 7 May 2015 12:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 30 19:07:47 2015

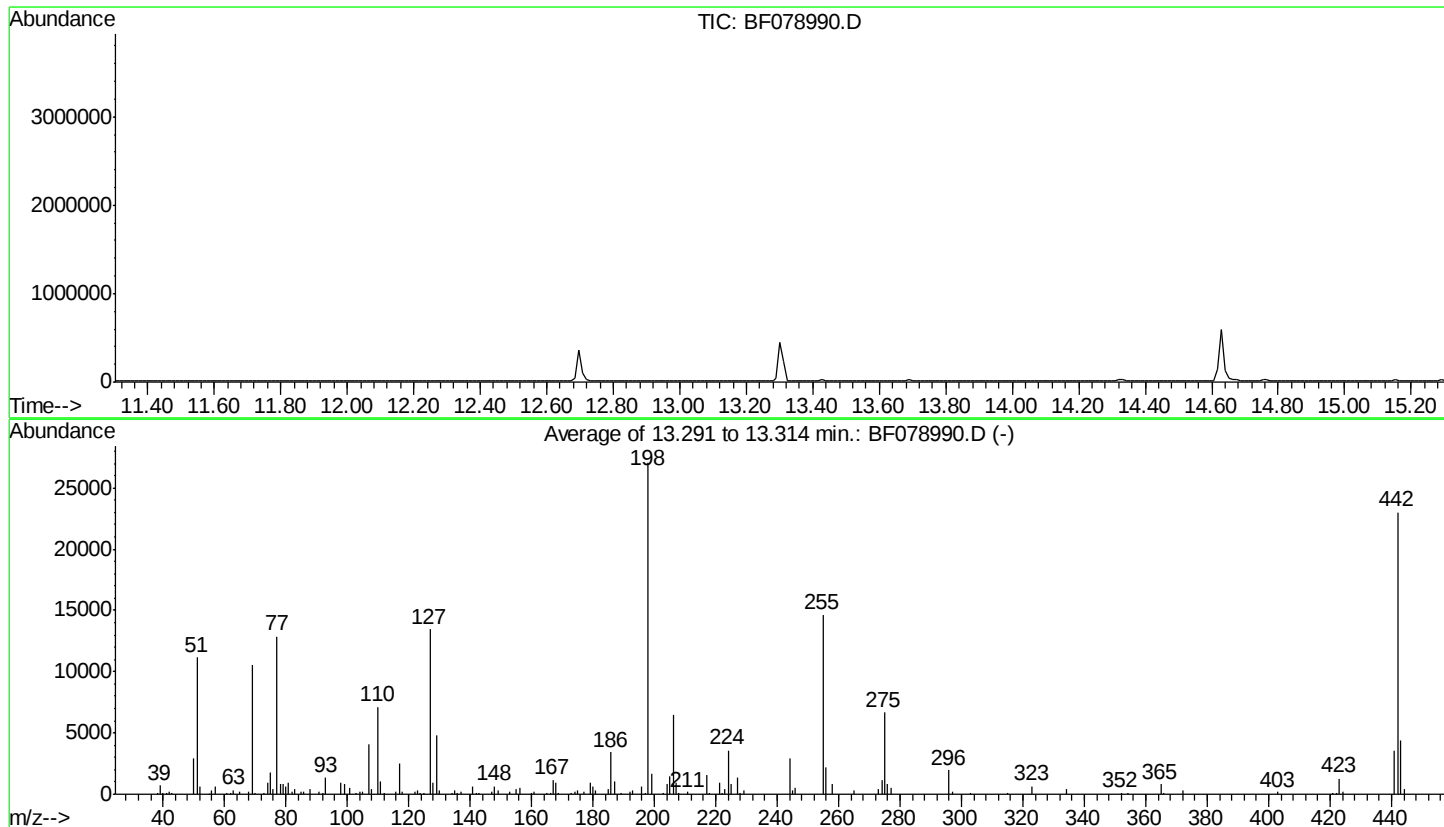

AutoFind: Scans 1059, 1060, 1061; Background Corrected with Scan 1056

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	11174	PASS
68	69	0.00	2	1.5	162	PASS
69	198	0.00	100	38.9	10533	PASS
70	69	0.00	2	0.9	100	PASS
127	198	10	80	49.7	13444	PASS
197	198	0.00	2	0.4	113	PASS
198	198	100	100	100.0	27063	PASS
199	198	5	9	6.3	1706	PASS
275	198	10	60	24.6	6658	PASS
365	198	1	100	3.1	834	PASS
441	442	0.01	24	15.4	3544	PASS
442	198	50	100	85.1	23037	PASS
443	442	15	24	19.0	4371	PASS