


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050715\
 Data File : BF079014.D
 Acq On : 8 May 2015 1:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

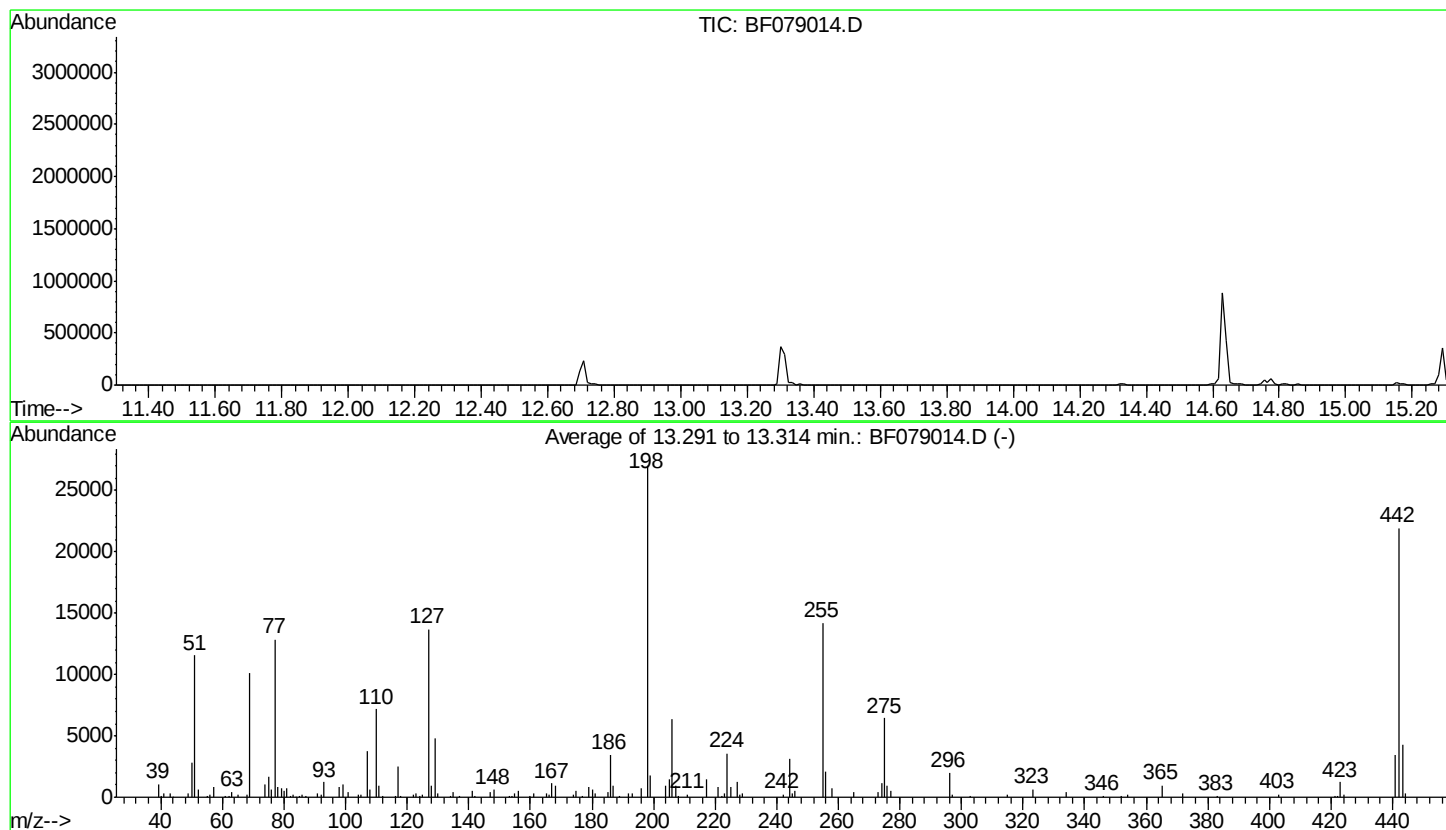

AutoFind: Scans 1059, 1060, 1061; Background Corrected with Scan 1056

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	11562	PASS
68	69	0.00	2	1.6	161	PASS
69	198	0.00	100	37.4	10122	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	13711	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27032	PASS
199	198	5	9	6.4	1735	PASS
275	198	10	60	23.8	6431	PASS
365	198	1	100	3.5	944	PASS
441	442	0.01	24	15.9	3492	PASS
442	198	50	100	81.2	21954	PASS
443	442	15	24	19.7	4328	PASS