
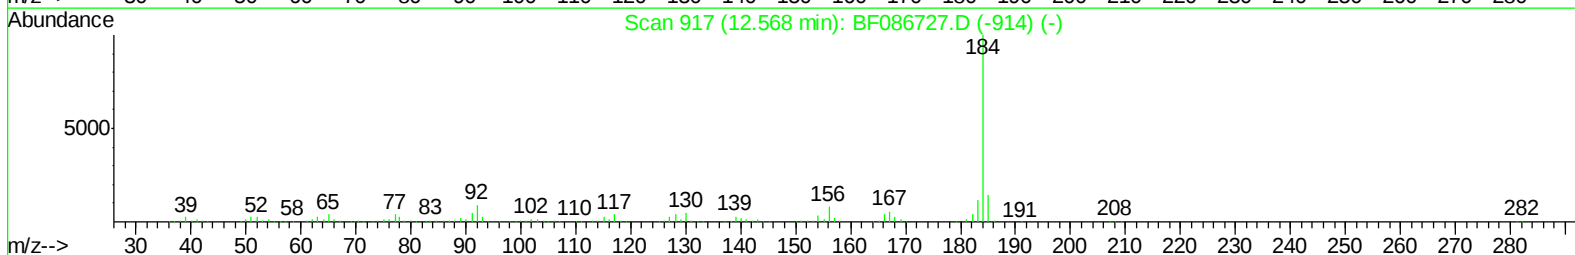
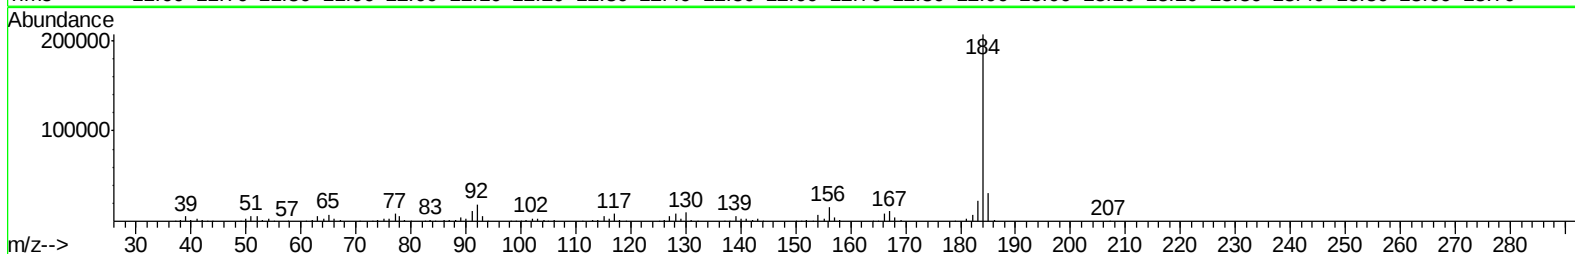


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050716\  
Data File : BF086798.D  
Acq On : 8 May 2016 2:51  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 03:55:55 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050416.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 09 03:38:20 2016  
Response via : Initial Calibration

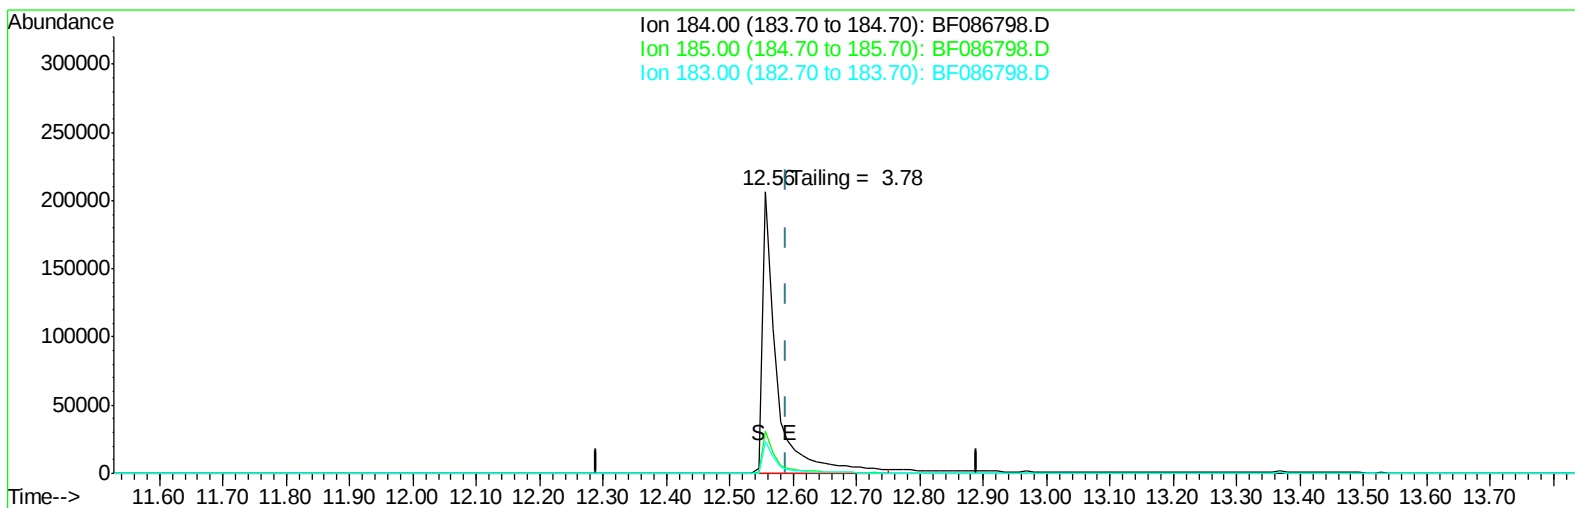

TIC: BF086798.D

(76) Benzidine




12.557min (-0.033) 0.00ng

response 338959

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.00 | 14.93 |
| 183.00 | 12.20 | 11.42 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050716\  
Data File : BF086798.D  
Acq On : 8 May 2016 2:51  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 03:55:55 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050416.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 09 03:38:20 2016  
Response via : Initial Calibration

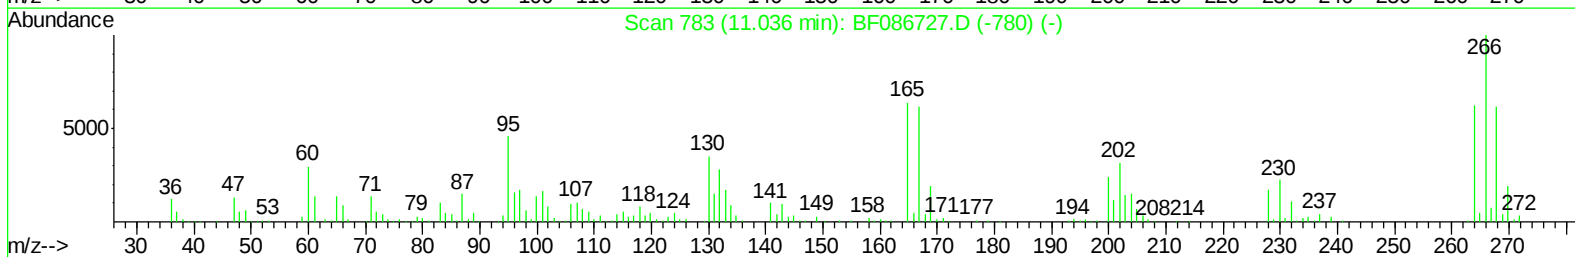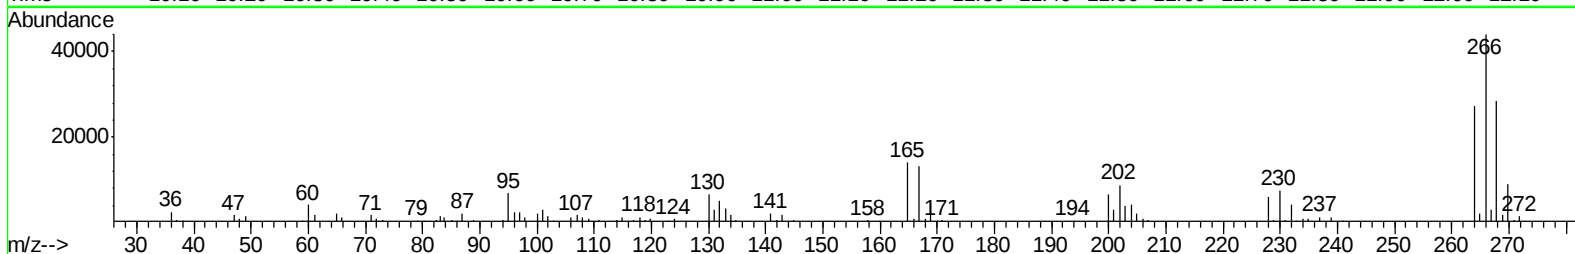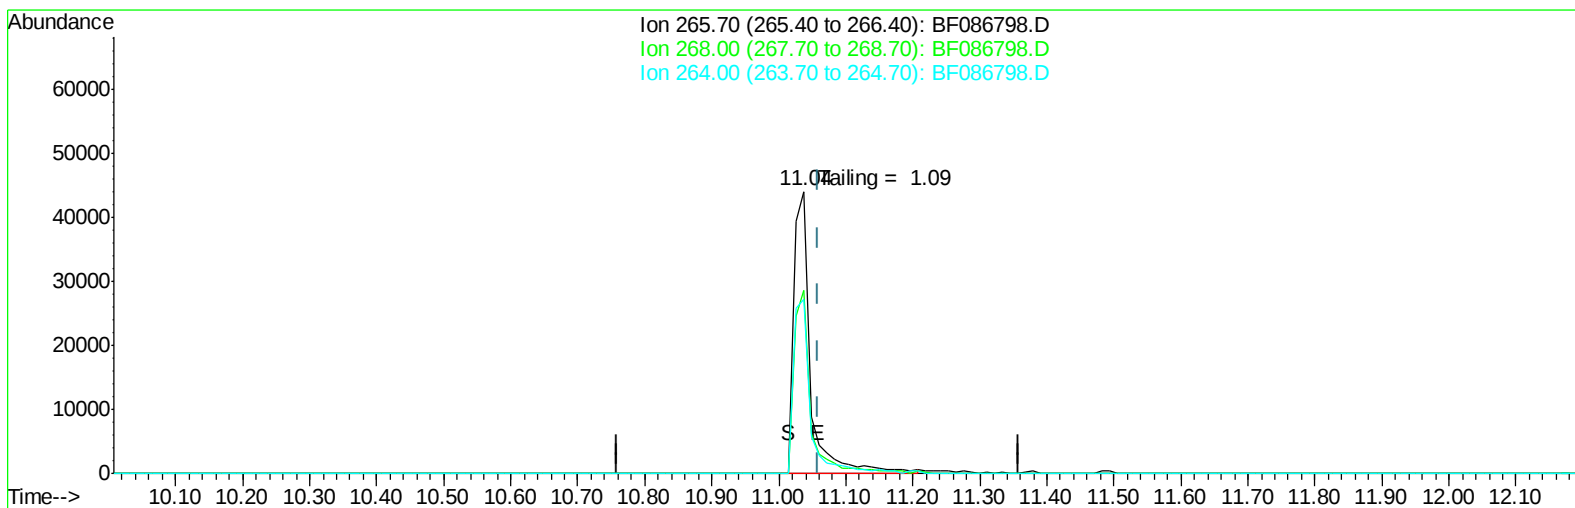

TIC: BF086798.D

(69) Pentachlorophenol (C)

11.036min (-0.023) 44314.62ng

response 76161

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 64.87 |
| 264.00 | 66.10 | 62.03 |
| 0.00   | 0.00  | 0.00  |