

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
 Data File : BF086810.D
 Acq On : 8 May 2016 8:38
 Operator : UM/SJ
 Sample : H2762-02DL2 100X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-B1COMPDL2

Manual Integrations
 APPROVED

Sohil
 5/9/2016 7:20:32 PM

Quant Time: May 09 18:13:32 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 15:12:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	162408	40.00	ng	-0.03
21) Naphthalene-d8	7.98	136	666712	40.00	ng	-0.05
38) Acenaphthene-d10	9.73	164	282297	40.00	ng	-0.05
63) Phenanthrene-d10	11.22	188	486567	40.00	ng	-0.03
75) Chrysene-d12	13.85	240	335463	40.00	ng	-0.03
86) Perylene-d12	15.22	264	297052	40.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	11753	1.20	ng	0.00
7) Phenol-d6	6.38	99	20619	1.56	ng	0.01
23) Nitrobenzene-d5	7.28	82	13170	1.02	ng	-0.03
41) 2,4,6-Tribromophenol	10.53	330	3577	1.30	ng	-0.03
44) 2-Fluorobiphenyl	9.07	172	24764	1.44	ng	-0.03
78) Terphenyl-d14	12.80	244	18283	1.10	ng	-0.05
Target Compounds						Qvalue
31) Naphthalene	8.02	128	1941375	56.99	ng	100
37) 2-Methylnaphthalene	8.70	142	486466	24.21	ng	98
45) 1,1'-Biphenyl	9.16	154	67741	2.94	ng	95
48) Acenaphthylene	9.60	152	81991	3.10	ng	# 92
51) Acenaphthene	9.77	154	216741	12.43	ng	98
57) Fluorene	10.28	166	170511	9.73	ng	98
70) Phenanthrene	11.24	178	560896	21.46	ng	100
71) Anthracene	11.29	178	156618	5.72	ng	99
74) Fluoranthene	12.42	202	164979	6.30	ng	97
77) Pyrene	12.65	202	228942	8.56	ng	99
80) Benzo(a)anthracene	13.84	228	61997m	3.27	ng	
82) Chrysene	13.87	228	56817m	2.81	ng	
89) Benzo(a)pyrene	15.17	252	42782	2.60	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
Data File : BF086810.D
Acq On : 8 May 2016 8:38
Operator : UM/SJ
Sample : H2762-02DL2 100X
Misc :
ALS Vial : 78 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
TEC-B1COMPDL2

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

Quant Time: May 09 18:13:32 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 15:12:53 2016
Response via : Initial Calibration

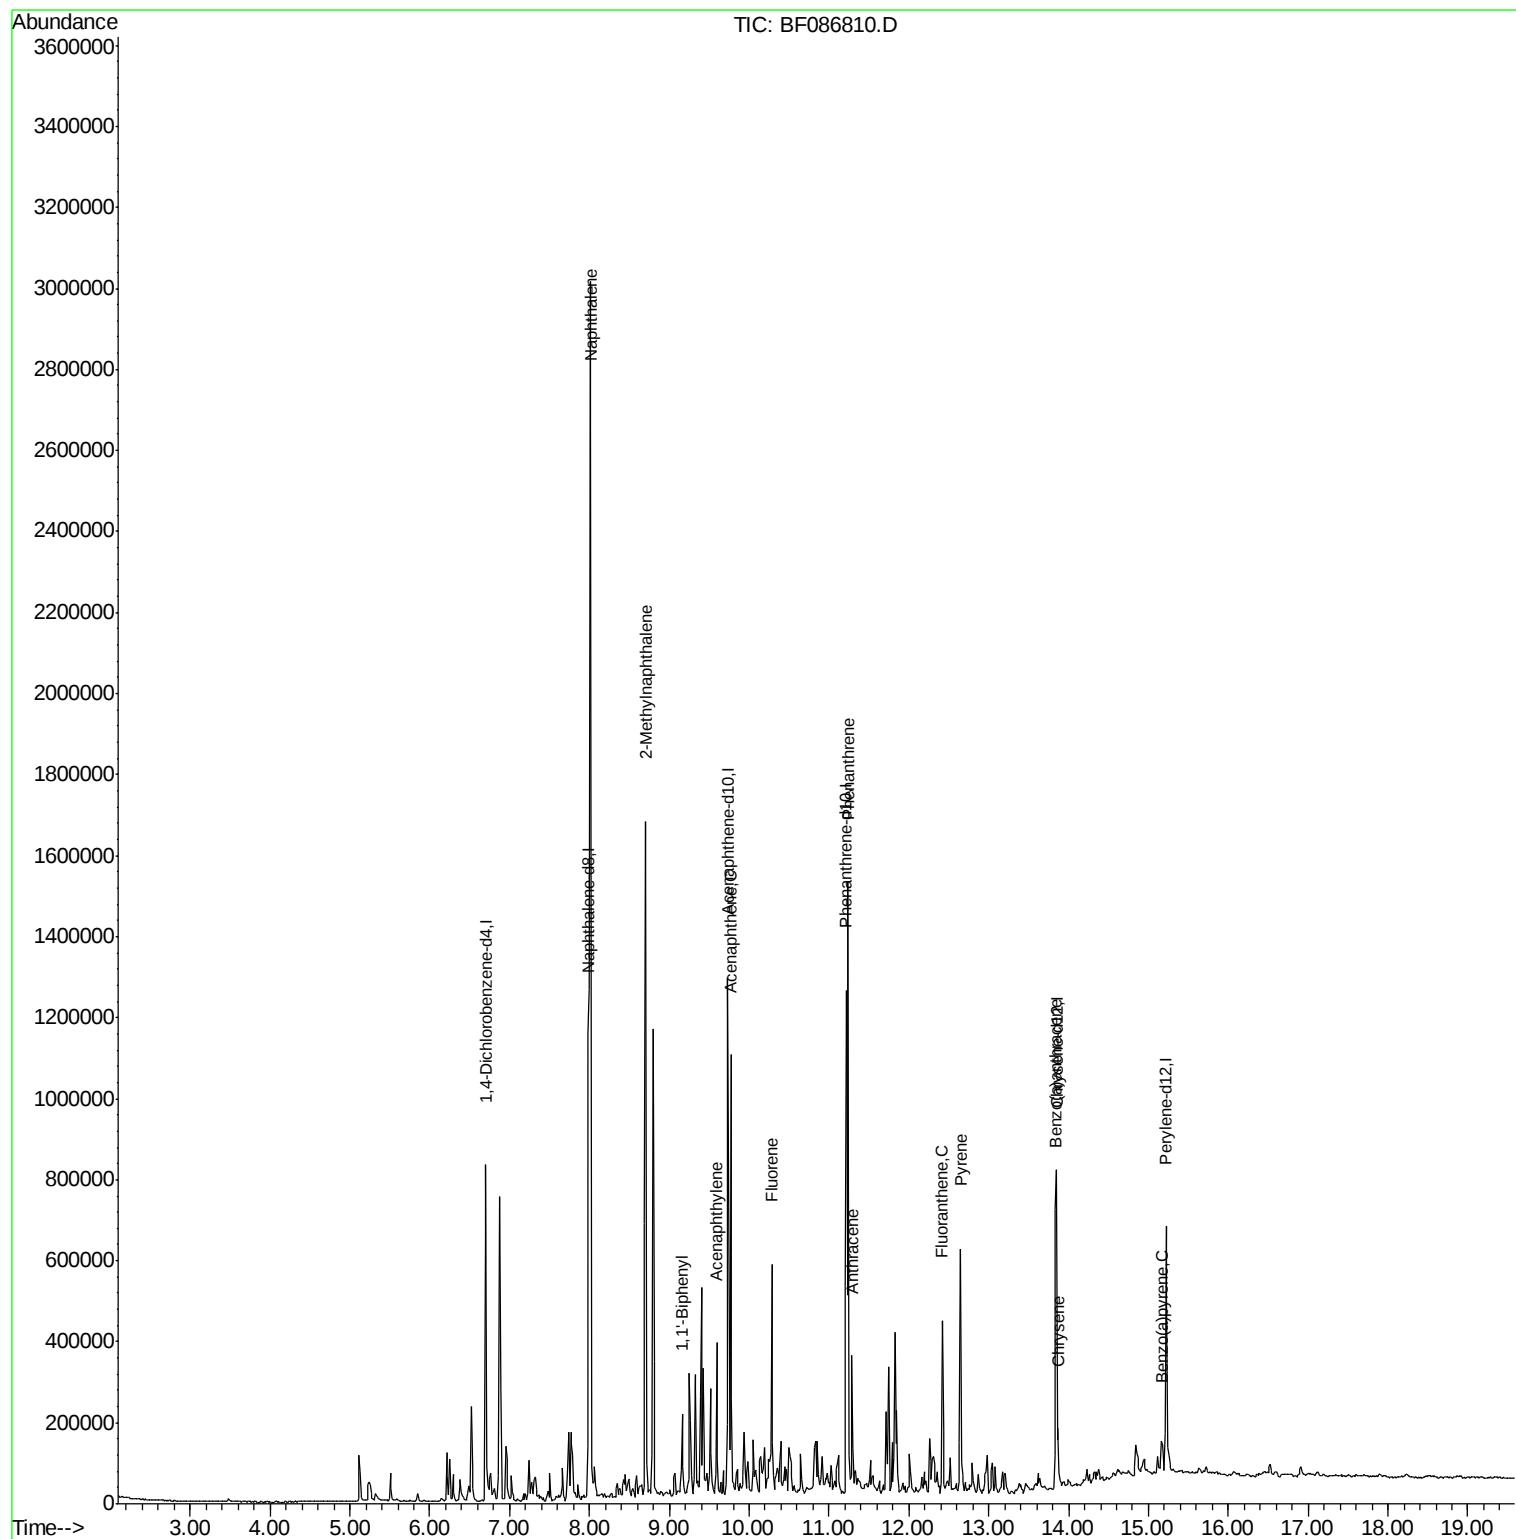

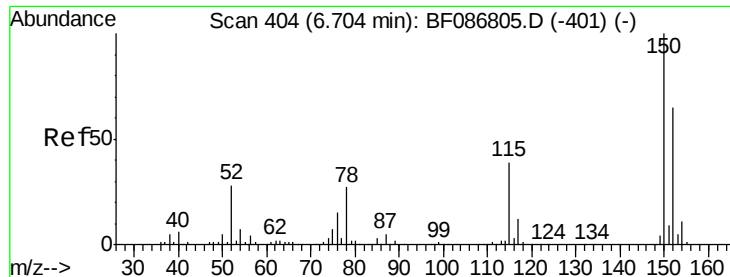

#1


1,4-Dichlorobenzene-d4
Concen: 40.00 ng
RT: 6.70 min Scan# 404
Delta R.T. -0.03 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Instrument :
BNA_F
ClientSampleId :
TEC-B1COMPDL2




Tgt Ion	Ratio	Lower	Upper
152	100		
150	153.2	125.8	188.6
115	57.4	51.5	77.3

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

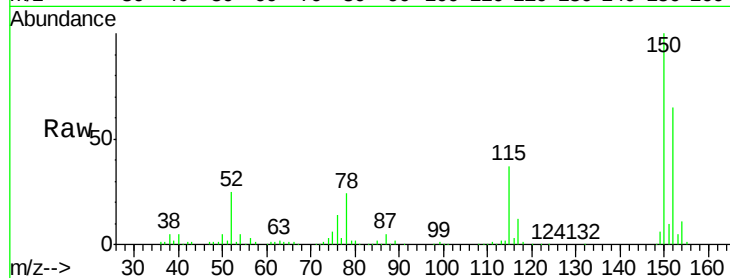


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

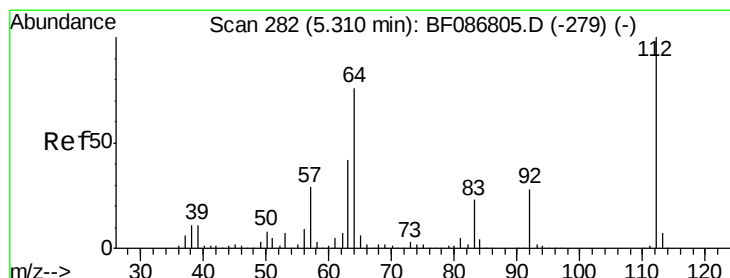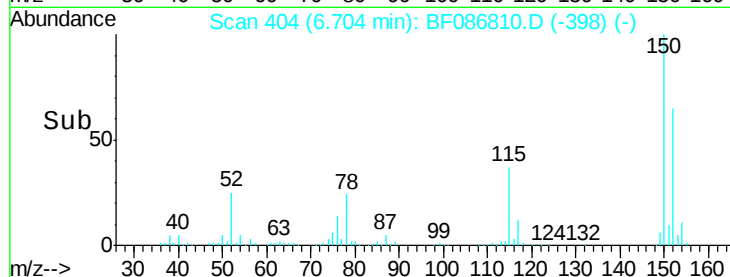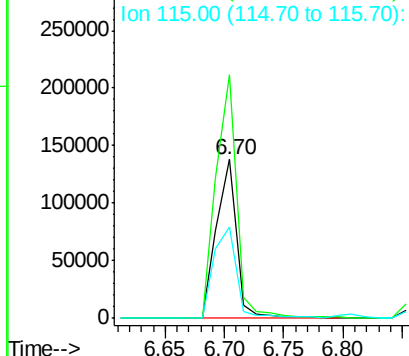



#5


2-Fluorophenol
Concen: 1.20 ng
RT: 5.32 min Scan# 283
Delta R.T. 0.00 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.4	52.1	78.1
63	44.4	25.7	38.5

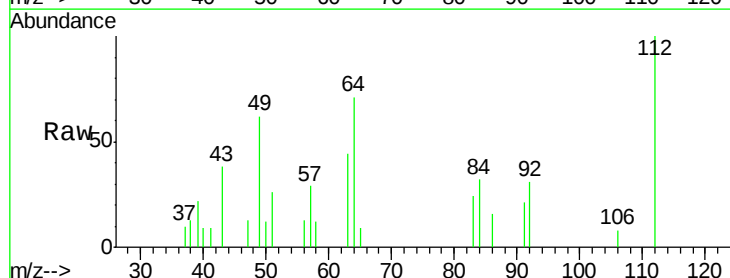

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

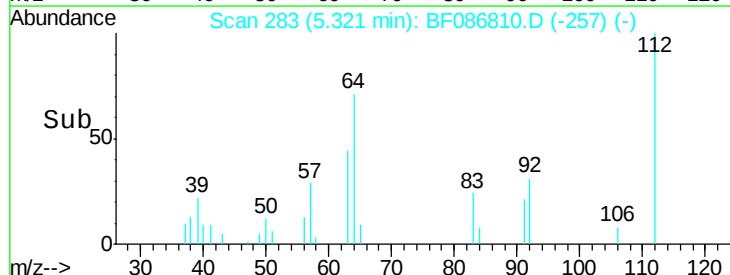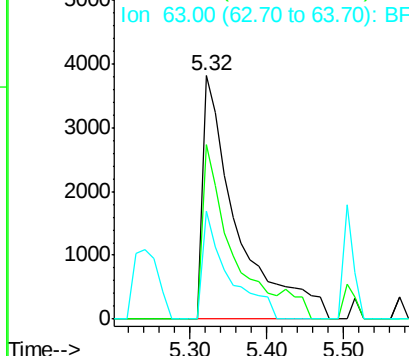



#7

Phenol-d6

Concen: 1.56 ng

RT: 6.38 min Scan# 376

Delta R.T. 0.01 min

Lab File: BF086810.D


Acq: 8 May 2016 8:38

Instrument :

BNA_F

ClientSampleId :




TEC-B1COMPDL2



Tgt Ion	Ratio	Lower	Upper
99	100		
42	29.6	13.6	20.4#
71	32.6	24.6	36.8

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

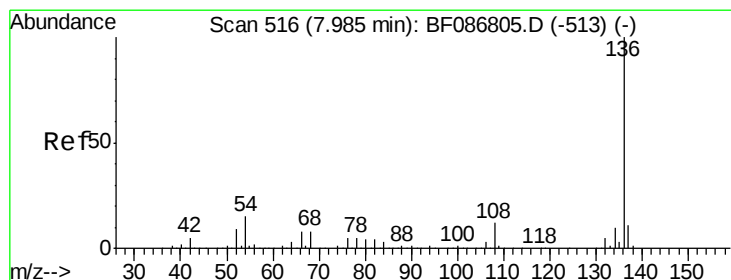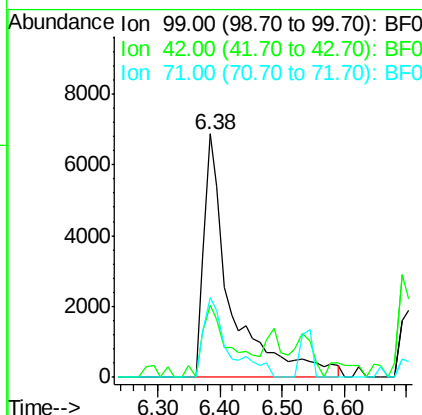

#21

Naphthalene-d8

Concen: 40.00 ng




RT: 7.98 min Scan# 516


Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.8	13.2
54	15.4	5.0	7.4#
68	8.0	4.4	6.6#

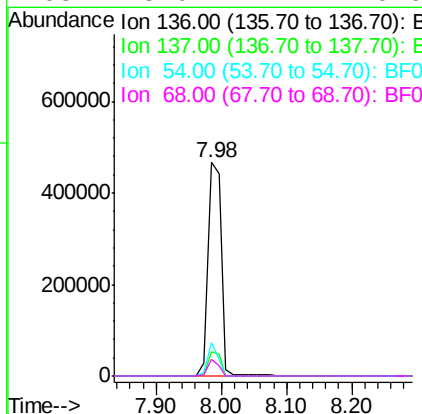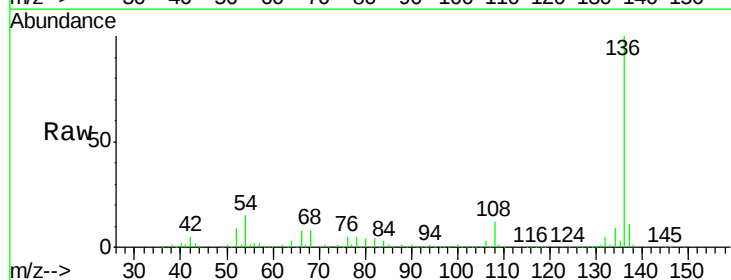




#23
 Nitrobenzene-d5
 Concen: 1.02 ng
 RT: 7.28 min Scan# 454
 Delta R.T. -0.03 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Instrument :
 BNA_F
 ClientSampleId :
 TEC-B1COMPDL2

Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.1	40.6	61.0#
54	62.3	38.1	57.1#

Manual Integrations
 APPROVED

Sohil
 5/9/2016 7:20:32 PM



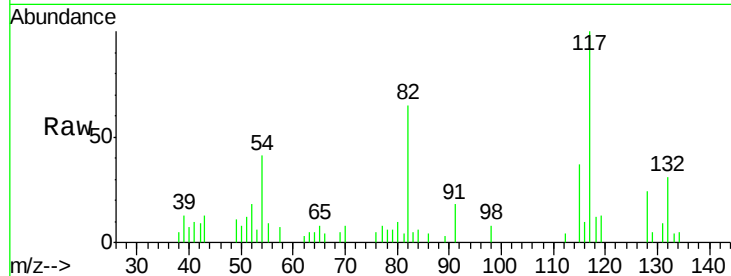


Abundance

Ion 82.00 (81.70 to 82.70): BF0


Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

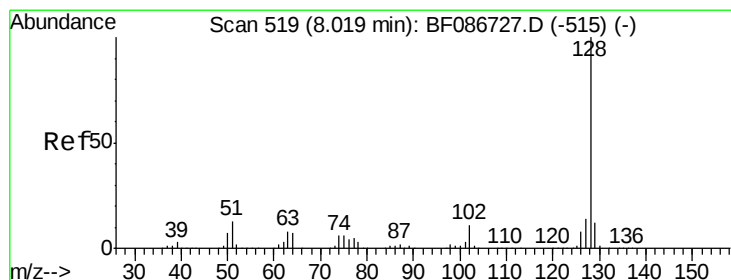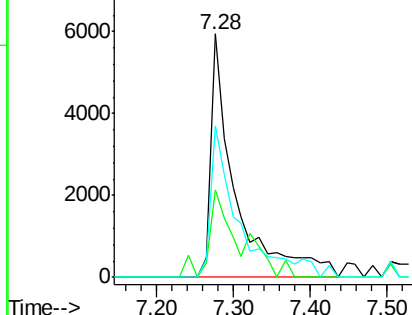

#31
 Naphthalene
 Concen: 56.99 ng
 RT: 8.02 min Scan# 519
 Delta R.T. -0.02 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.6	13.0
127	13.5	10.8	16.2






Abundance

Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

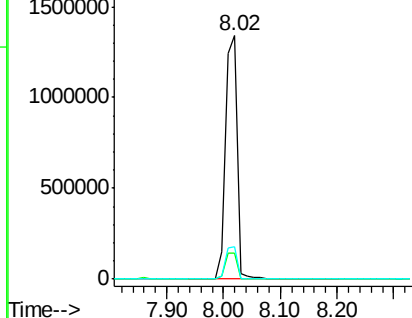







#37
2-Methylnaphthalene
Concen: 24.21 ng
RT: 8.70 min Scan# 579
Delta R.T. -0.03 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Instrument :
BNA_F
ClientSampleId :
TEC-B1COMPDL2

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	486466		
141	90.2	71.0	106.6	
115	34.9	26.6	39.8	




Manual Integrations
APPROVED


Sohil
5/9/2016 7:20:32 PM

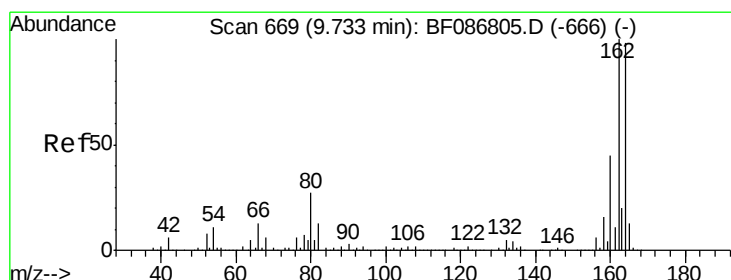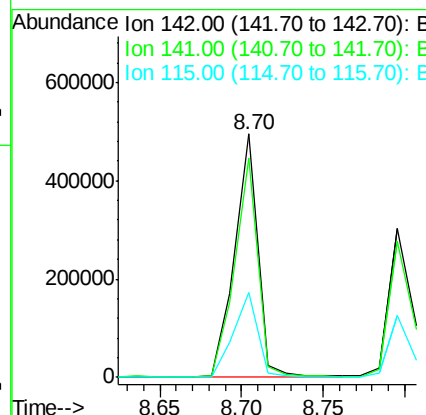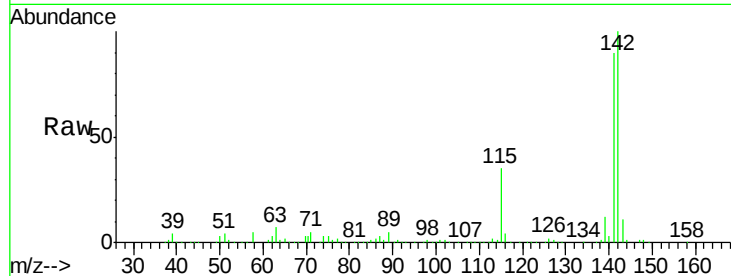

#38
Acenaphthene-d10
Concen: 40.00 ng
RT: 9.73 min Scan# 669
Delta R.T. -0.05 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Resp	Lower	Upper
164	100	282297		
162	102.8	82.8	124.2	
160	46.8	36.9	55.3	

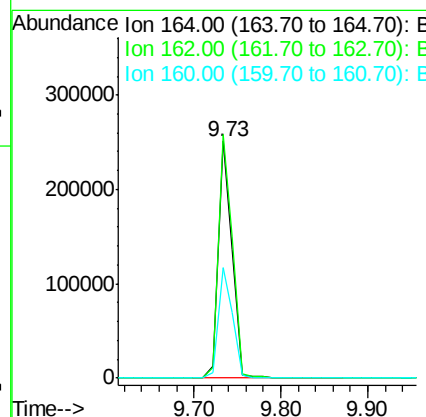

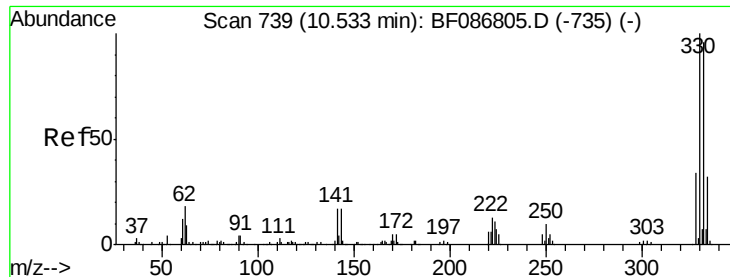





#41
 2,4,6-Tribromophenol
 Concen: 1.30 ng
 RT: 10.53 min Scan# 739
 Delta R.T. -0.03 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Instrument :
 BNA_F
 ClientSampleId :
 TEC-B1COMPDL2

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	3577		
332	88.3	79.0	118.4	
141	68.1	31.2	46.8	




Manual Integrations
 APPROVED


Sohil
 5/9/2016 7:20:32 PM

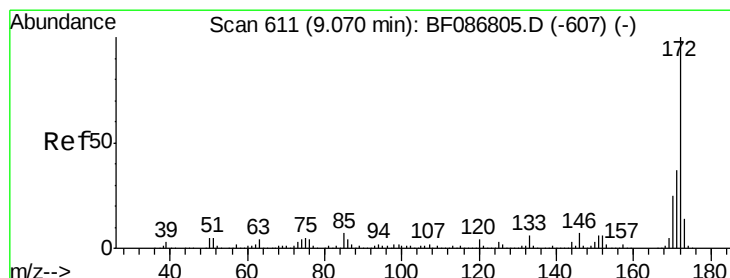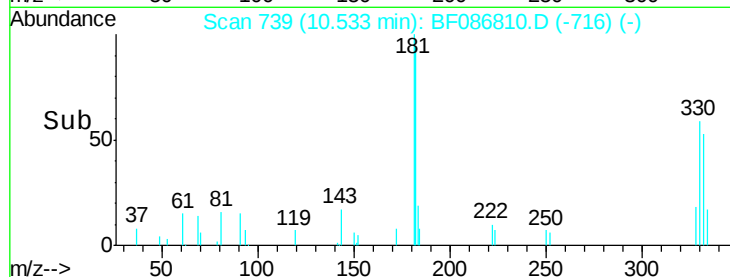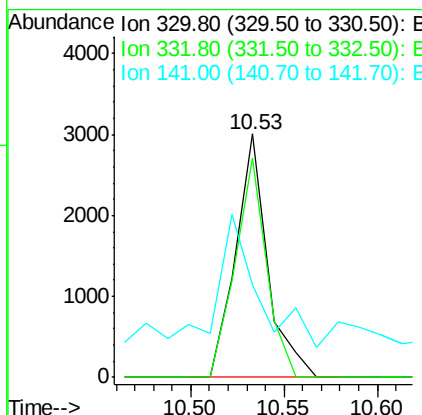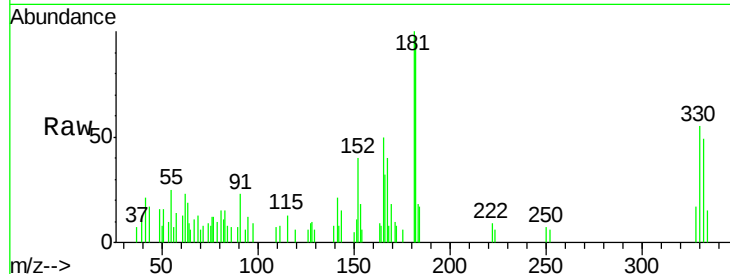

#44
 2-Fluorobiphenyl
 Concen: 1.44 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.03 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	24764		
171	33.6	29.0	43.6	
170	23.6	19.8	29.8	

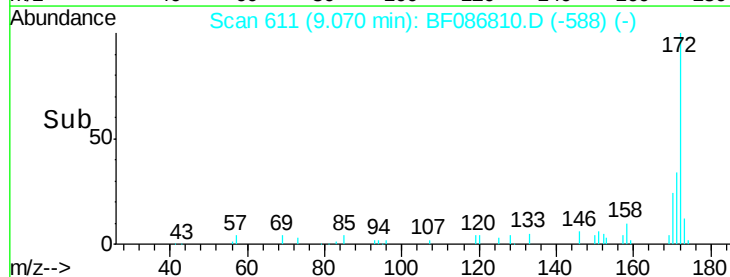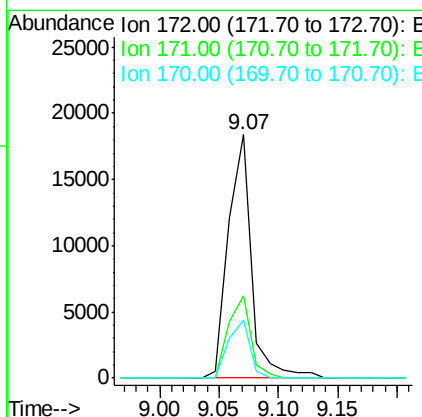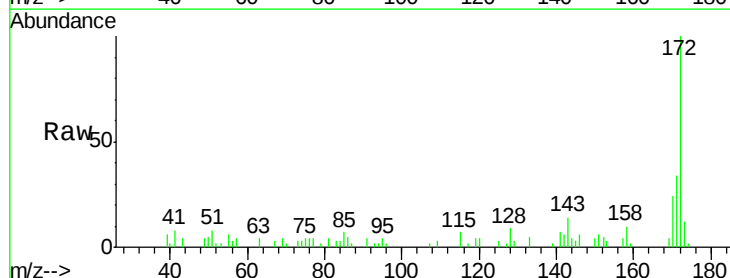



#45

1,1'-Biphenyl

Concen: 2.94 ng

RT: 9.16 min Scan# 619

Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Instrument :

BNA_F





ClientSampleId :

TEC-B1COMPDL2

Tgt Ion:	154	Resp:	67741
Ion Ratio	Lower	Upper	
154	100		
153	39.1	20.3	60.3
76	15.7	0.0	30.2

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

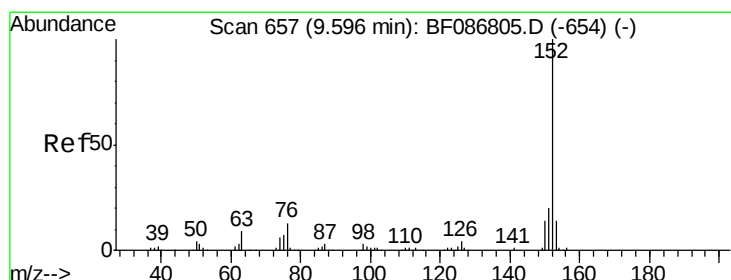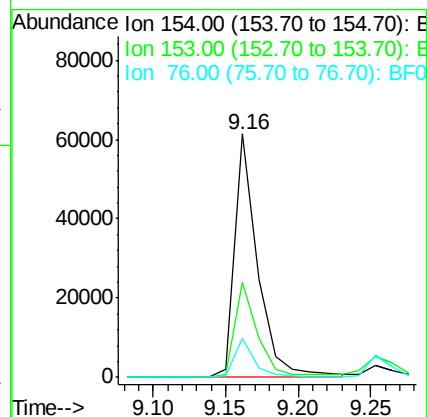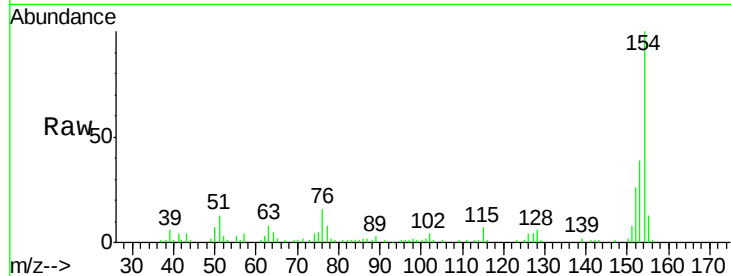

#48

Acenaphthylene

Concen: 3.10 ng




RT: 9.60 min Scan# 657


Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Tgt Ion:	152	Resp:	81991
Ion Ratio	Lower	Upper	
152	100		
151	20.0	16.8	25.2
153	20.0	10.9	16.3#

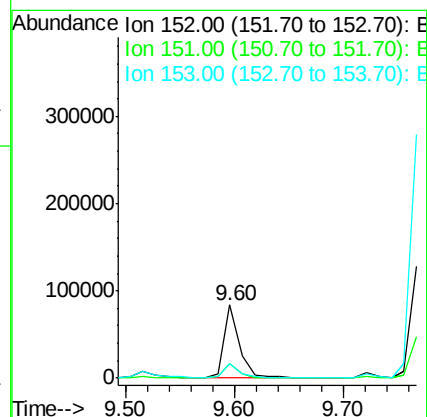



#51

Acenaphthene

Concen: 12.43 ng

RT: 9.77 min Scan# 672

Delta R.T. -0.05 min

Lab File: BF086810.D


Acq: 8 May 2016 8:38

Instrument :

BNA_F

ClientSampleId :




TEC-B1COMPDL2

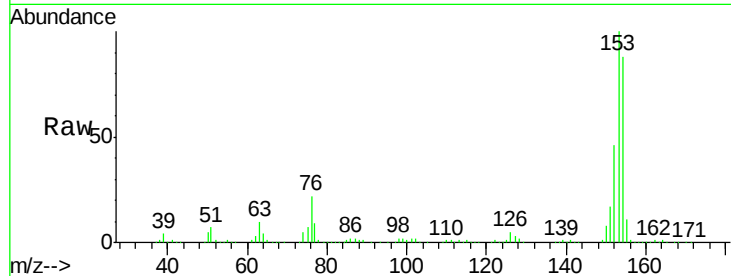

Tgt Ion:	154	Resp:	216741
Ion Ratio	Lower	Upper	
154	100		
153	113.5	89.8	134.6
152	52.1	43.4	65.0

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

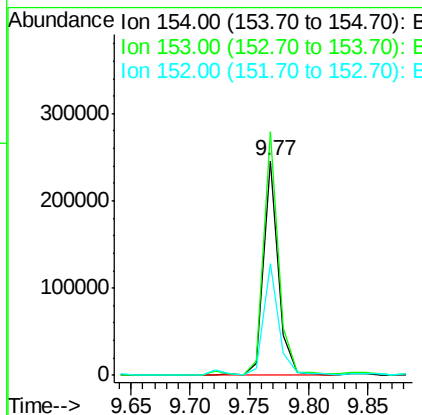

#57

Fluorene

Concen: 9.73 ng




RT: 10.28 min Scan# 717


Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Tgt Ion:	166	Resp:	170511
Ion Ratio	Lower	Upper	
166	100		
165	101.2	79.0	118.6
167	14.1	10.6	15.8

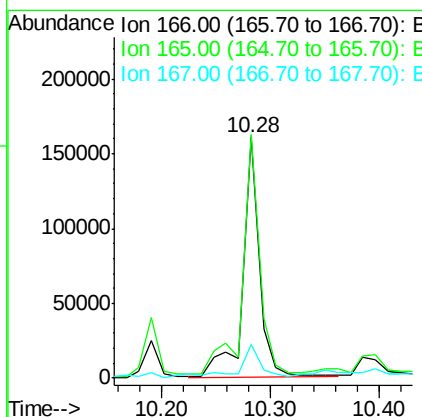



#63

Phenanthrene-d10

Concen: 40.00 ng

RT: 11.22 min Scan# 799

Delta R.T. -0.03 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Instrument :

BNA_F

ClientSampleId :

TEC-B1COMPL2

Tgt Ion:188 Resp: 486567

Ion Ratio Lower Upper





188 100

94 8.2 6.8 10.2

80 8.9 7.1 10.7

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

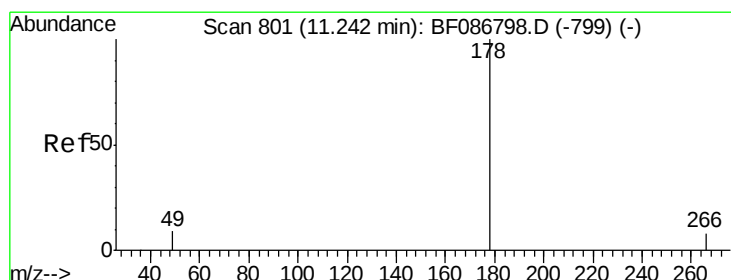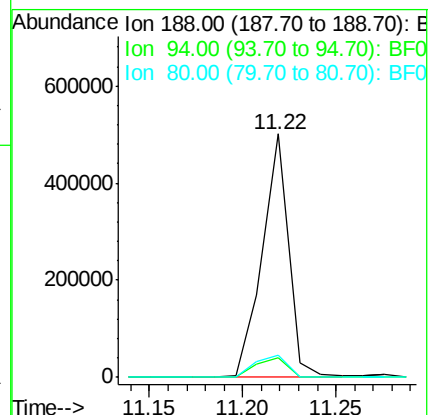

#70

Phenanthrene

Concen: 21.46 ng

RT: 11.24 min Scan# 801

Delta R.T. -0.03 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38




Tgt Ion:178 Resp: 560896


Ion Ratio Lower Upper

178 100

176 19.8 16.0 24.0

179 15.6 12.6 18.8

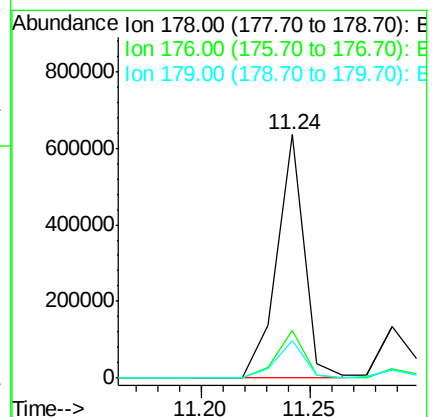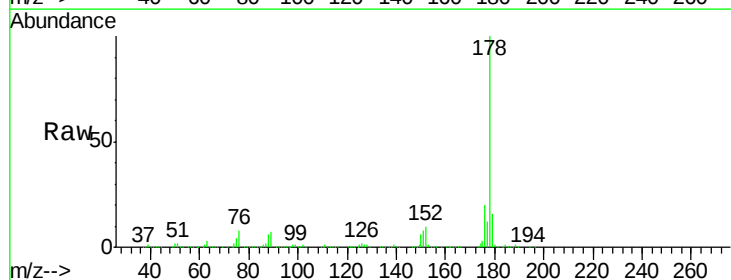



#71

Anthracene

Concen: 5.72 ng

RT: 11.29 min Scan# 805

Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Instrument :

BNA_F


ClientSampleId :

TEC-B1COMPDL2




Tgt Ion:	178	Resp:	156618
Ion Ratio	Lower	Upper	
178	100		
176	18.7	15.6	23.4
179	16.1	12.7	19.1

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

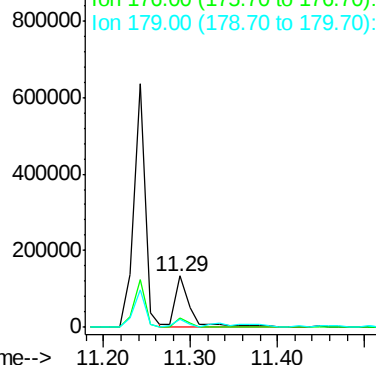

#74

Fluoranthene

Concen: 6.30 ng


RT: 12.42 min Scan# 904

Delta R.T. -0.05 min



Lab File: BF086810.D


Acq: 8 May 2016 8:38

Tgt Ion:	202	Resp:	164979
Ion Ratio	Lower	Upper	
202	100		
101	14.1	0.0	35.4
203	17.2	0.0	38.1



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

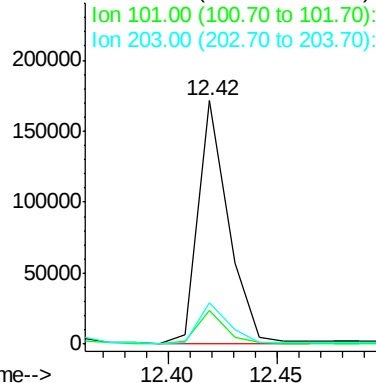



#75

Chrysene-d12

Concen: 40.00 ng

RT: 13.85 min Scan# 1029

Delta R.T. -0.03 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Instrument :

BNA_F





ClientSampleId :

TEC-B1COMPDL2

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	335463		
120	8.6	11.2	16.8#	
236	26.1	21.2	31.8	

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

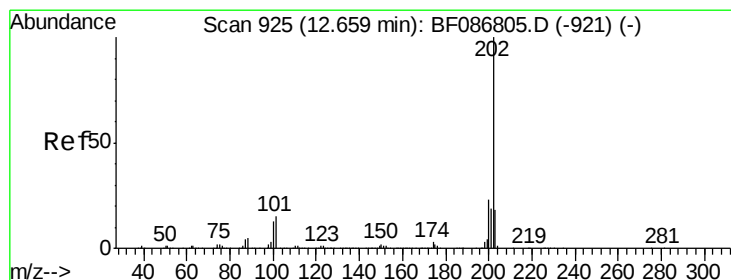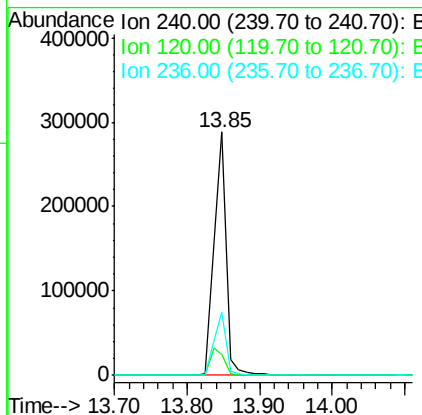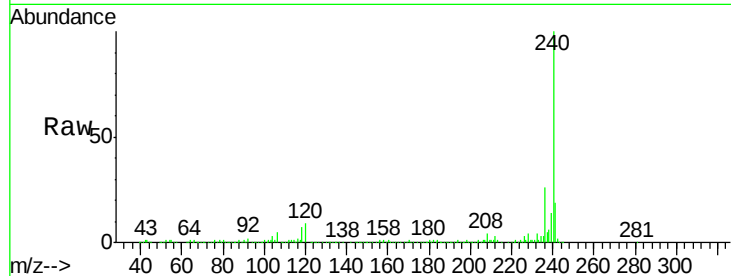

#77

Pyrene

Concen: 8.56 ng




RT: 12.65 min Scan# 924


Delta R.T. -0.05 min

Lab File: BF086810.D

Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	228942		
200	21.8	17.7	26.5	
203	17.5	14.2	21.4	

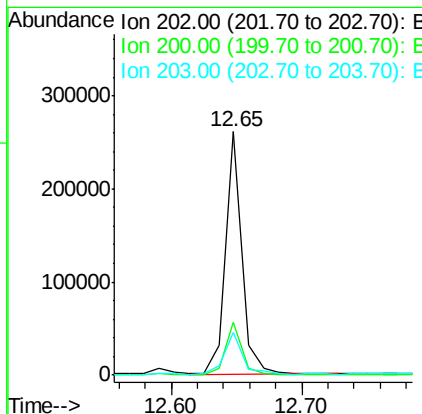







#78
 Terphenyl-d14
 Concen: 1.10 ng
 RT: 12.80 min Scan# 937
 Delta R.T. -0.05 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Instrument :
 BNA_F
 ClientSampleId :
 TEC-B1COMPDL2

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.6	6.2	9.2
122	10.3	12.0	18.0#




Manual Integrations
 APPROVED


Sohil
 5/9/2016 7:20:32 PM

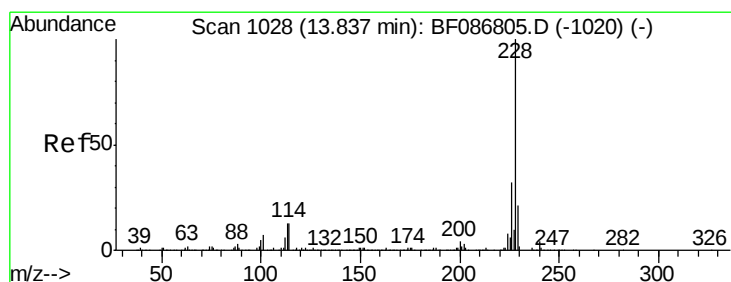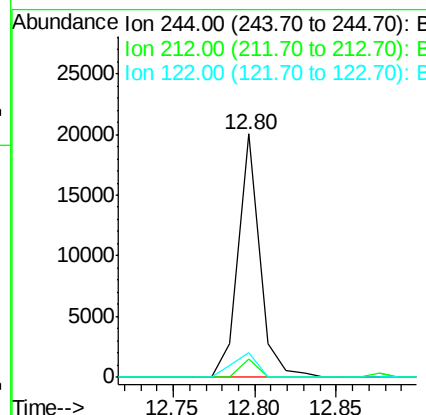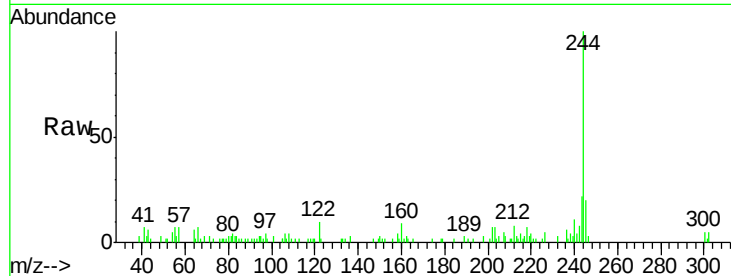

#80
 Benzo(a)anthracene
 Concen: 3.27 ng m
 RT: 13.84 min Scan# 1028
 Delta R.T. -0.03 min
 Lab File: BF086810.D
 Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Lower	Upper
228	100		
226	47.7	22.5	33.7#
229	20.2	16.6	25.0

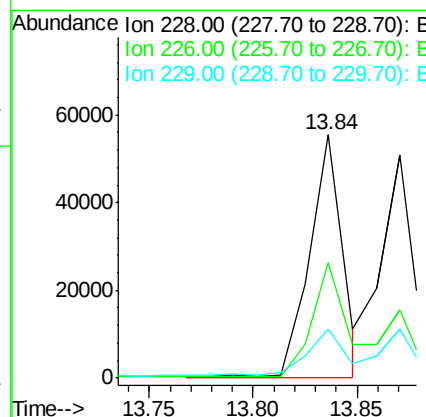

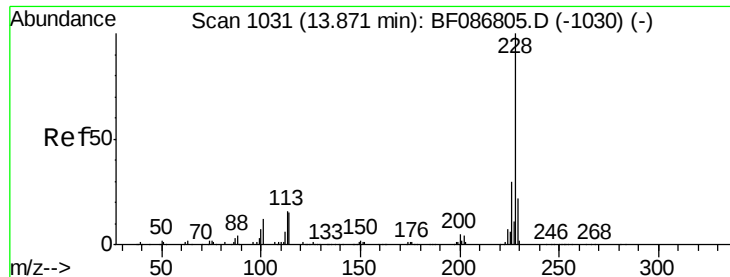


#82
Chrysene
Concen: 2.81 ng m
RT: 13.87 min Scan# 1031
Delta R.T. -0.05 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Instrument :
BNA_F
ClientSampleId :
TEC-B1COMPDL2




Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.5	24.4	36.6
229	21.7	15.8	23.8

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

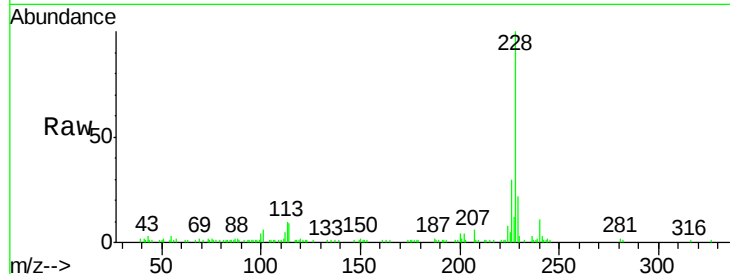




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

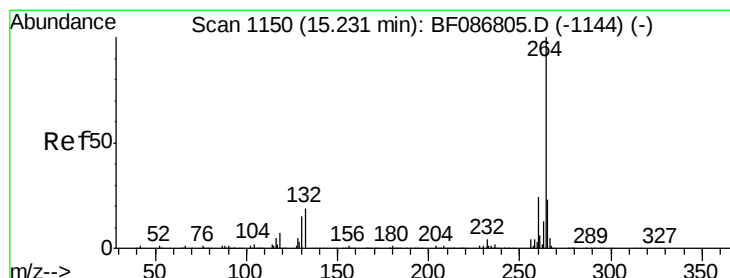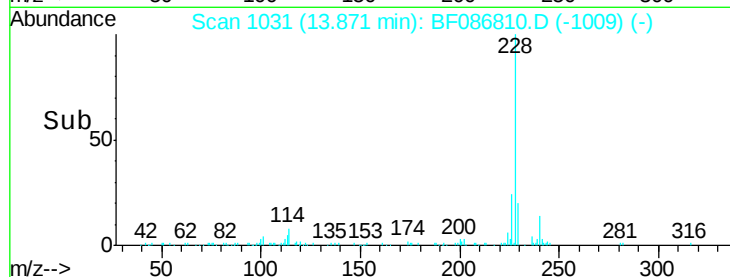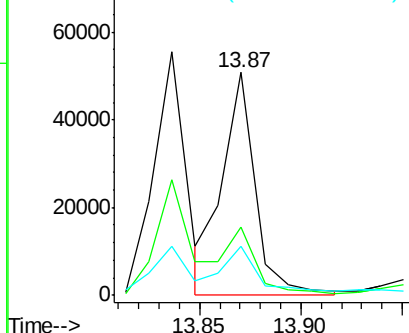


#86
Perylene-d12
Concen: 40.00 ng
RT: 15.22 min Scan# 1149
Delta R.T. -0.05 min
Lab File: BF086810.D
Acq: 8 May 2016 8:38

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.5	29.3
265	21.9	17.3	25.9

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

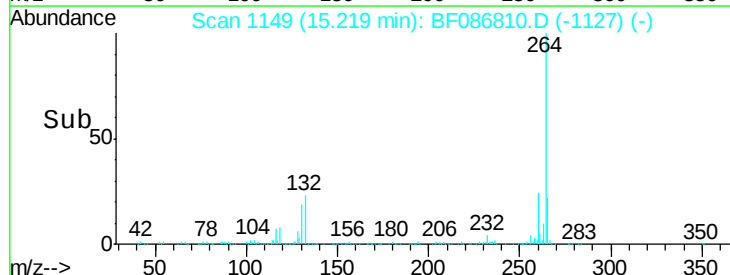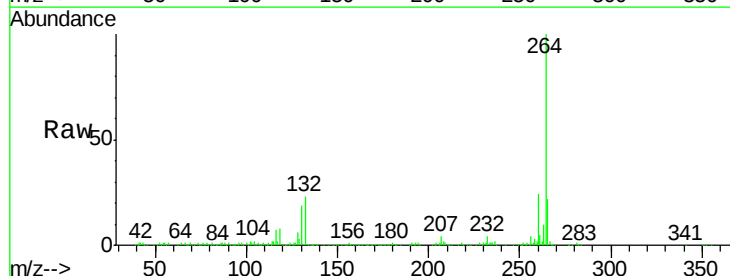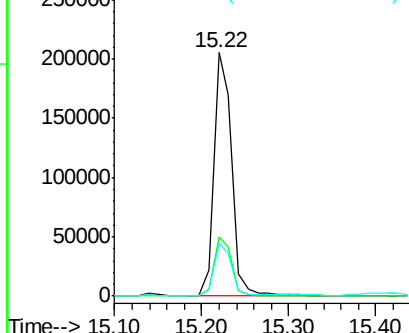



#89

Benzo(a)pyrene

Concen: 2.60 ng

RT: 15.17 min Scan# 1145

Delta R.T. -0.05 min

Lab File: BF086810.D


Acq: 8 May 2016 8:38

Instrument :

BNA_F

ClientSampleId :

TEC-B1COMPDL2



Tgt Ion:	252	Resp:	42782
Ion Ratio	Lower	Upper	
252	100		
253	24.2	17.2	25.8
125	10.6	9.0	13.6

Manual Integrations
APPROVED

Sohil
5/9/2016 7:20:32 PM

