

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
 Data File : BF086814.D
 Acq On : 8 May 2016 10:34
 Operator : UM/SJ
 Sample : H2720-13 5X
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.853	241	242	250	rBV	34184	69847	4.67%	0.424%
2	5.299	279	281	290	rBV	1058935	1221860	81.76%	7.410%
3	5.687	312	315	317	rBV3	8462	15908	1.06%	0.096%
4	6.362	371	374	382	rBV	1164589	1344169	89.94%	8.152%
5	6.476	382	384	395	rVB	1320747	1400758	93.73%	8.496%
6	6.704	401	404	406	rBV	1106450	1274742	85.30%	7.731%
7	6.853	415	417	420	rBV	1012880	1002252	67.06%	6.079%
8	6.967	425	427	432	rVB4	6863	18154	1.21%	0.110%
9	7.265	451	453	456	rBV	465920	723778	48.43%	4.390%
10	7.985	514	516	519	rBV	1404899	1494475	100.00%	9.064%
11	9.059	608	610	613	rBV	845038	1193526	79.86%	7.239%
12	9.150	616	618	620	rVB	17363	20225	1.35%	0.123%
13	9.470	643	646	648	rBV	102861	115907	7.76%	0.703%
14	9.676	662	664	667	rBV	36305	30582	2.05%	0.185%
15	9.733	667	669	672	rBV2	1302264	1429036	95.62%	8.667%
16	10.179	706	708	709	rVV	31515	32896	2.20%	0.200%
17	10.259	713	715	720	rVB4	12768	21752	1.46%	0.132%
18	10.396	724	727	730	rBV	17099	29539	1.98%	0.179%
19	10.522	736	738	745	rBV	649637	675626	45.21%	4.098%
20	10.648	747	749	755	rVB	46546	61206	4.10%	0.371%
21	11.093	786	788	789	rBV	21629	18751	1.25%	0.114%
22	11.219	797	799	801	rBV	1178850	1221238	81.72%	7.407%
23	11.276	803	804	808	rVB	15850	18634	1.25%	0.113%
24	11.756	844	846	849	rBV	16904	21744	1.45%	0.132%
25	12.625	920	922	928	rBV2	18074	41281	2.76%	0.250%
26	12.796	934	937	939	rBV	929385	825323	55.22%	5.006%
27	13.334	982	984	986	rBV	16958	16053	1.07%	0.097%
28	13.711	1015	1017	1022	rBV	44565	94098	6.30%	0.571%
29	13.848	1026	1029	1031	rBV	863522	1023240	68.47%	6.206%
30	14.328	1068	1071	1072	rBV3	18063	31151	2.08%	0.189%
31	14.614	1094	1096	1097	rBV2	21701	30413	2.04%	0.184%
32	14.842	1114	1116	1119	rBV2	21800	33103	2.22%	0.201%
33	15.220	1147	1149	1152	rBV	611087	898316	60.11%	5.448%
34	15.631	1183	1185	1187	rBV	23105	38647	2.59%	0.234%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
Data File : BF086814.D
Acq On : 8 May 2016 10:34
Operator : UM/SJ
Sample : H2720-13 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS7

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 16488230

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
Data File : BF086814.D
Acq On : 8 May 2016 10:34
Operator : UM/SJ
Sample : H2720-13 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS7

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

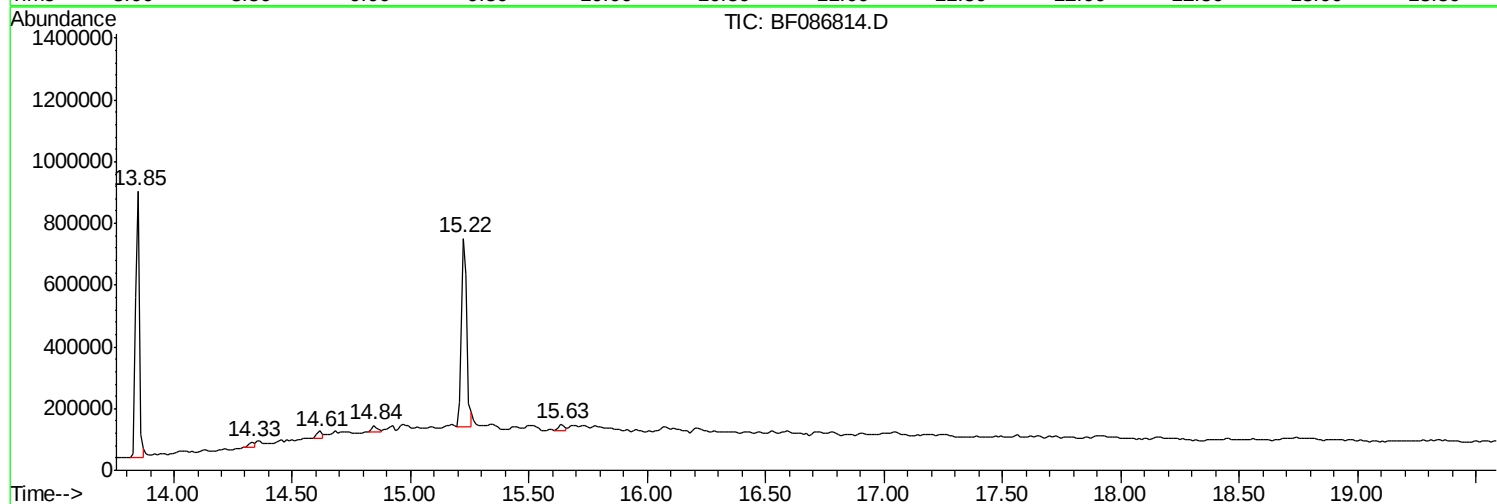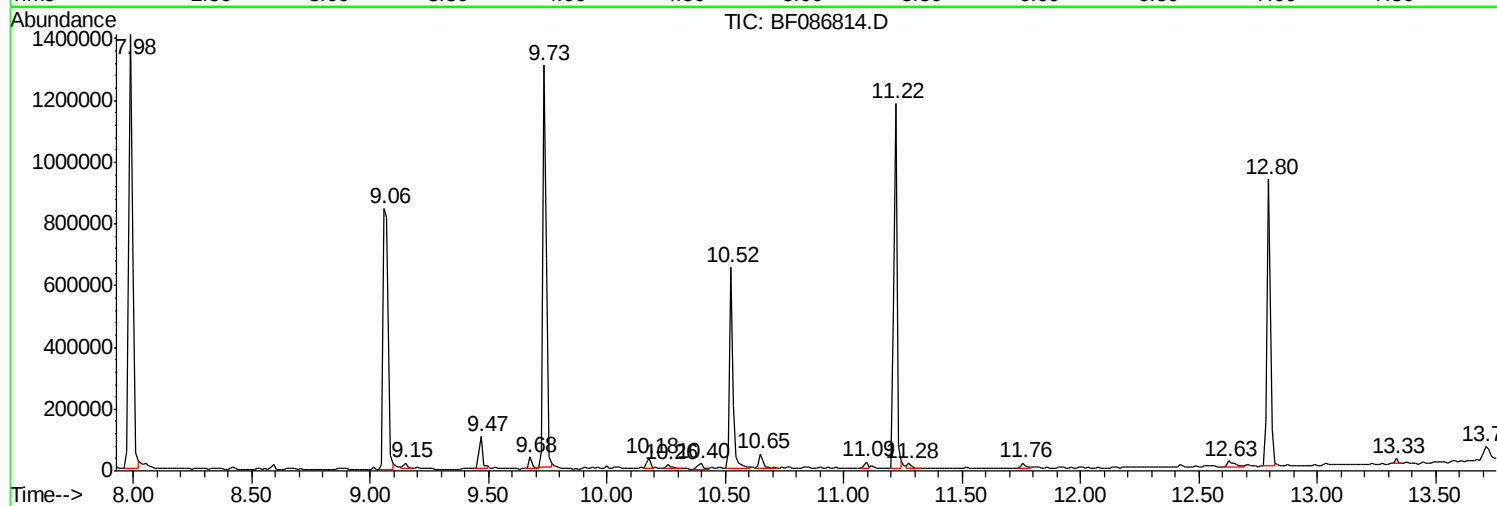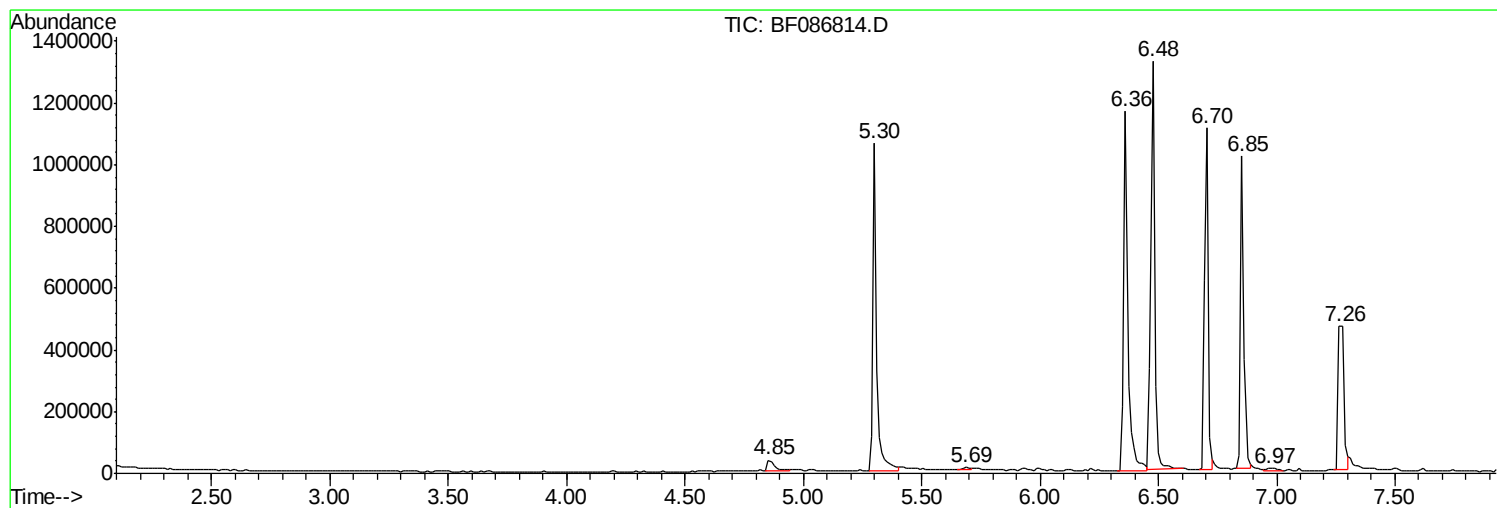

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
Data File : BF086814.D
Acq On : 8 May 2016 10:34
Operator : UM/SJ
Sample : H2720-13 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS7









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.48 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	43.95 ng	1400760	1,4-Dichlorobenzene-d4	6.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	22
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		5-Aminoindole	132	C8H8N2	005192-03-0	9

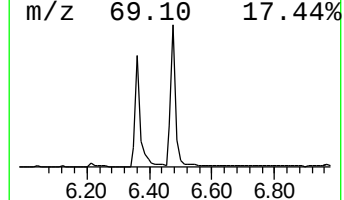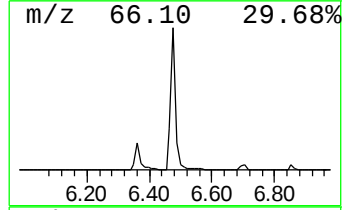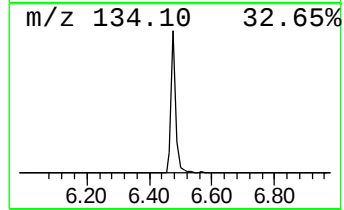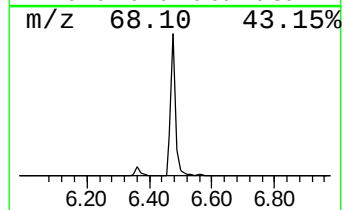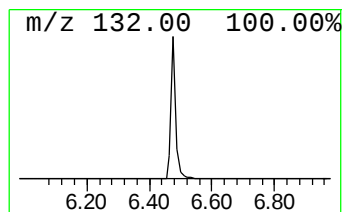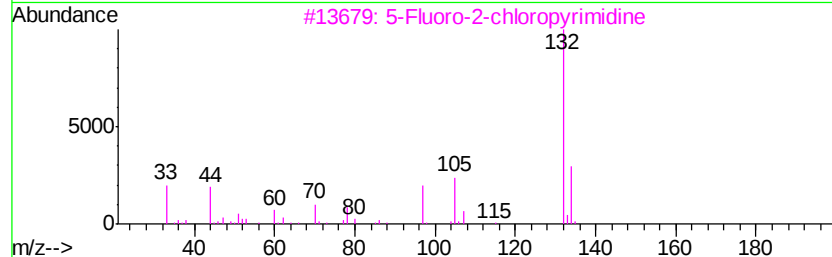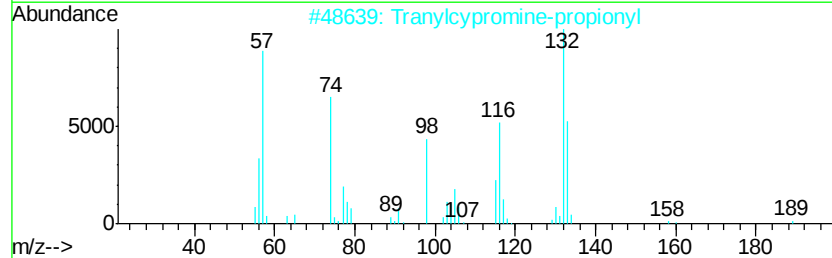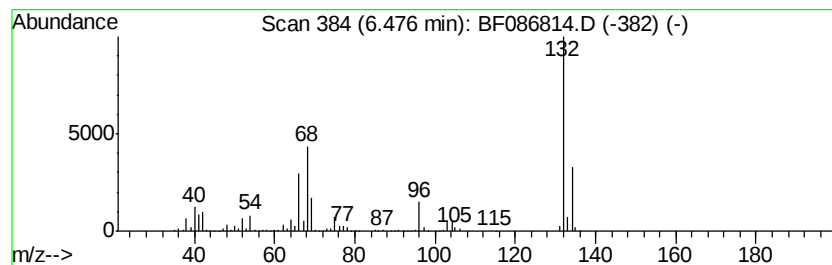

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
Data File : BF086814.D
Acq On : 8 May 2016 10:34
Operator : UM/SJ
Sample : H2720-13 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS7

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	44.0	ng	1400760	1	6.70	1274740	40.0