


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050716\  
 Data File : BF086777.D  
 Acq On : 7 May 2016 16:41  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050416.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 04 15:12:53 2016

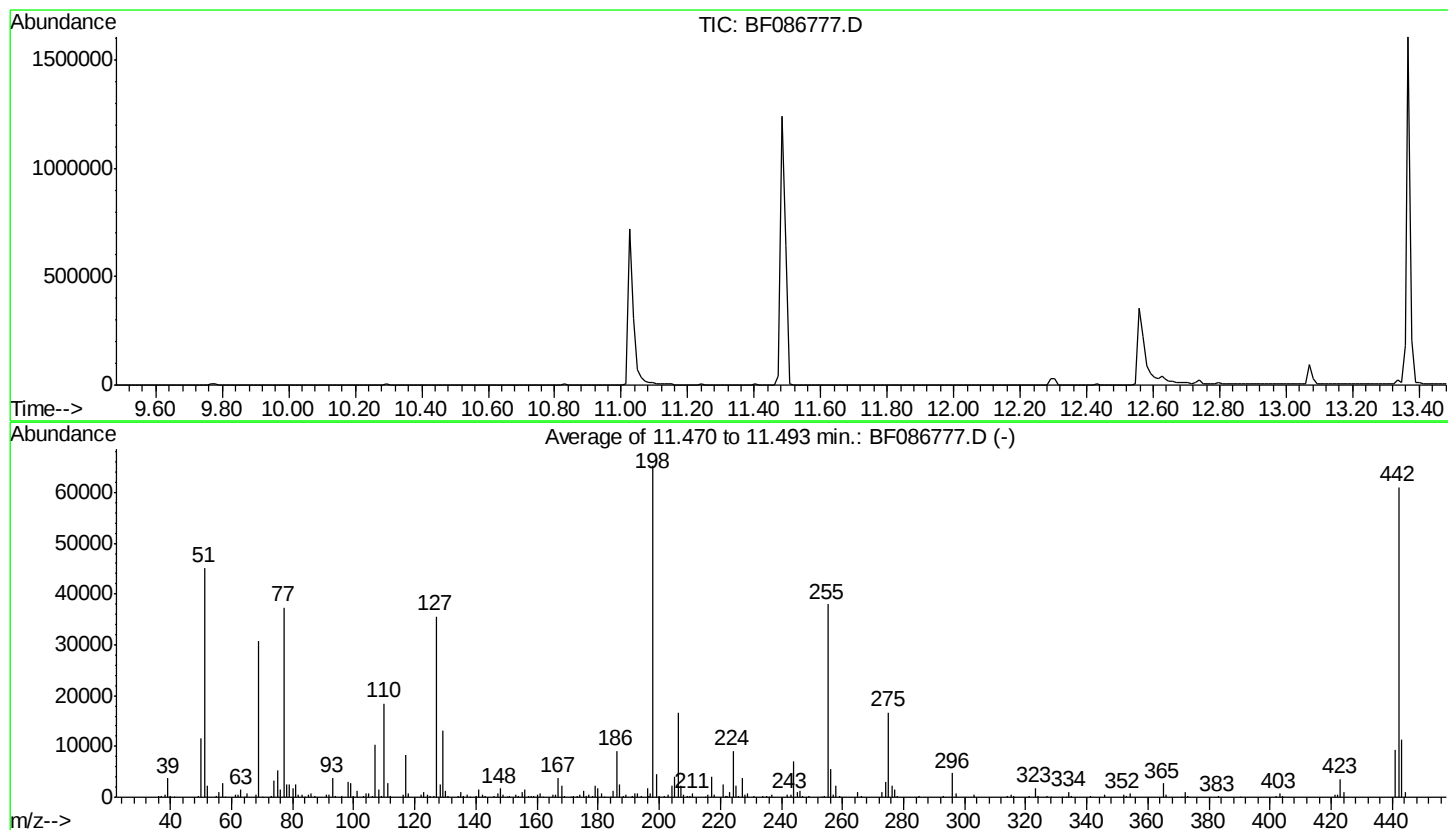

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 818

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 69.3         | 45218      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 481        | PASS                |
| 69             | 198             | 0.00            | 100             | 47.3         | 30858      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 135        | PASS                |
| 127            | 198             | 10              | 80              | 54.4         | 35537      | PASS                |
| 197            | 198             | 0.00            | 2               | 1.0          | 644        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 65268      | PASS                |
| 199            | 198             | 5               | 9               | 7.1          | 4615       | PASS                |
| 275            | 198             | 10              | 60              | 25.5         | 16664      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 2696       | PASS                |
| 441            | 442             | 0.01            | 24              | 15.5         | 9453       | PASS                |
| 442            | 198             | 50              | 100             | 93.4         | 60992      | PASS                |
| 443            | 442             | 15              | 24              | 18.6         | 11370      | PASS                |