


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050716\
 Data File : BF086798.D
 Acq On : 8 May 2016 2:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:12:53 2016

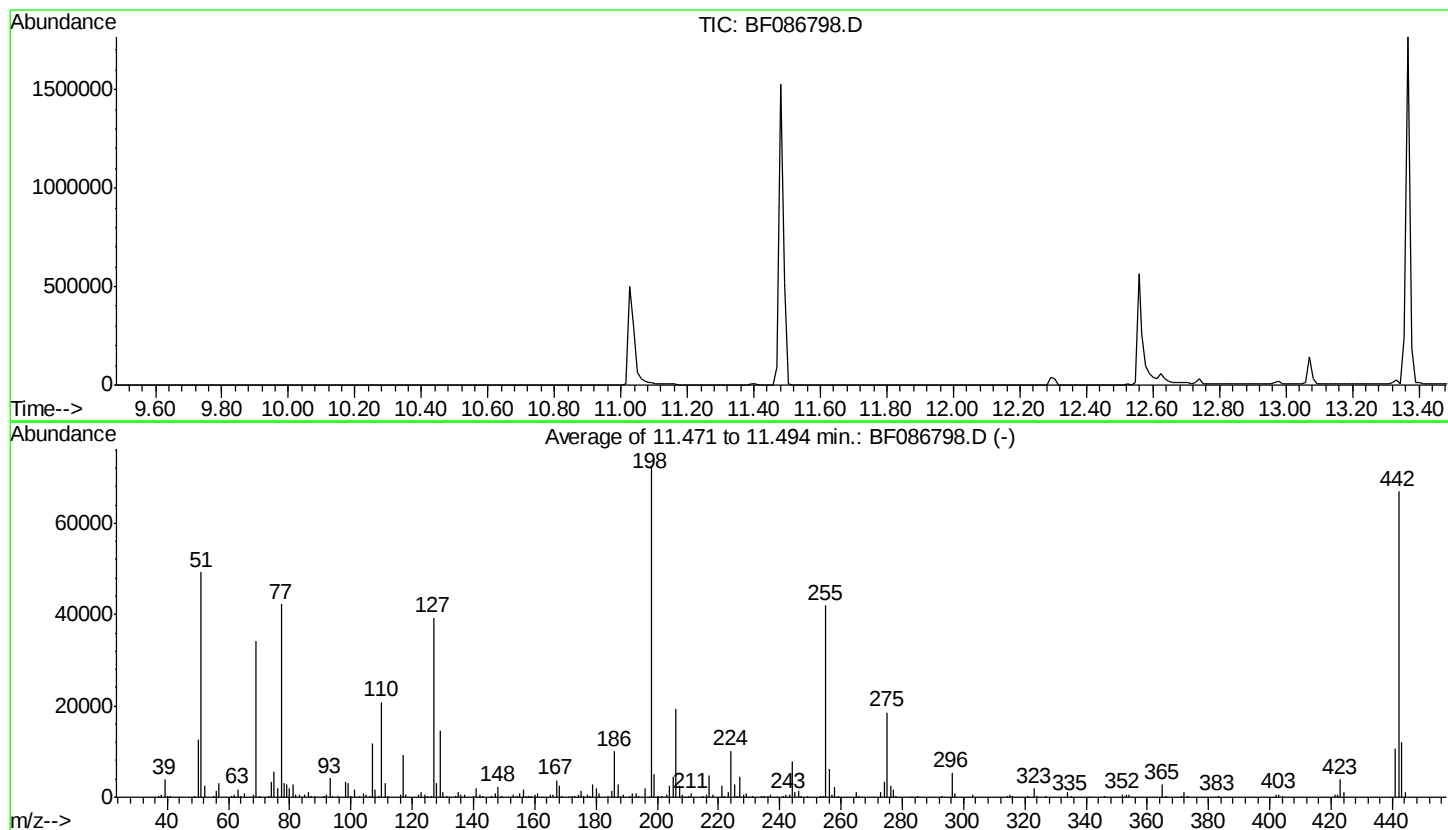

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.9	49284	PASS
68	69	0.00	2	1.5	510	PASS
69	198	0.00	100	47.3	34322	PASS
70	69	0.00	2	0.5	175	PASS
127	198	10	80	54.1	39245	PASS
197	198	0.00	2	0.2	120	PASS
198	198	100	100	100.0	72577	PASS
199	198	5	9	6.9	5029	PASS
275	198	10	60	25.5	18541	PASS
365	198	1	100	3.7	2683	PASS
441	442	0.01	24	16.1	10766	PASS
442	198	50	100	92.1	66857	PASS
443	442	15	24	18.1	12069	PASS