
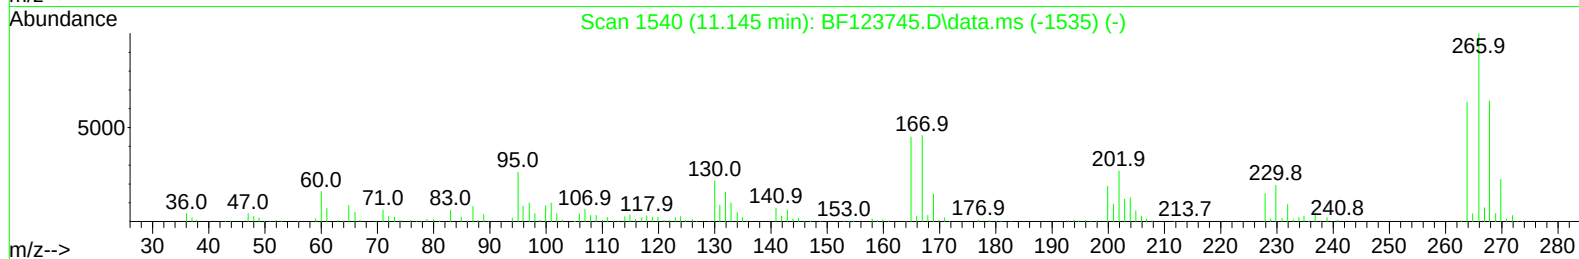
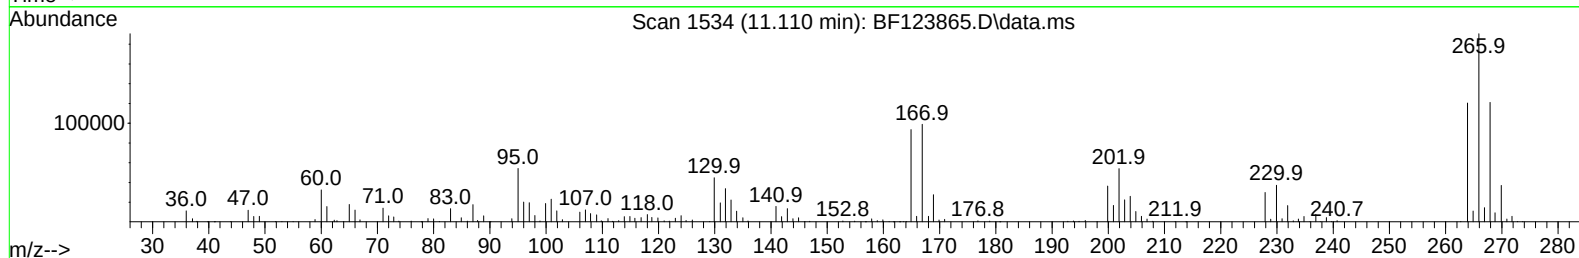


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050721\
Data File : BF123865.D
Acq On : 7 May 2021 11:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:13:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

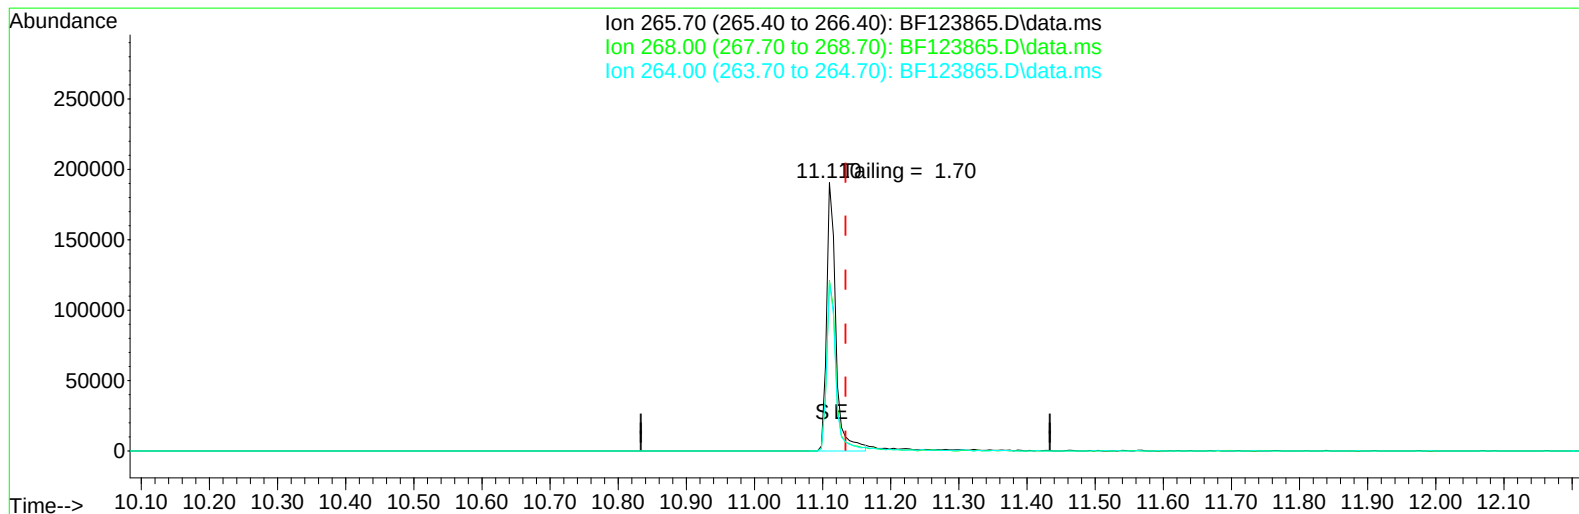

TIC: BF123865.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.024) 30461.70 ng

response 185159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.58
264.00	65.70	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050721\
Data File : BF123865.D
Acq On : 7 May 2021 11:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:13:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

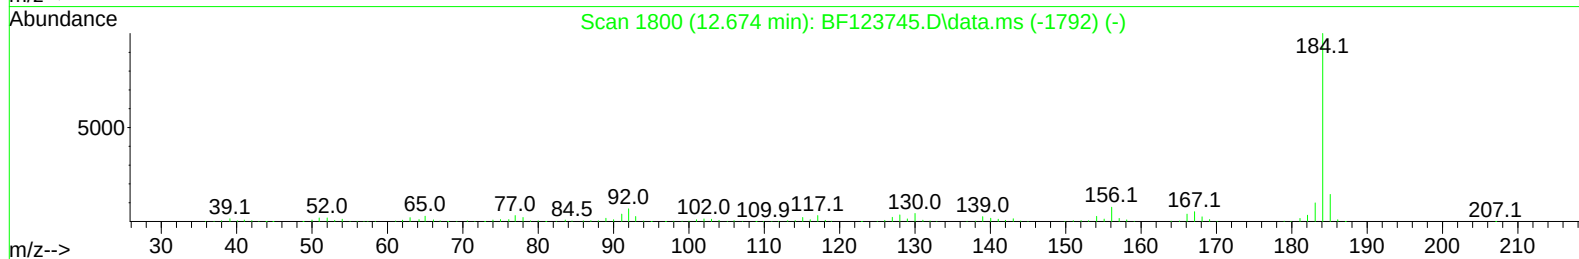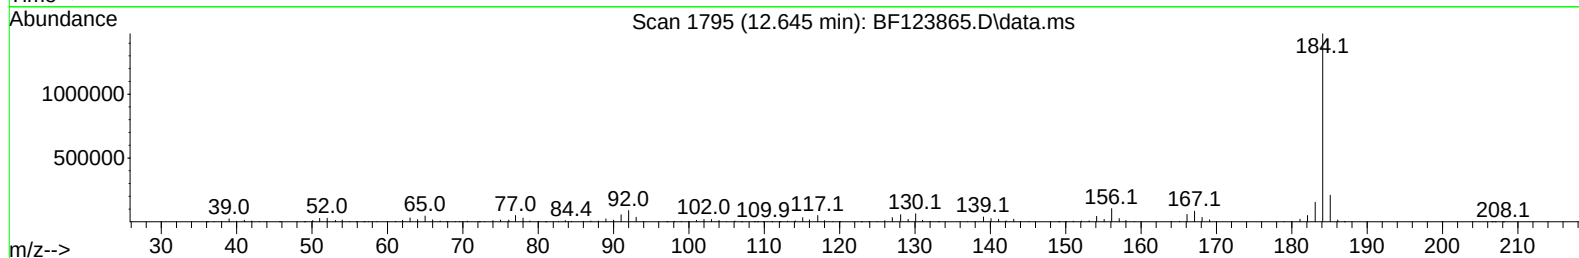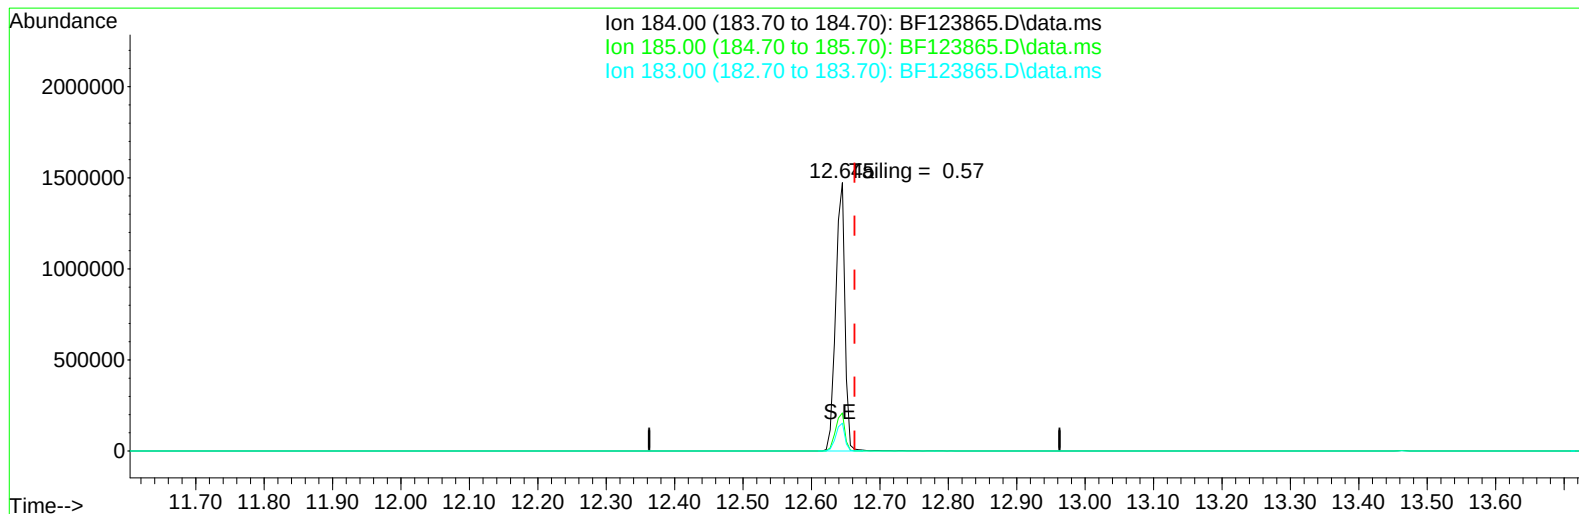

TIC: BF123865.D\data.ms

(77) Benzidine

12.645min (-0.018) 0.00 ng

response 1386149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.19
183.00	9.80	10.38
0.00	0.00	0.00