


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050721\
 Data File : BF123865.D
 Acq On : 7 May 2021 11:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 07 13:43:24 2021

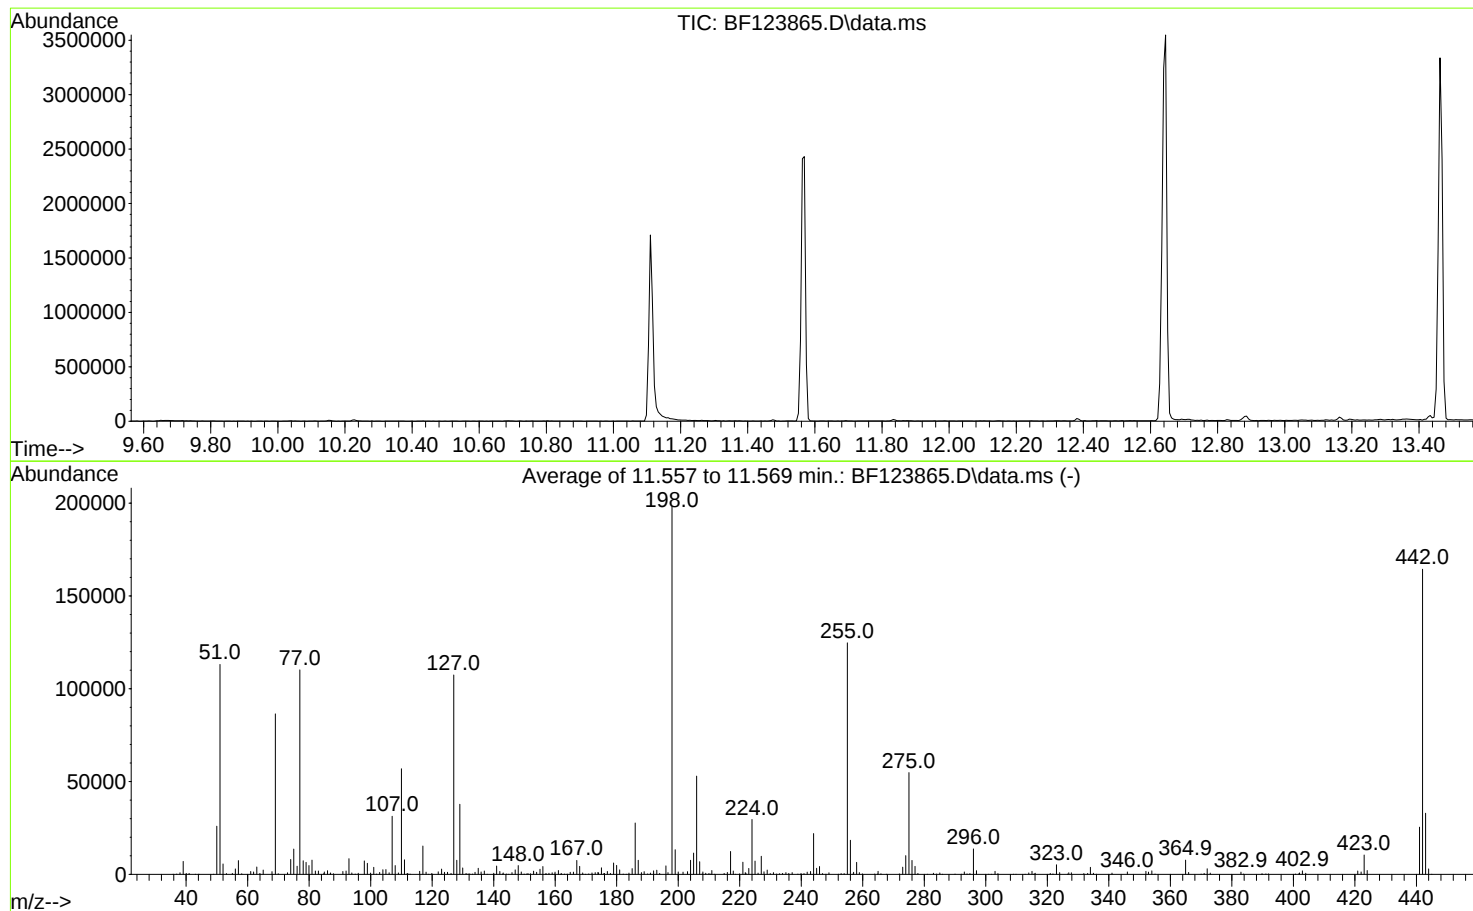

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	113133	PASS
68	69	0.00	2	1.7	1455	PASS
69	198	0.00	100	43.6	86445	PASS
70	69	0.00	2	0.4	389	PASS
127	198	10	80	54.2	107397	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	198189	PASS
199	198	5	9	6.7	13241	PASS
275	198	10	60	27.7	54809	PASS
365	198	1	100	3.9	7701	PASS
441	198	0.01	100	12.8	25450	PASS
442	442	50	100	100.0	164408	PASS
443	442	15	24	20.0	32900	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/7/2021	BNA_F	<u>BF123865.D</u>
Compound Name	Response	Retention Time
DDT	539081	13.46
DDD	4815	13.16
DDE	1259	12.82
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6074	545155	1.11

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050721\
 Data File : BF123865.D
 Acq On : 7 May 2021 11:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 07 12:13:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 13:09:28 2021
 Response via : Initial Calibration

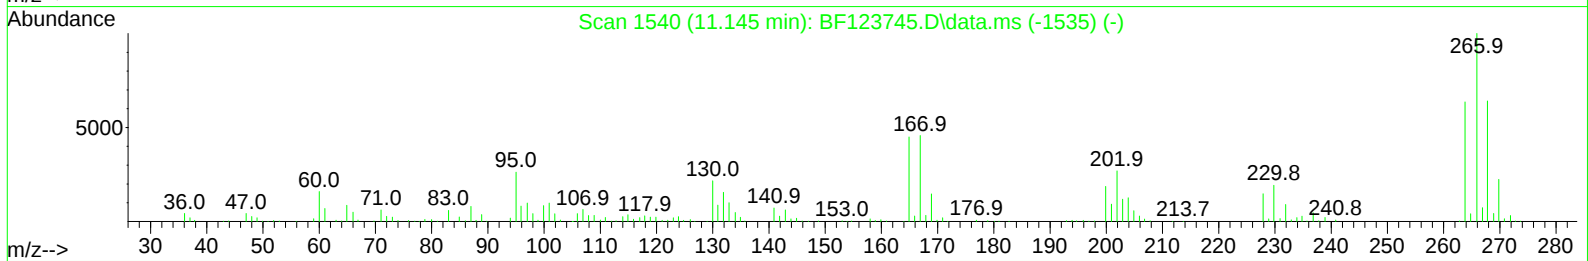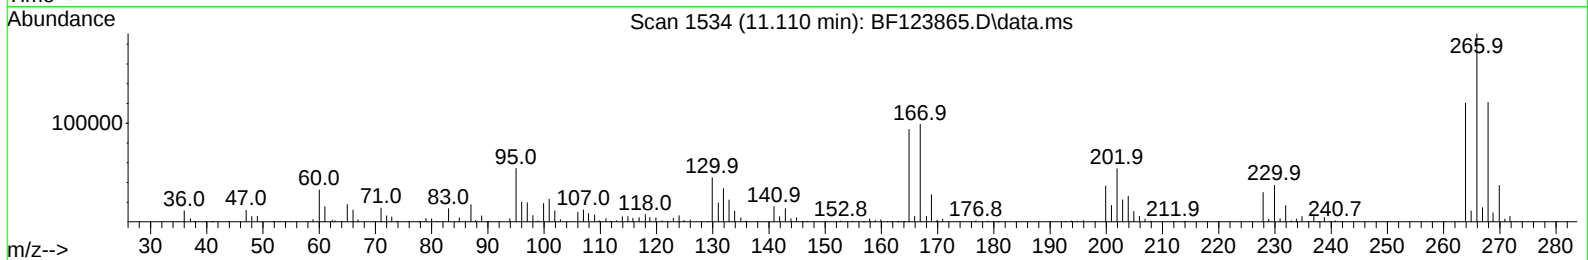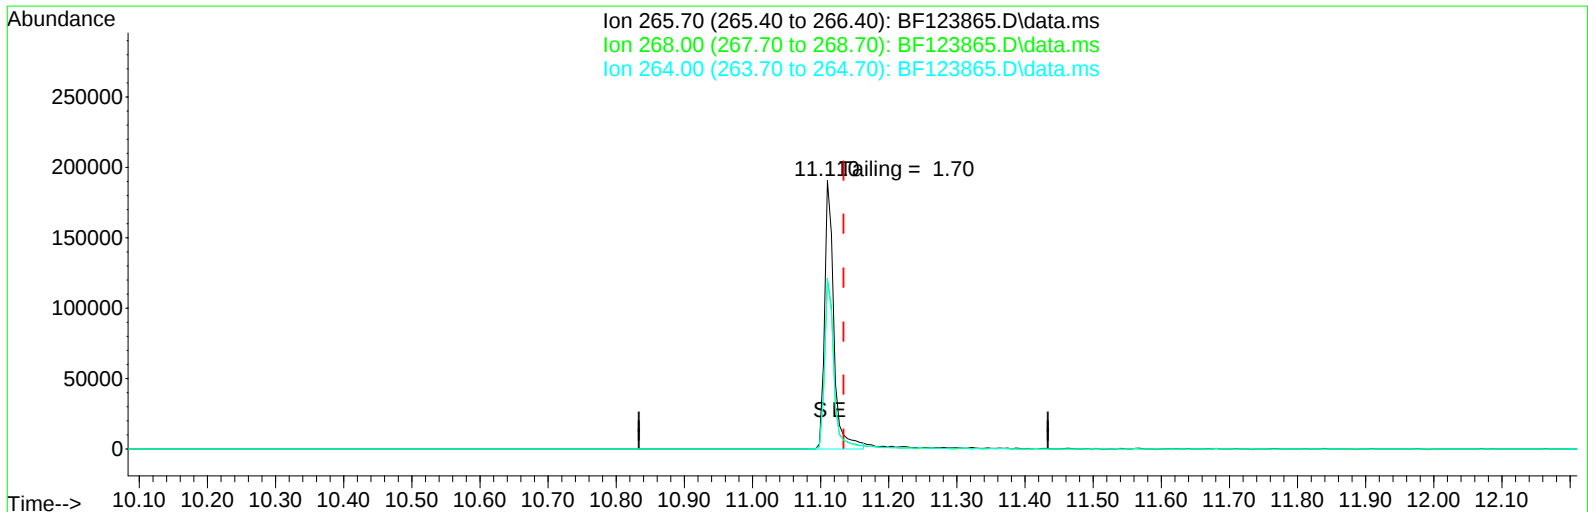

TIC: BF123865.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.024) 30461.70 ng




response 185159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.58
264.00	65.70	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050721\
Data File : BF123865.D
Acq On : 7 May 2021 11:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 07 12:13:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

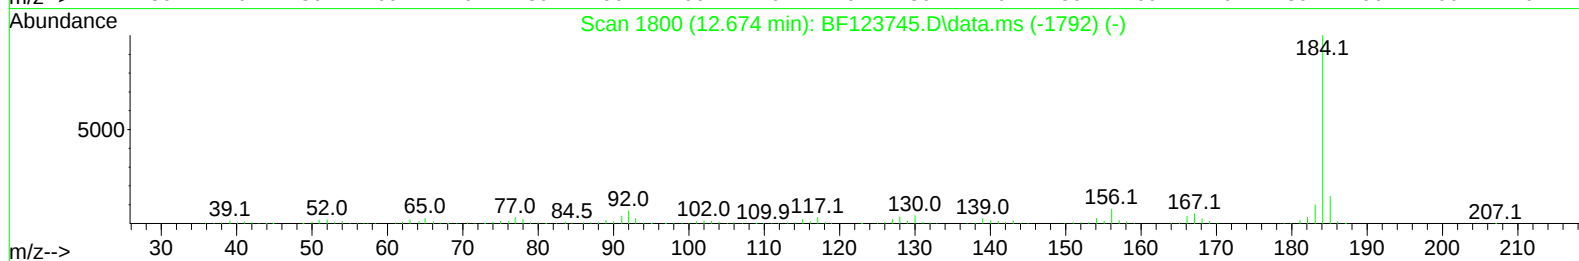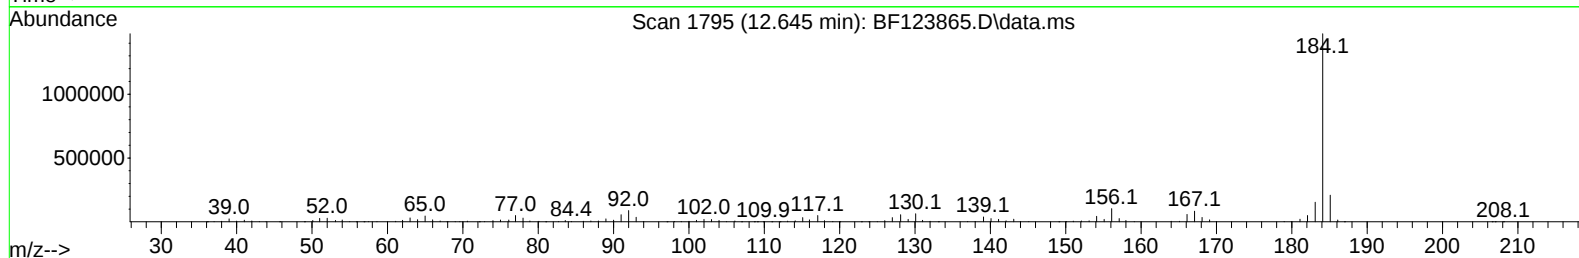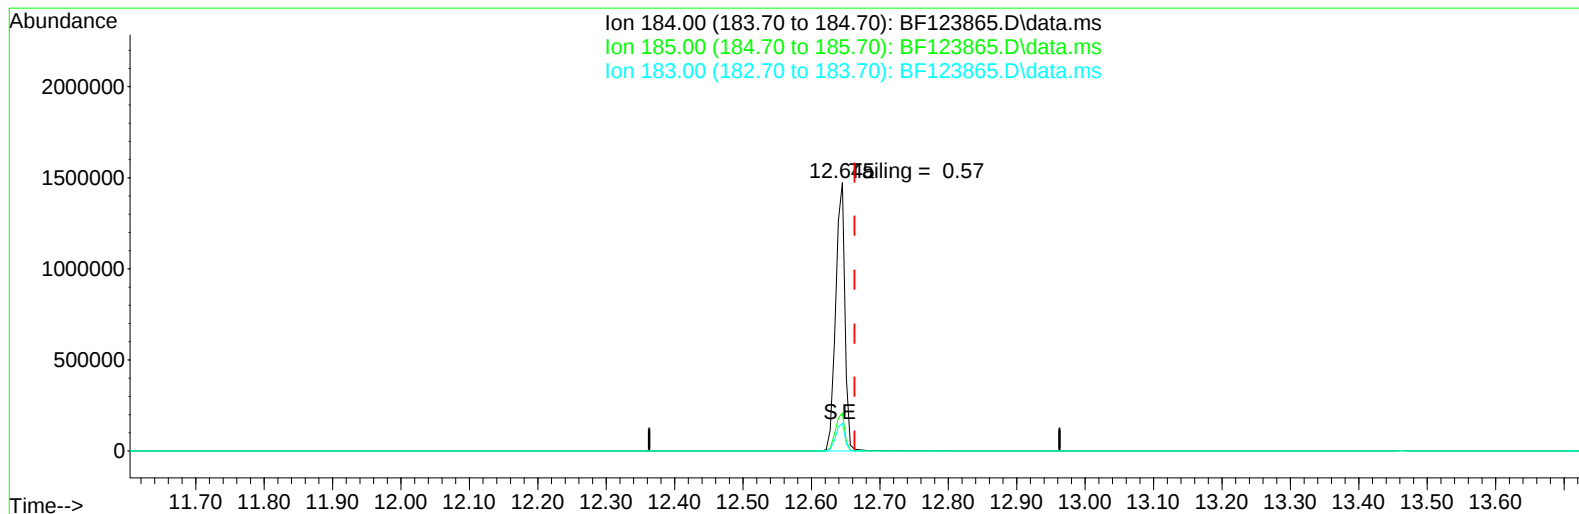

TIC: BF123865.D\data.ms

(77) Benzidine

12.645min (-0.018) 0.00 ng

response 1386149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.19
183.00	9.80	10.38
0.00	0.00	0.00