
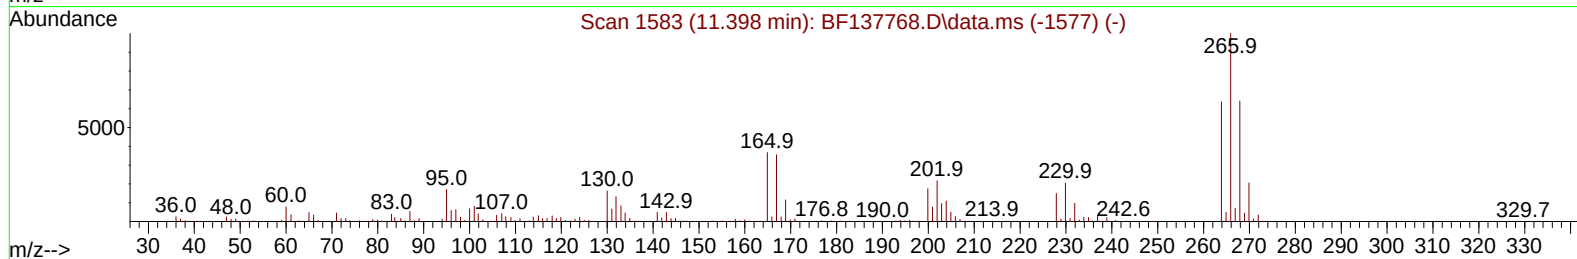
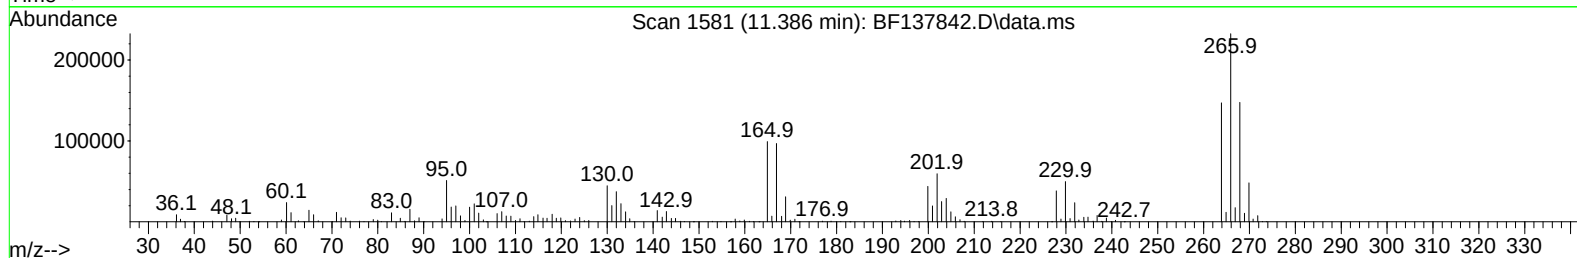


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050724\
Data File : BF137842.D
Acq On : 07 May 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 13:51:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

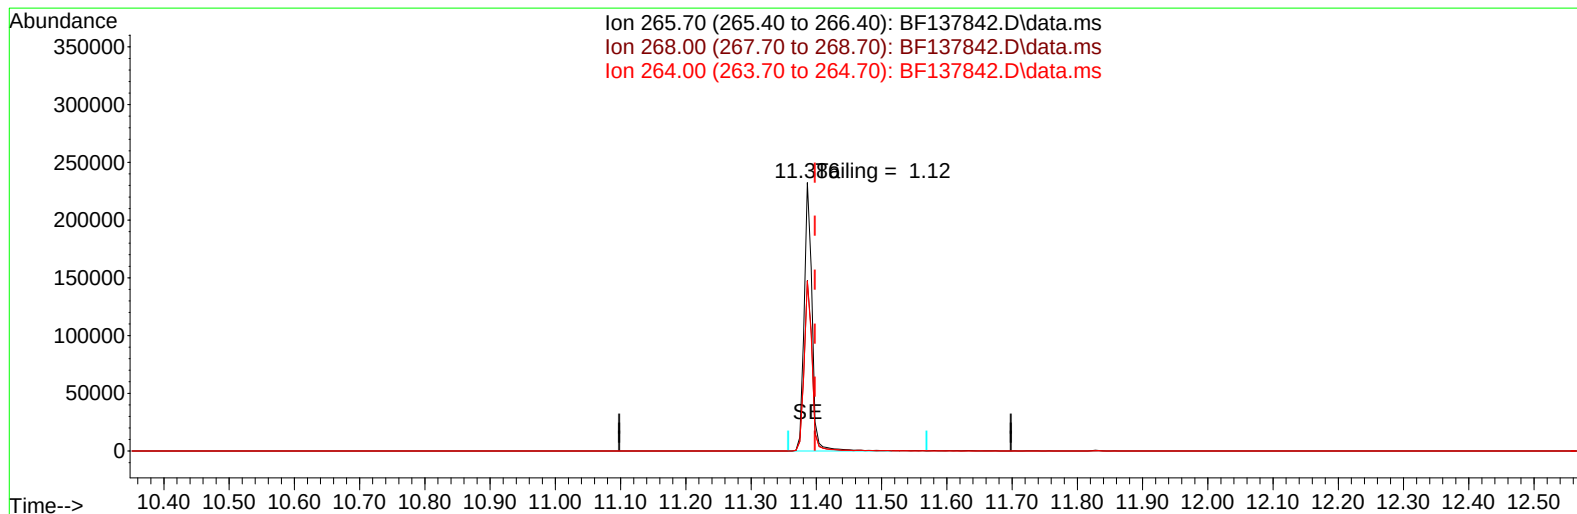

TIC: BF137842.D\data.ms

(70) Pentachlorophenol (C)




11.386min (-0.012) 26720.70 ng

response 197173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.52
264.00	63.70	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050724\
 Data File : BF137842.D
 Acq On : 07 May 2024 12:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 13:51:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:25:08 2024
 Response via : Initial Calibration

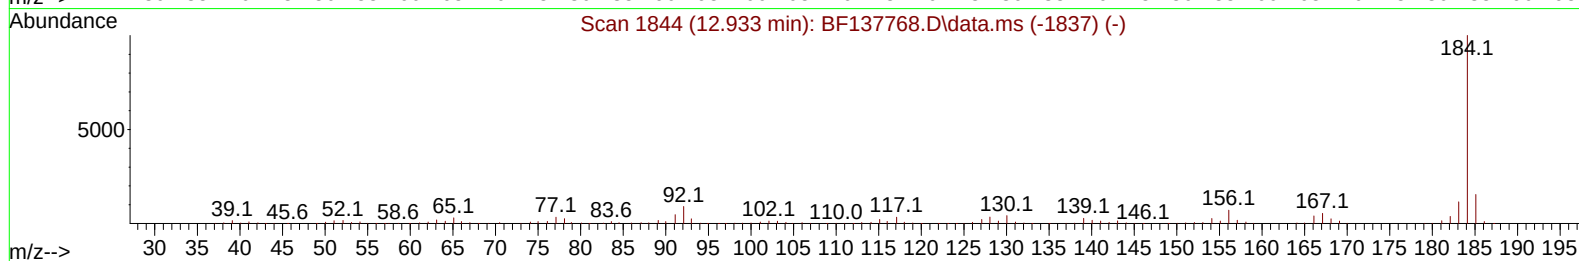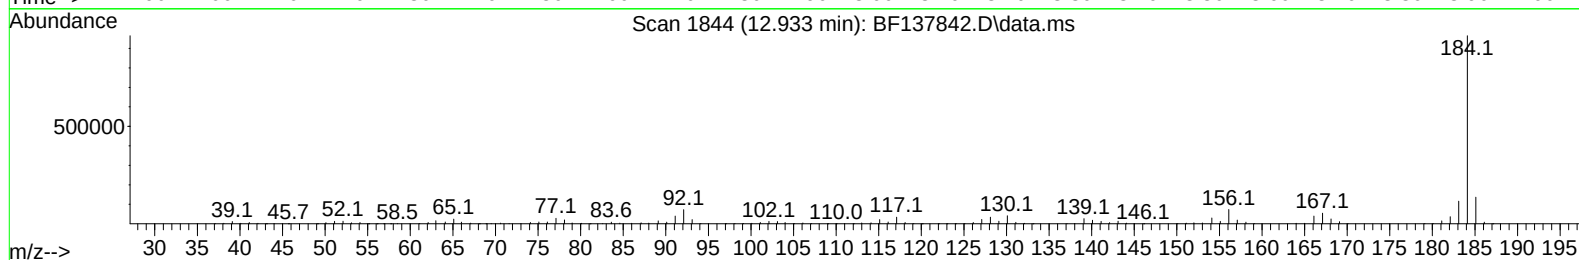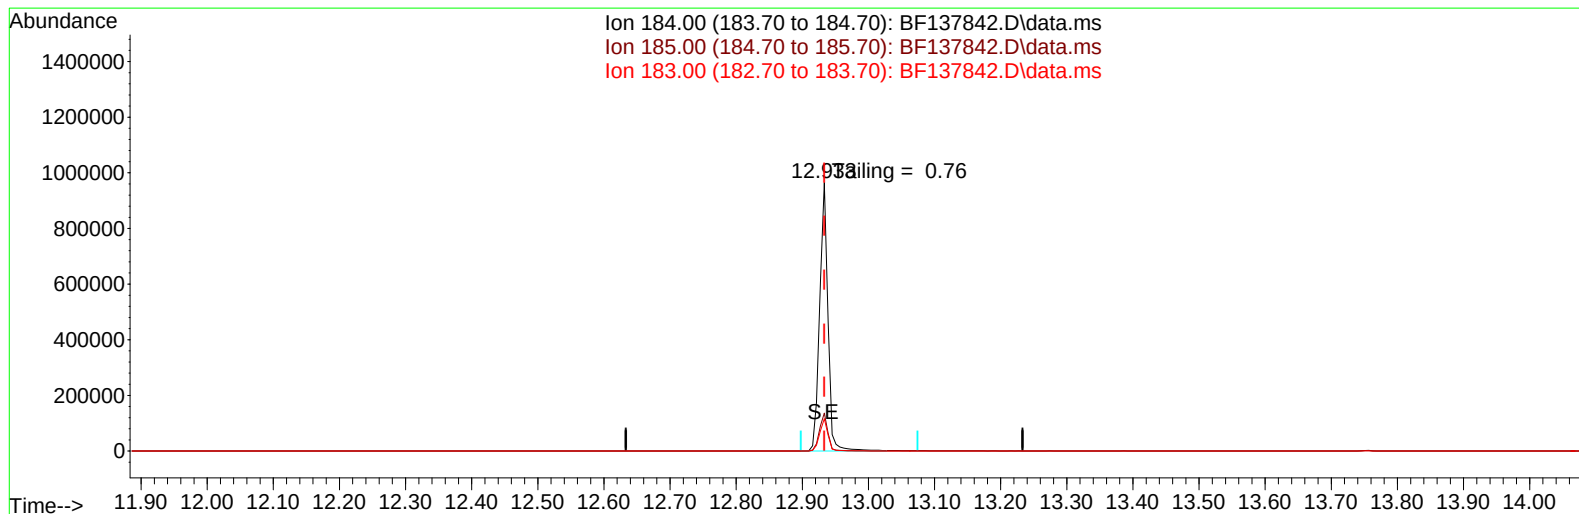

TIC: BF137842.D\data.ms

(77) Benzidine

12.933min (-0.000) 0.00 ng

response 848143

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.17
183.00	11.50	12.03
0.00	0.00	0.00