


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050724\
Data File : BF137842.D
Acq On : 07 May 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

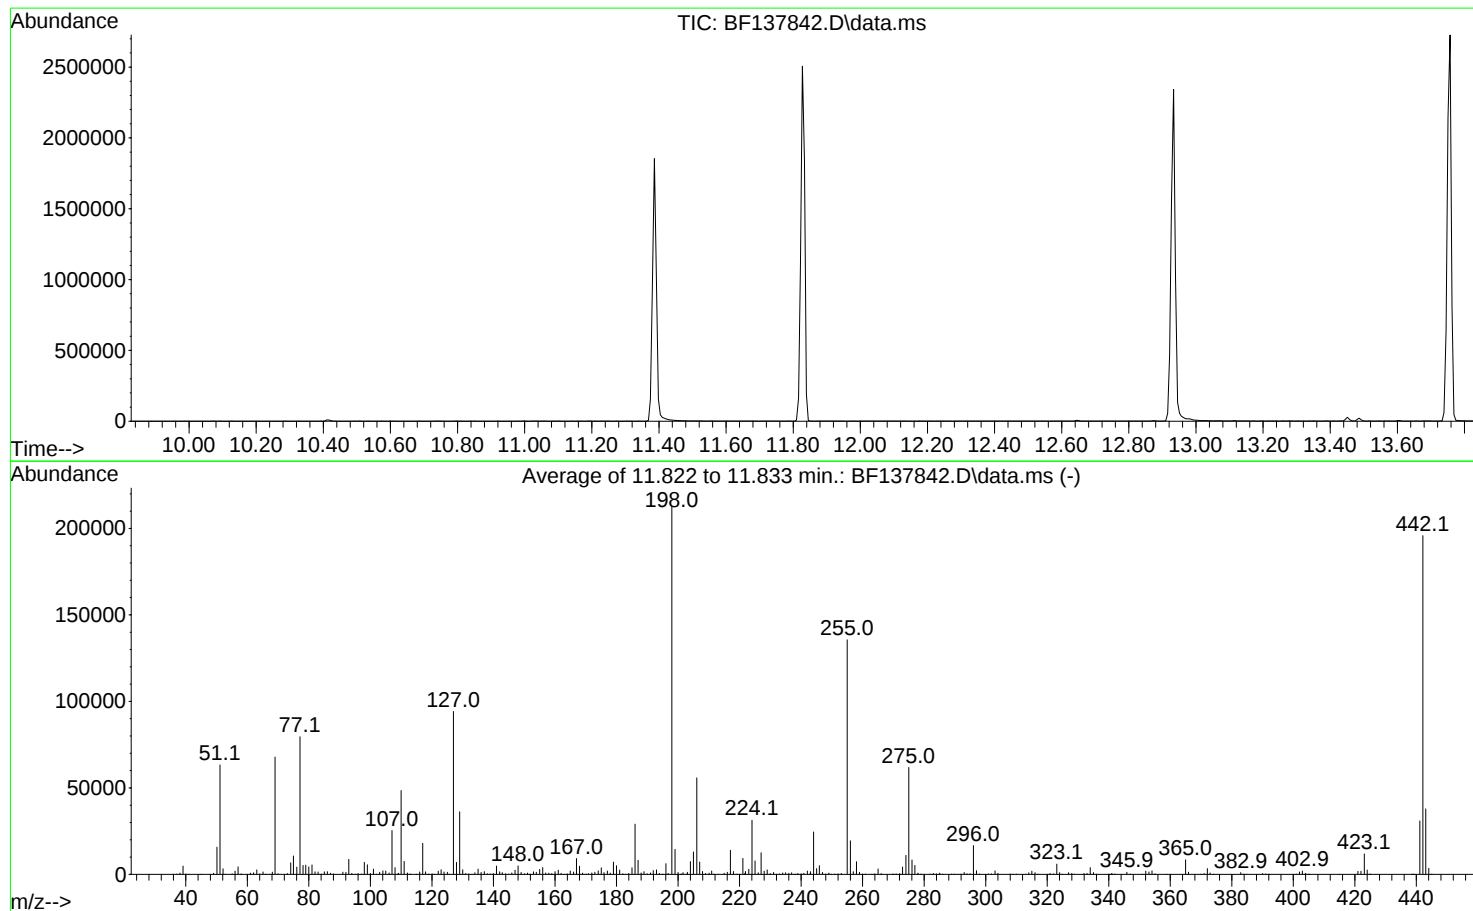

AutoFind: Scans 1655, 1656, 1657; Background Corrected with Scan 1650

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	63237	PASS
68	69	0.00	2	1.9	1288	PASS
69	198	0.00	100	31.9	67795	PASS
70	69	0.00	2	0.6	416	PASS
127	198	10	80	44.3	94179	PASS
197	198	0.00	2	0.3	557	PASS
198	198	100	100	100.0	212672	PASS
199	198	5	9	6.8	14476	PASS
275	198	10	60	29.1	61835	PASS
365	198	1	100	3.9	8384	PASS
441	198	0.01	100	14.5	30917	PASS
442	442	50	100	100.0	195803	PASS
443	442	15	24	19.3	37886	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/7/2024	BNA_F	<u>BF137842.D</u>
Compound Name	Response	Retention Time
DDT	459962	13.757
DDD	8107	13.451
DDE	340	13.116
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8447	468409	1.80

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050724\
Data File : BF137842.D
Acq On : 07 May 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 07 13:51:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

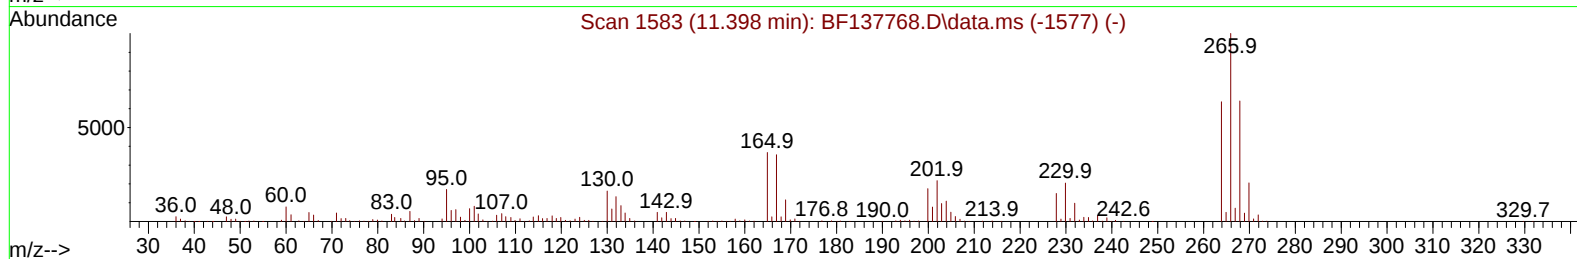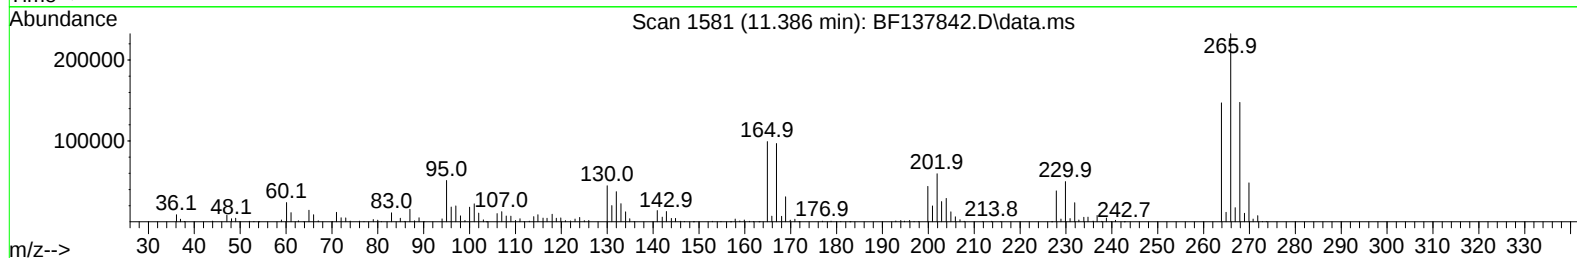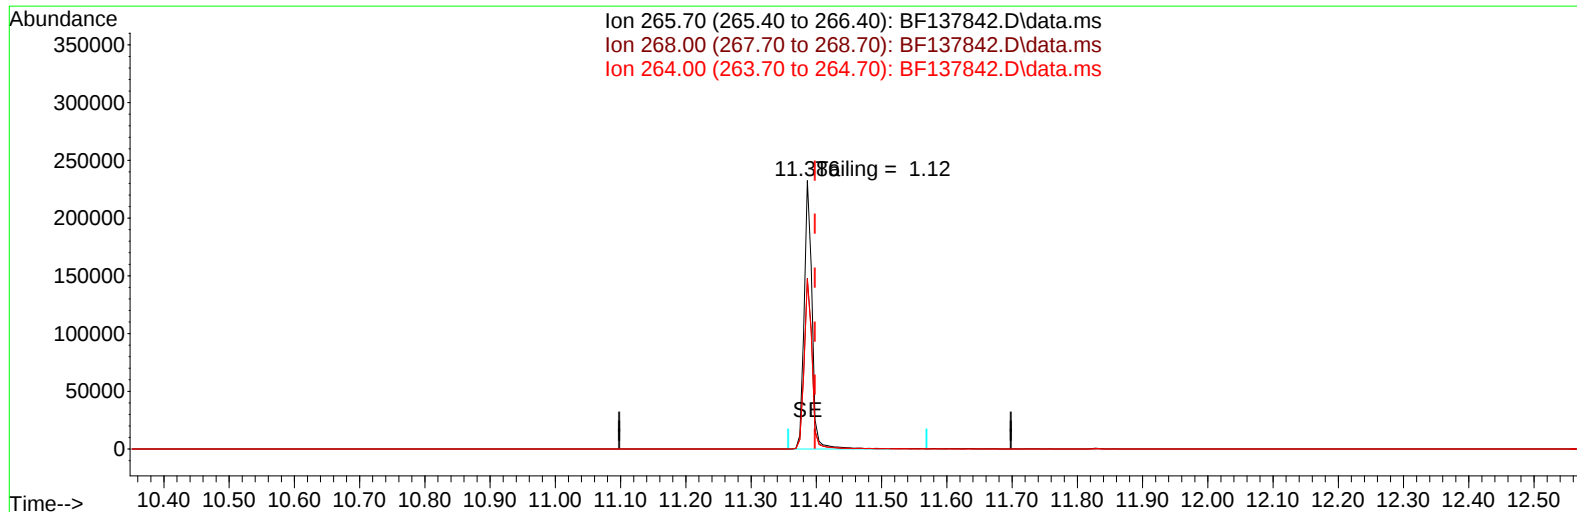

TIC: BF137842.D\data.ms

(70) Pentachlorophenol (C)

11.386min (-0.012) 26720.70 ng




response 197173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.52
264.00	63.70	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050724\
 Data File : BF137842.D
 Acq On : 07 May 2024 12:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 07 13:51:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:25:08 2024
 Response via : Initial Calibration

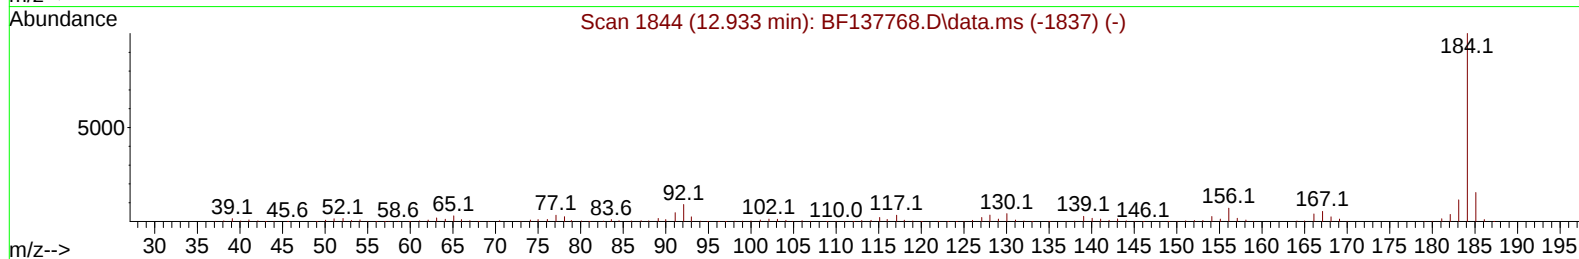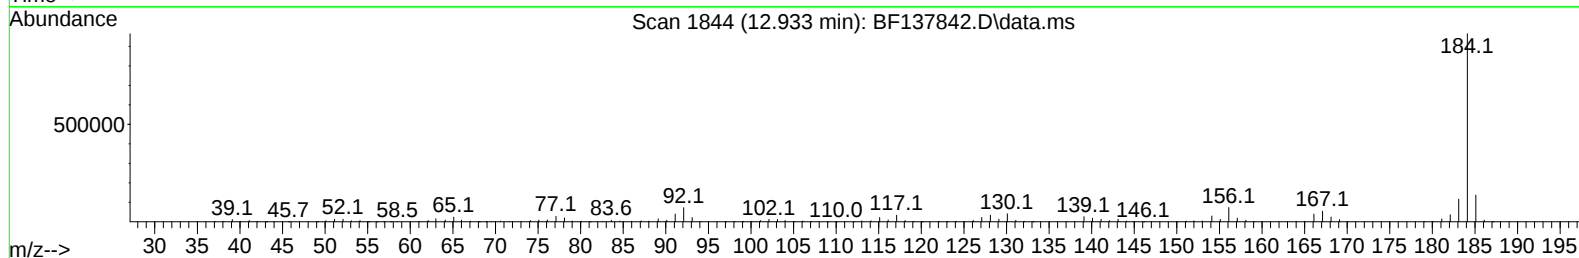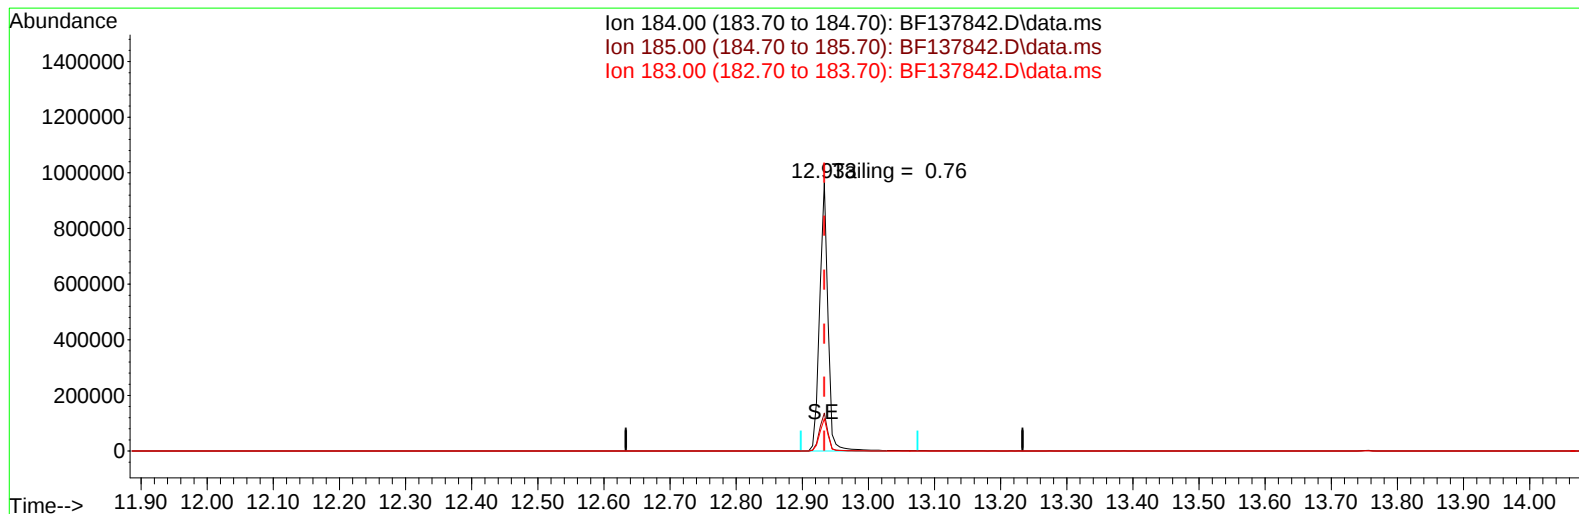

TIC: BF137842.D\data.ms

(77) Benzidine

12.933min (-0.000) 0.00 ng

response 848143

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.17
183.00	11.50	12.03
0.00	0.00	0.00