
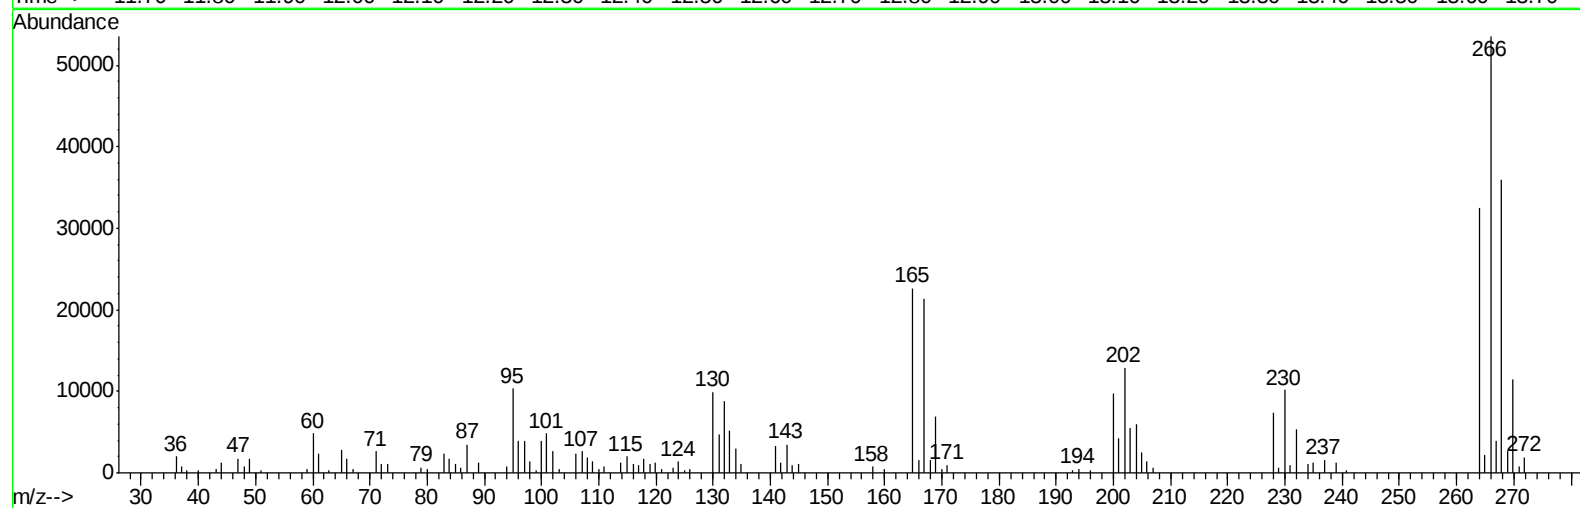


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079036.D
Acq On : 8 May 2015 14:14
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 04:38:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

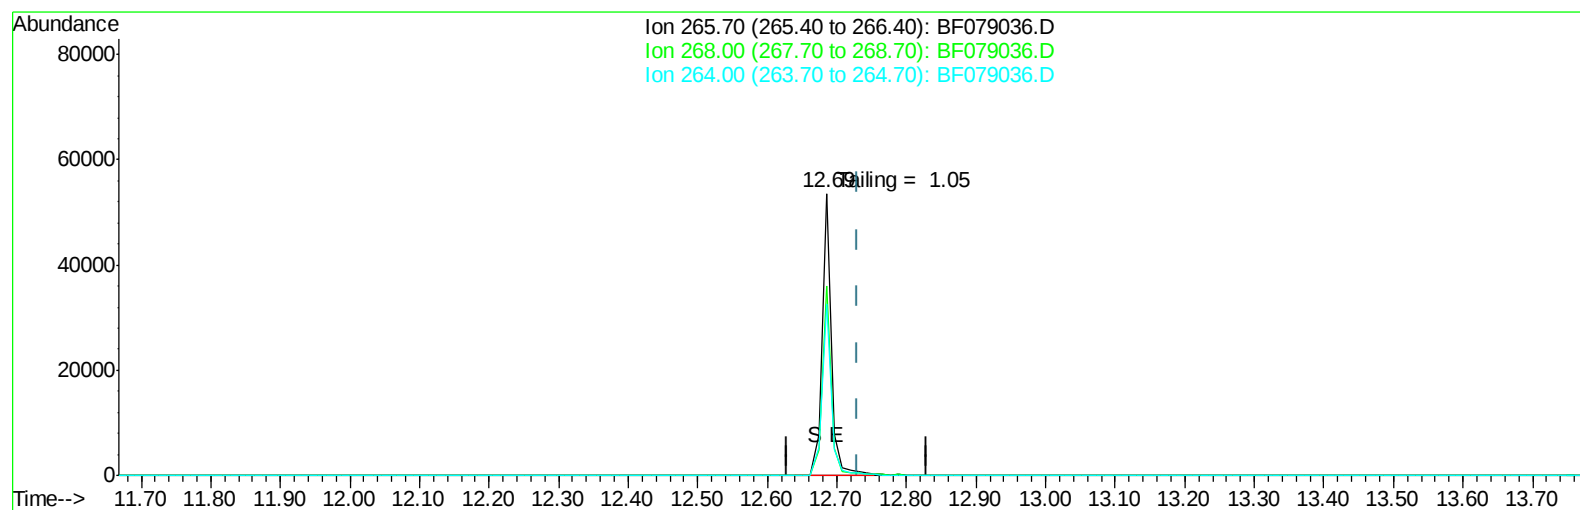

TIC: BF079036.D

(69) Pentachlorophenol (C)



12.685min (-0.045) 0.00ng

response 50549

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.30
264.00	60.20	60.80
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\  
Data File : BF079036.D  
Acq On    : 8 May 2015 14:14  
Operator  : TP/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: May 11 04:38:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

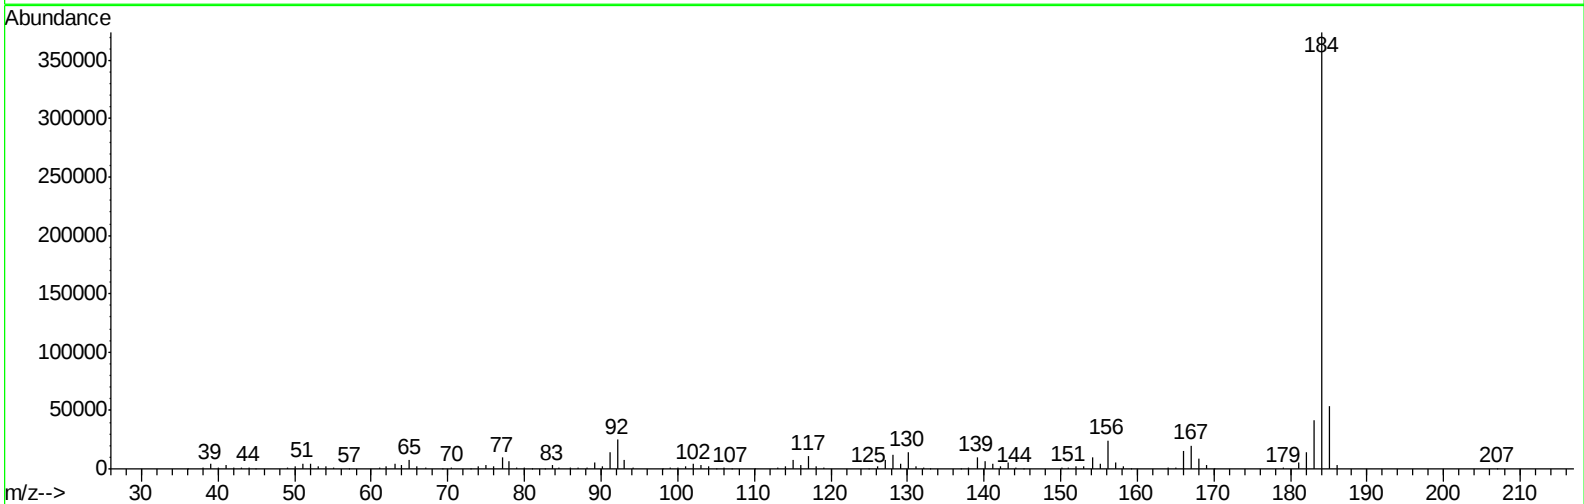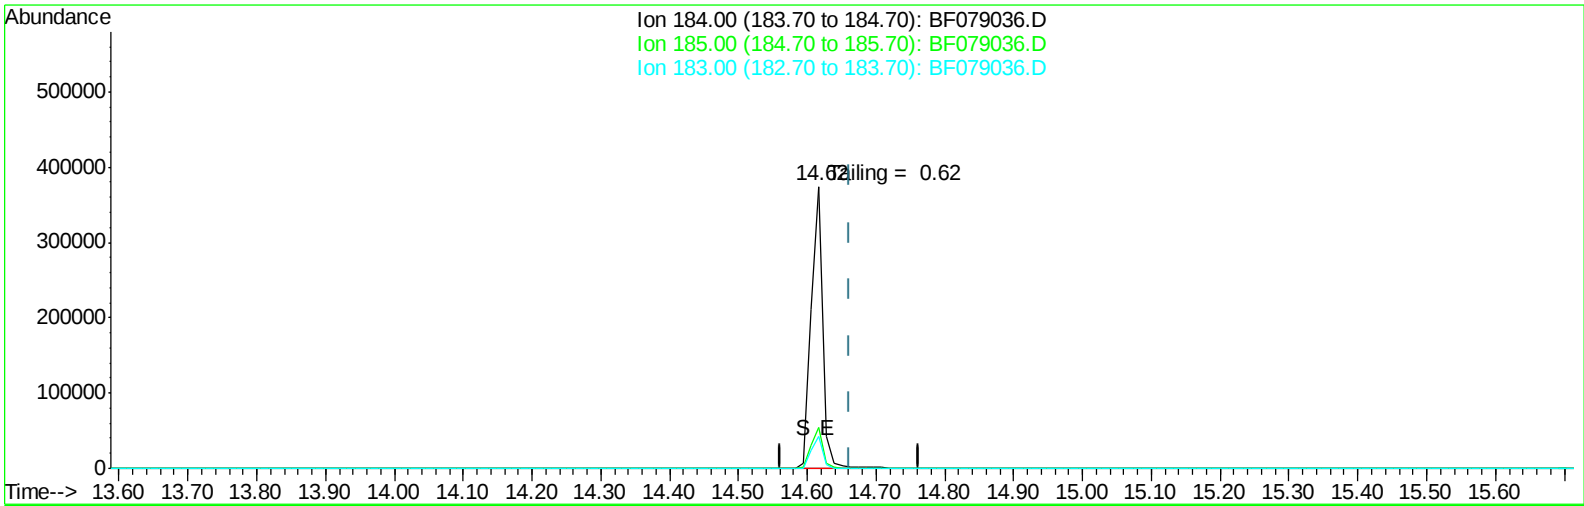

TIC: BF079036.D

(76) Benzidine

14.617min (-0.046) 0.00ng

response 446909

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.40
183.00	10.50	11.16
0.00	0.00	0.00