
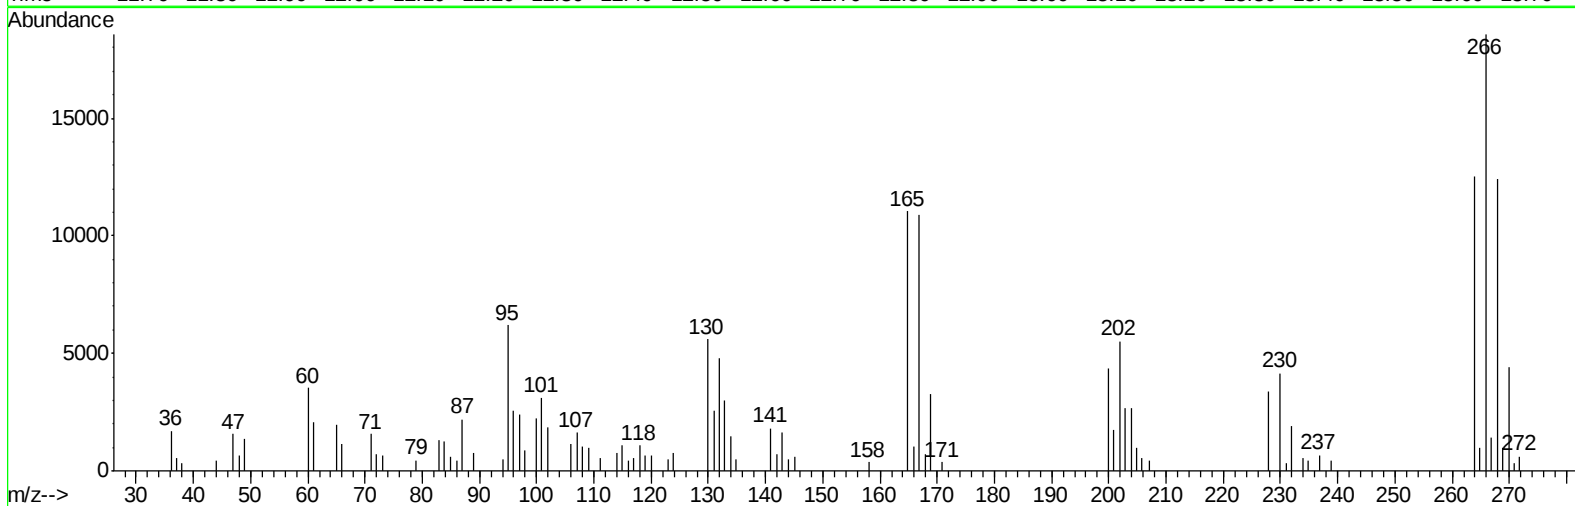


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079085.D
Acq On : 9 May 2015 17:05
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 04:41:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

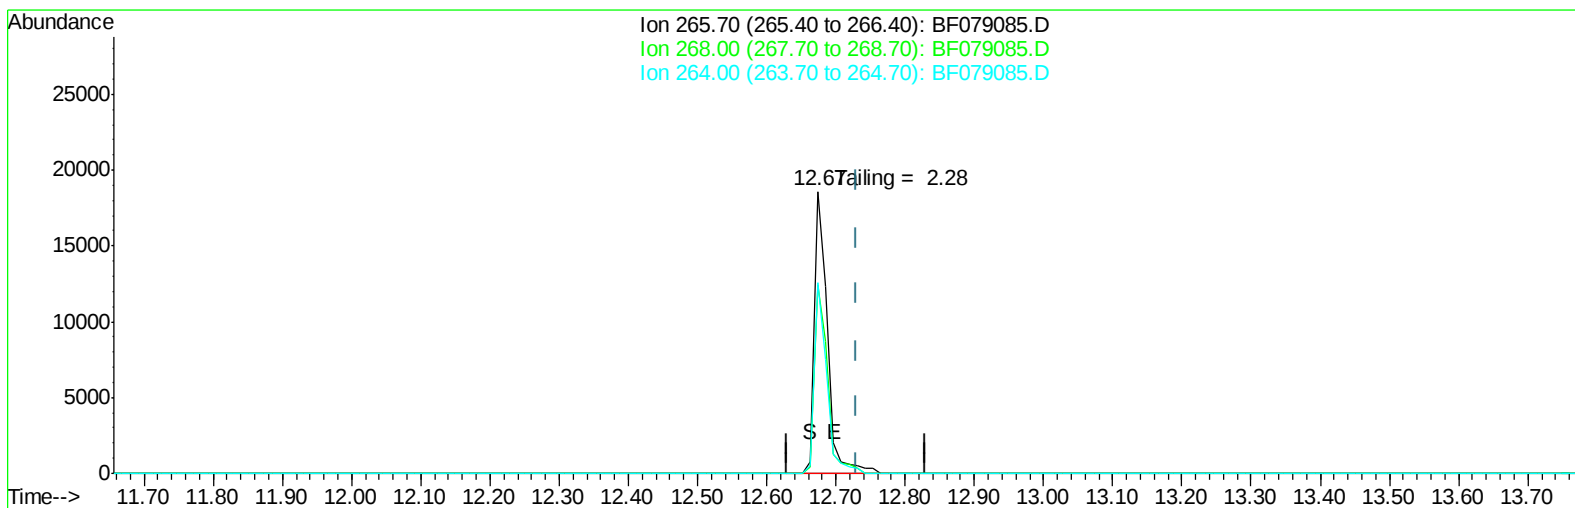

TIC: BF079085.D

(69) Pentachlorophenol (C)



12.674min (-0.056) 0.00ng

response 24805

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.90
264.00	60.20	67.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079085.D
Acq On : 9 May 2015 17:05
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 04:41:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

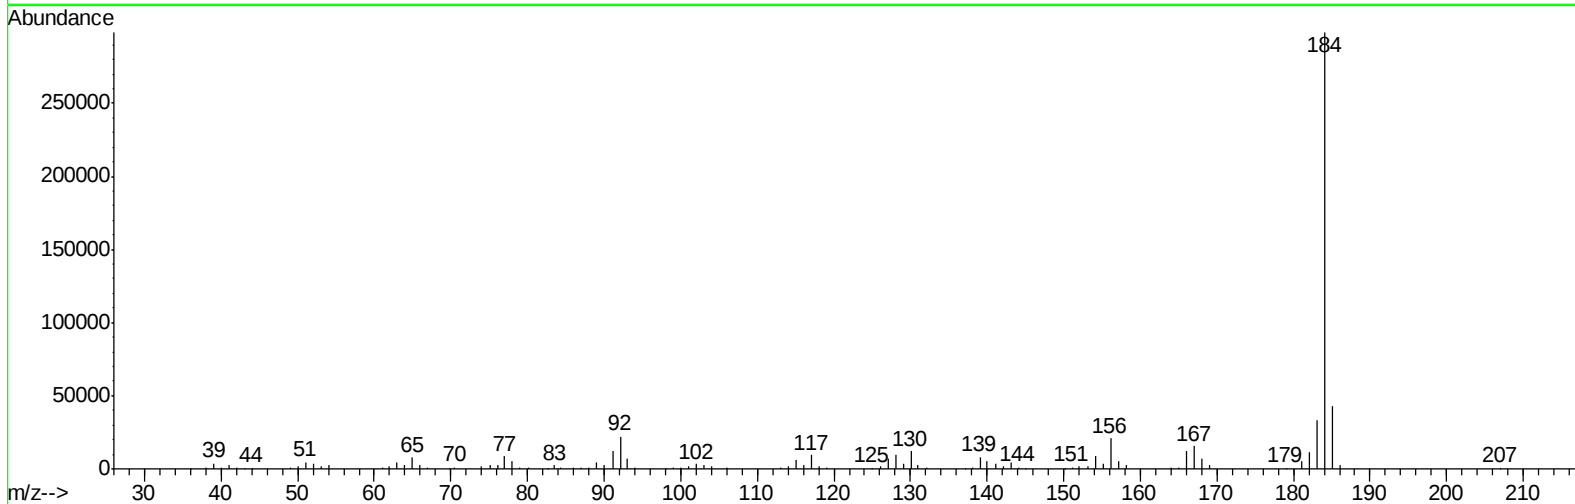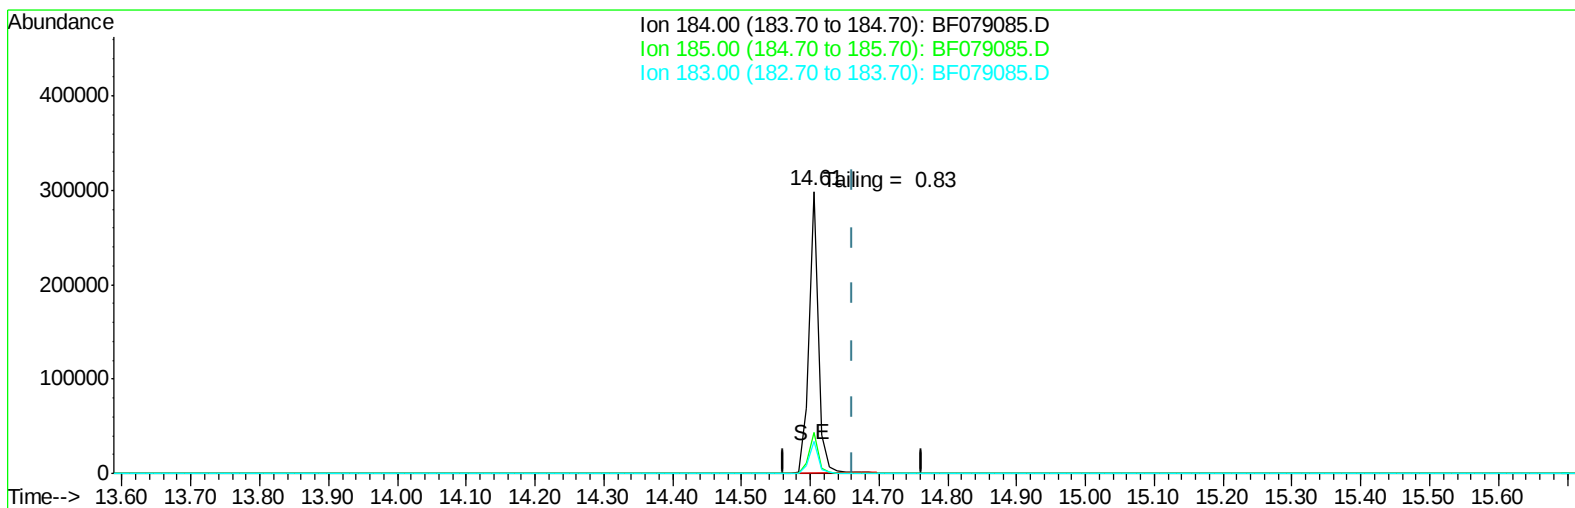

TIC: BF079085.D

(76) Benzidine

14.605min (-0.057) 0.00ng

response 286512

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.49
183.00	10.50	11.21
0.00	0.00	0.00