

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050815\
 Data File : BF079069.D
 Acq On : 9 May 2015 8:04
 Operator : TP/IZ
 Sample : G2152-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-13-5.0

Quant Time: May 11 01:30:07 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 11 00:37:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.32	152	77681	20.00	ng	0.00
21) Naphthalene-d8	8.89	136	327800	20.00	ng	-0.01
38) Acenaphthene-d10	11.07	164	165763	20.00	ng	0.00
63) Phenanthrene-d10	12.91	188	312592	20.00	ng	0.00
75) Chrysene-d12	16.22	240	306251	20.00	ng	0.00
86) Perylene-d12	17.98	264	301135	20.00	ng	0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	375096	83.12	ng	0.00
7) Phenol-d6	6.88	99	524069	87.86	ng	0.00
23) Nitrobenzene-d5	8.01	82	282582	49.54	ng	0.00
41) 2,4,6-Tribromophenol	12.06	330	137395	76.62	ng	0.00
44) 2-Fluorobiphenyl	10.24	172	531128	44.64	ng	0.00
78) Terphenyl-d14	14.91	244	603031	47.14	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050815\
Data File : BF079069.D
Acq On : 9 May 2015 8:04
Operator : TP/IZ
Sample : G2152-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TU021-SB-13-5.0

Quant Time: May 11 01:30:07 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 00:37:37 2015
Response via : Initial Calibration

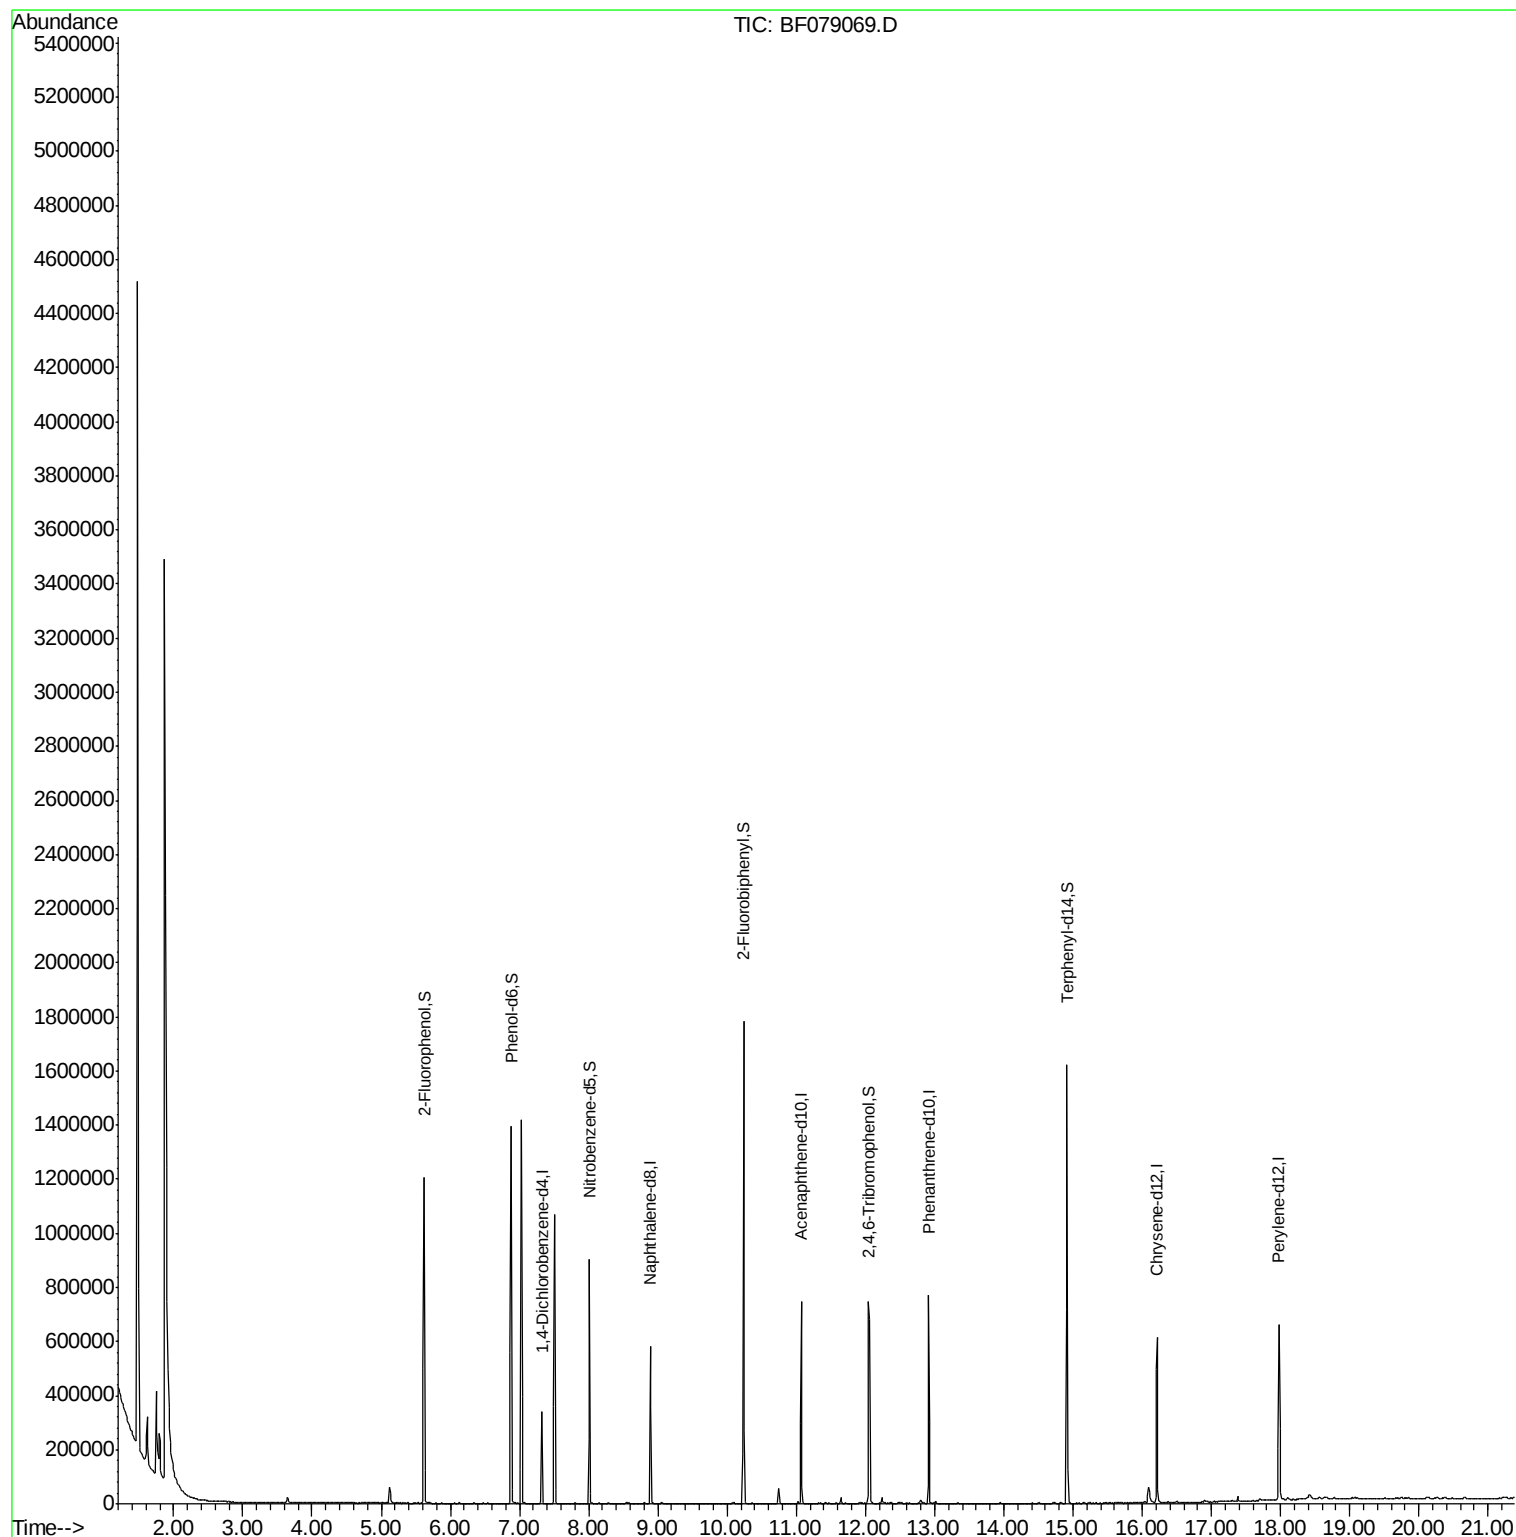




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.32 min Scan# 537
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-13-5.0

Tot Ion:152 Resp: 77681
 Ion Ratio Lower Upper
 152 100
 150 153.4 122.0 183.0
 115 51.4 46.3 69.5

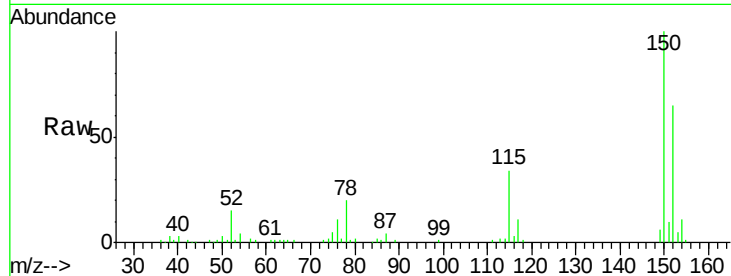


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

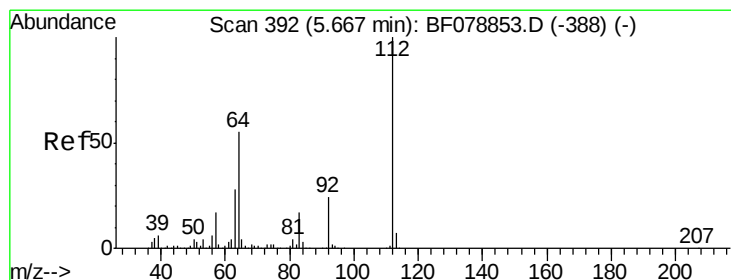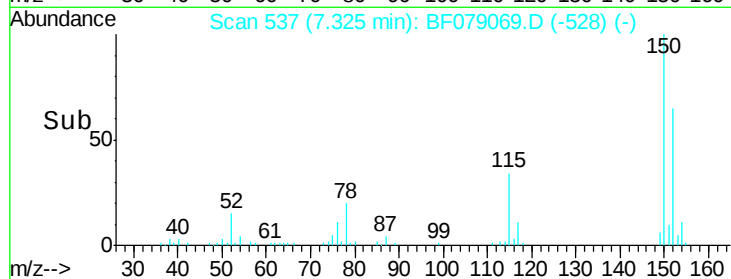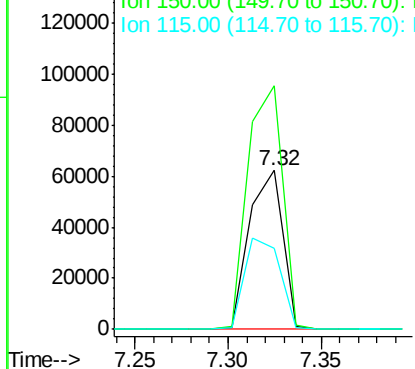



#5

2-Fluorophenol
 Concen: 83.12 ng
 RT: 5.62 min Scan# 388
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Tgt Ion:112 Resp: 375096
 Ion Ratio Lower Upper
 112 100
 64 56.0 53.5 80.3
 63 27.0 27.5 41.3#

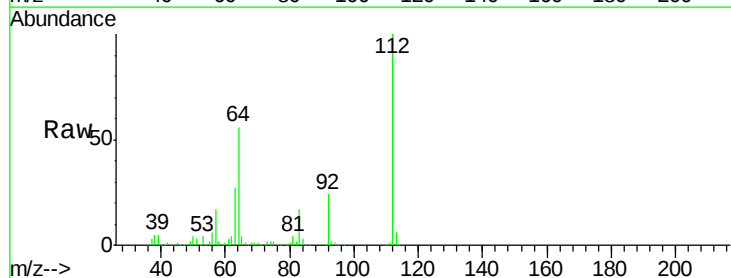

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

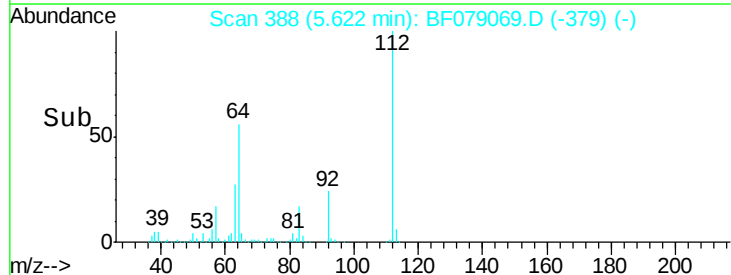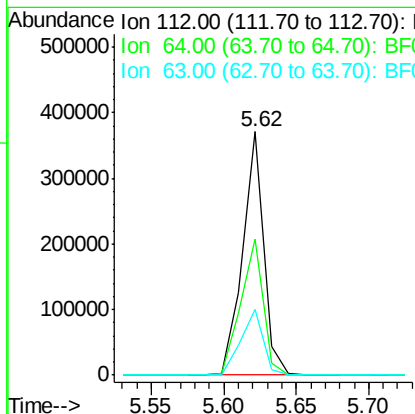



#7

Phenol-d6

Concen: 87.86 ng

RT: 6.88 min Scan# 498

Delta R.T. -0.00 min

Lab File: BF079069.D

Acq: 9 May 2015 8:04

Instrument :

BNA_F

ClientSampleId :

TU021-SB-13-5.0


Tot Ion: 99 Resp: 524069

Ion Ratio Lower Upper

99 100

42 15.7 12.8 19.2




71 28.6 23.4 35.2

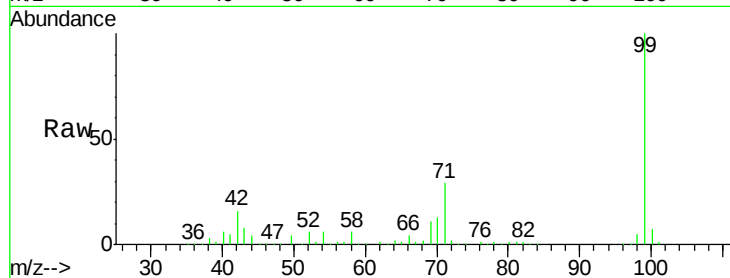

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

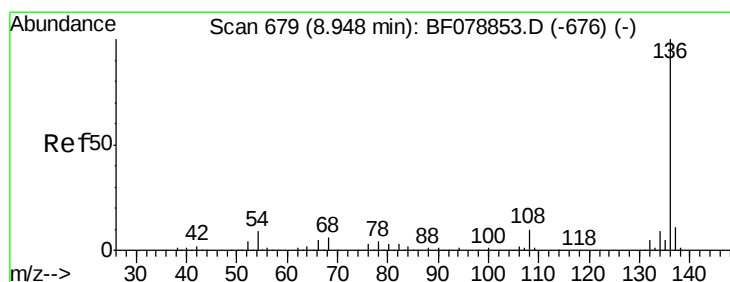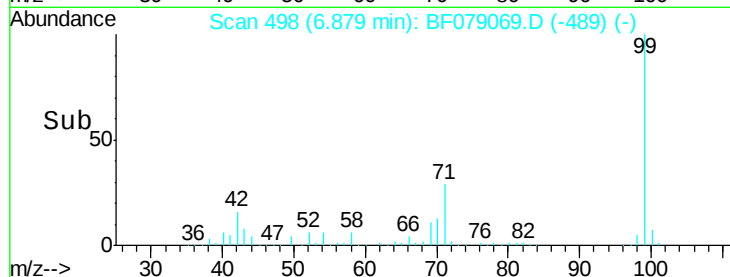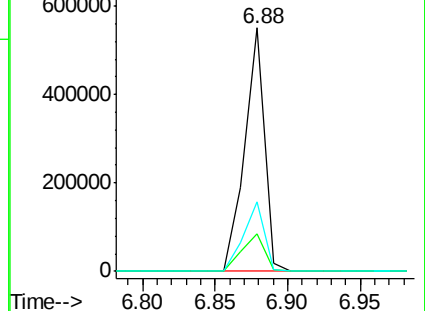

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.89 min Scan# 674

Delta R.T. -0.01 min

Lab File: BF079069.D

Acq: 9 May 2015 8:04

Tgt Ion: 136 Resp: 327800


Ion Ratio Lower Upper

136 100

137 11.2 8.7 13.1

54 9.9 5.8 8.8#

68 7.1 4.2 6.4#


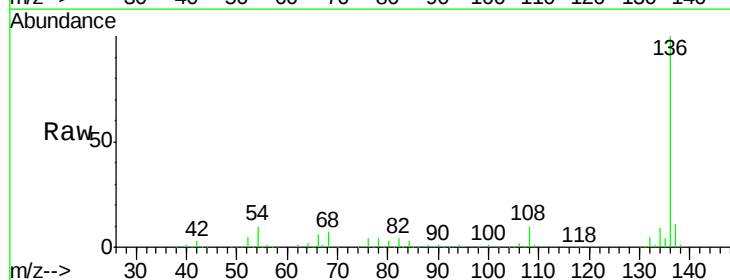



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

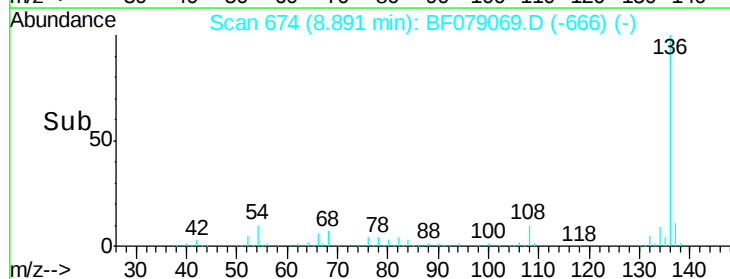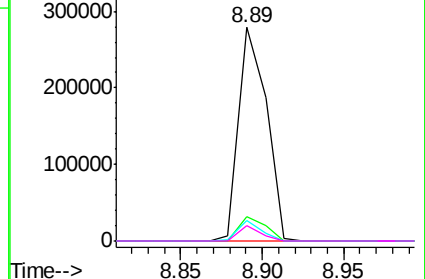


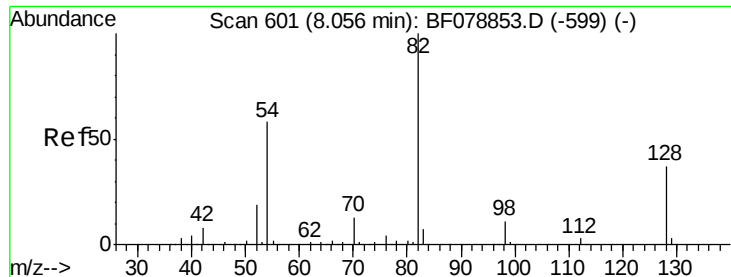




#23
 Nitrobenzene-d5
 Concen: 49.54 ng
 RT: 8.01 min Scan# 597
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-13-5.0

Tot Ion	82	Resp	282582
Ion Ratio	100	Lower	Upper
128	44.3	30.0	45.0
54	49.6	46.4	69.6

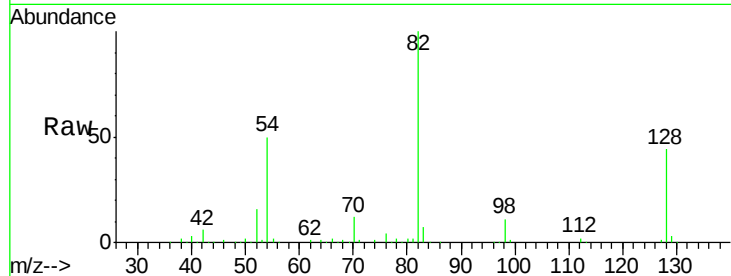


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

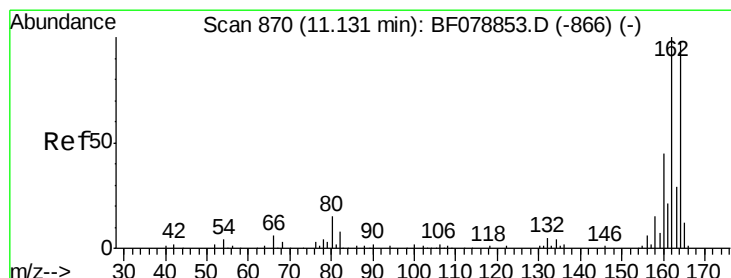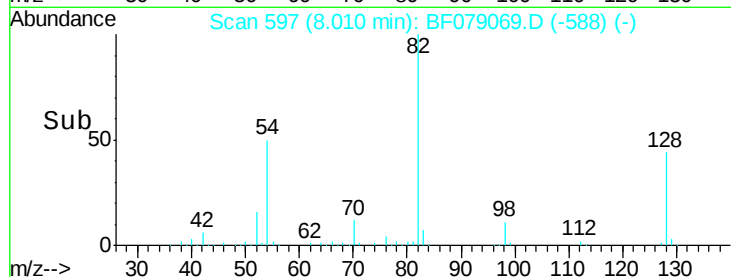
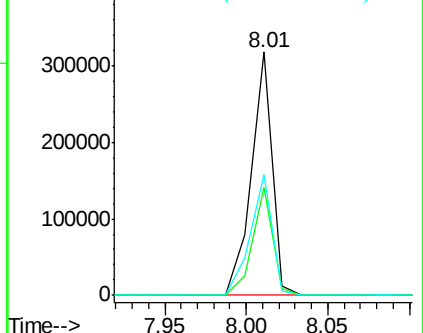


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.07 min Scan# 865
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Tgt Ion	164	Resp	165763
Ion Ratio	100	Lower	Upper
162	103.2	82.7	124.1
160	45.8	35.8	53.8

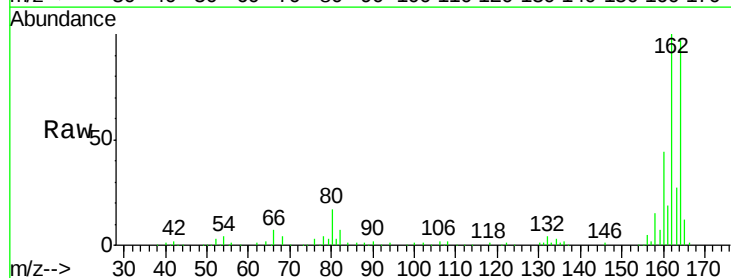

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



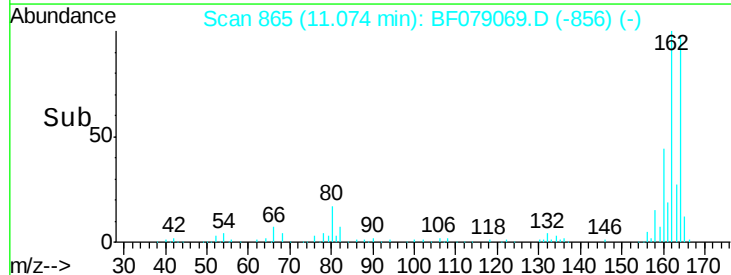
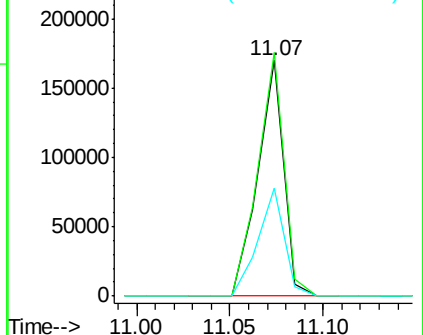




#41
 2,4,6-Tribromophenol
 Concen: 76.62 ng
 RT: 12.06 min Scan# 951
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04




Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-13-5.0


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	0.0	0.0#
141	32.8	0.0	0.0#

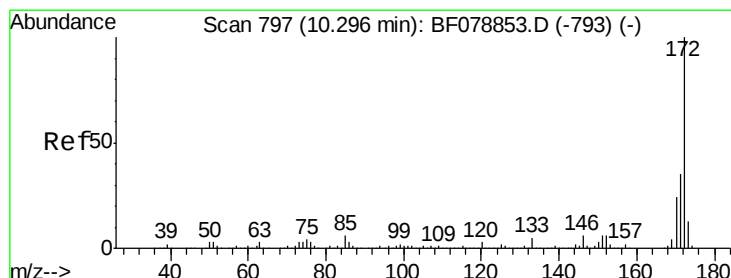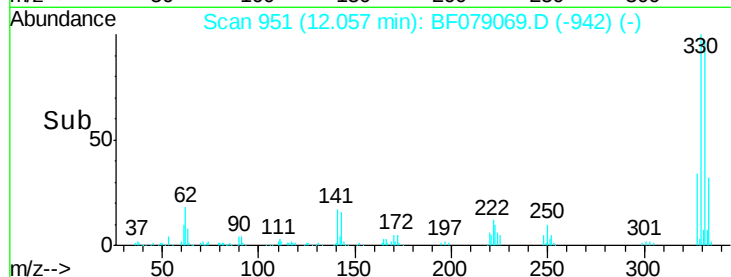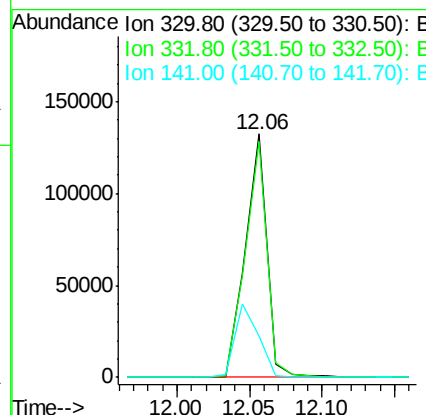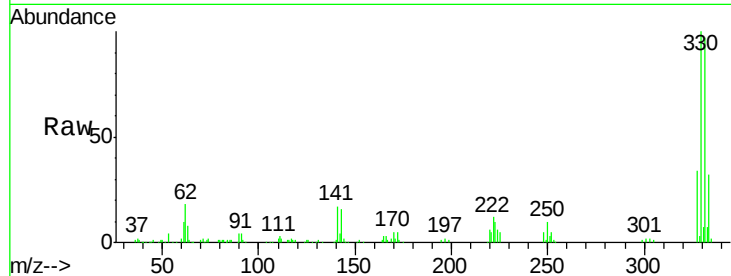

#44
 2-Fluorobiphenyl
 Concen: 44.64 ng
 RT: 10.24 min Scan# 792
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	27.9	41.9
170	24.0	19.4	29.0

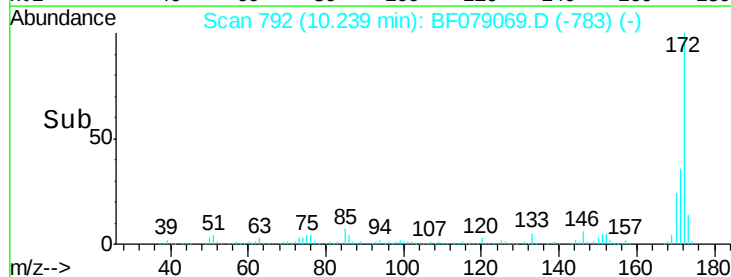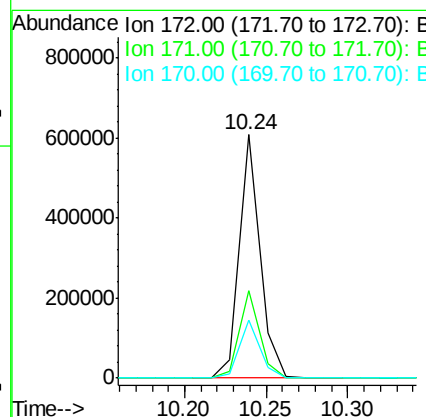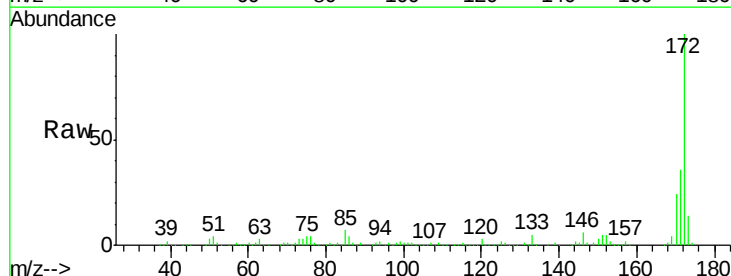


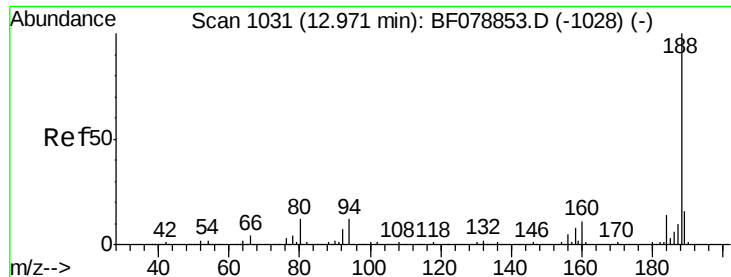




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.91 min Scan# 1026
Delta R.T. -0.00 min
Lab File: BF079069.D
Acq: 9 May 2015 8:04

Instrument :
BNA_F
ClientSampleId :
TU021-SB-13-5.0

Tot Ion:188 Resp: 312592
Ion Ratio Lower Upper
188 100
94 12.6 8.2 12.2#
80 13.3 8.9 13.3

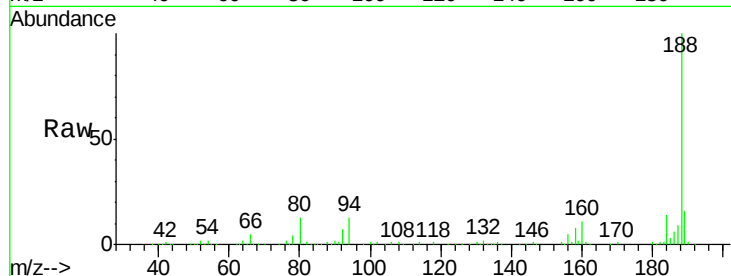


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

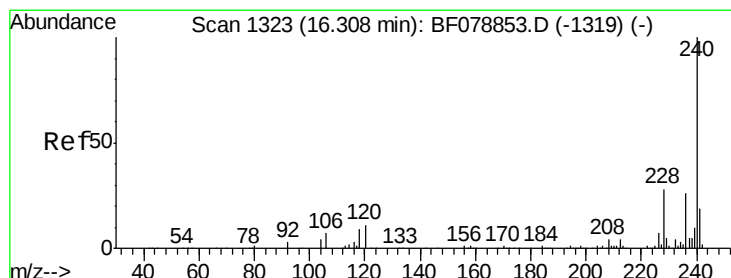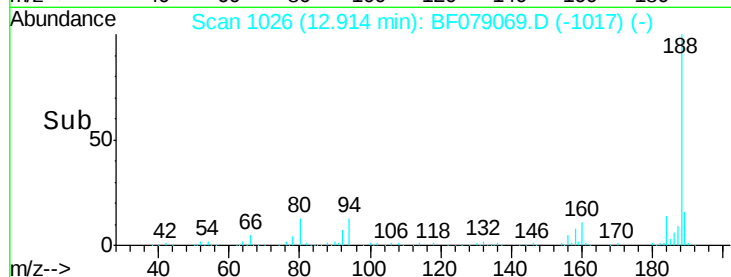
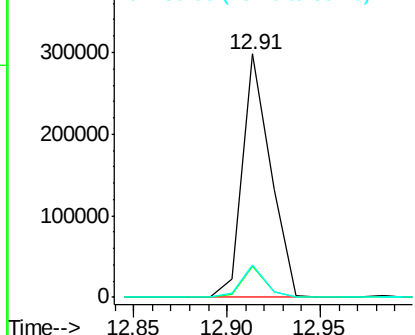


#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.22 min Scan# 1315
Delta R.T. -0.00 min
Lab File: BF079069.D
Acq: 9 May 2015 8:04

Tgt Ion:240 Resp: 306251
Ion Ratio Lower Upper
240 100
120 9.5 9.7 14.5#
236 25.9 20.2 30.4

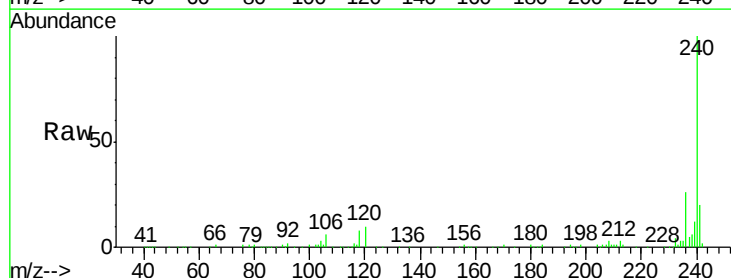

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



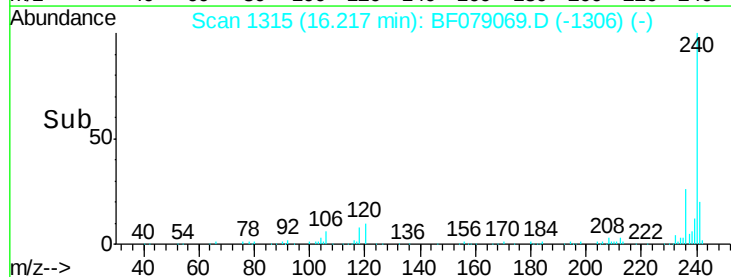
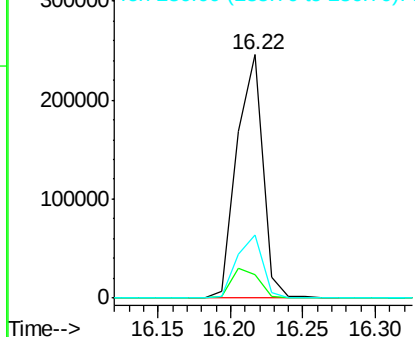




#78
 Terphenyl-d14
 Concen: 47.14 ng
 RT: 14.91 min Scan# 1201
 Delta R.T. -0.00 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-13-5.0

Tot Ion:244 Resp: 603031
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.6 8.4
 122 10.4 10.3 15.5

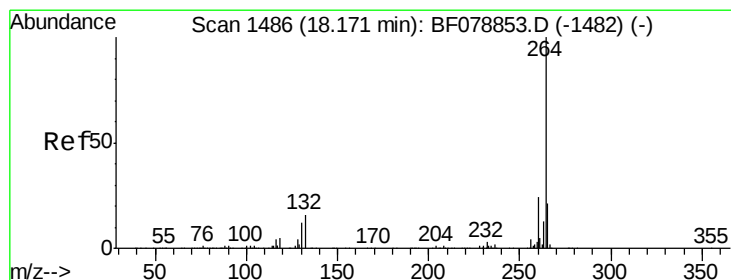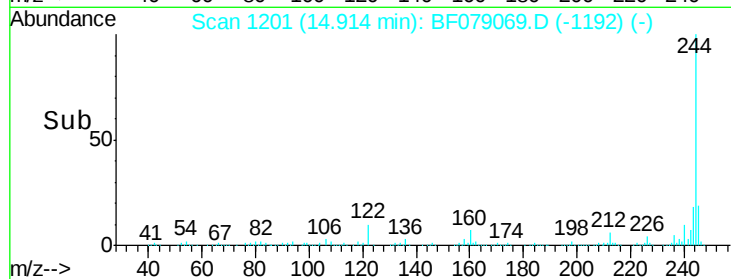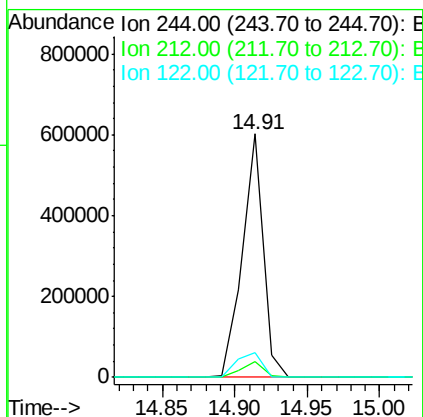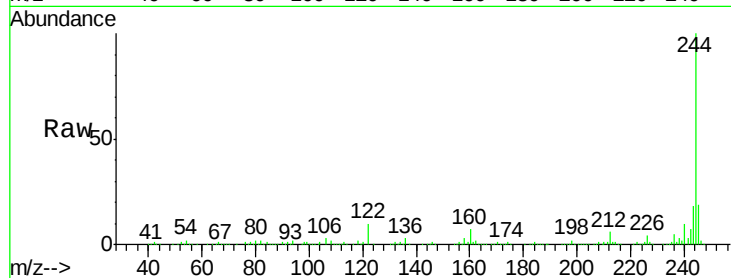

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.98 min Scan# 1469
 Delta R.T. 0.05 min
 Lab File: BF079069.D
 Acq: 9 May 2015 8:04

Tgt Ion:264 Resp: 301135
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.4 29.2
 265 21.7 18.3 27.5

