

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
 Data File : BF079038.D
 Acq On : 8 May 2015 15:24
 Operator : TP/IZ
 Sample : PB83243BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83243BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.507	25	28	31	rVB	7510073	9994079	100.00%	28.475%
2	1.747	47	49	59	rBV	939967	1520757	15.22%	4.333%
3	1.873	59	60	92	rVB	2340588	4606352	46.09%	13.124%
4	5.130	343	345	352	rBV	97183	118551	1.19%	0.338%
5	5.633	386	389	391	rBV	1422176	1933244	19.34%	5.508%
6	6.879	496	498	501	rBV	1432857	1912546	19.14%	5.449%
7	7.039	509	512	514	rBV	1678257	2039158	20.40%	5.810%
8	7.325	535	537	539	rVB	407382	410068	4.10%	1.168%
9	7.508	550	553	556	rBV	1754095	1560402	15.61%	4.446%
10	8.010	595	597	600	rBV	1238460	1155897	11.57%	3.293%
11	8.902	672	675	677	rBV	543646	567144	5.67%	1.616%
12	10.251	790	793	795	rBV	1814547	2366945	23.68%	6.744%
13	11.074	863	865	868	rVB	641385	616421	6.17%	1.756%
14	12.057	948	951	954	rBV	1579984	1523185	15.24%	4.340%
15	12.925	1024	1027	1029	rBV	654247	648316	6.49%	1.847%
16	14.925	1199	1202	1204	rBV	2677434	2752877	27.55%	7.843%
17	16.263	1316	1319	1322	rBV	632961	690935	6.91%	1.969%
18	18.149	1481	1484	1487	rBV	524368	680926	6.81%	1.940%


Sum of corrected areas: 35097803

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079038.D
Acq On : 8 May 2015 15:24
Operator : TP/IZ
Sample : PB83243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83243BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

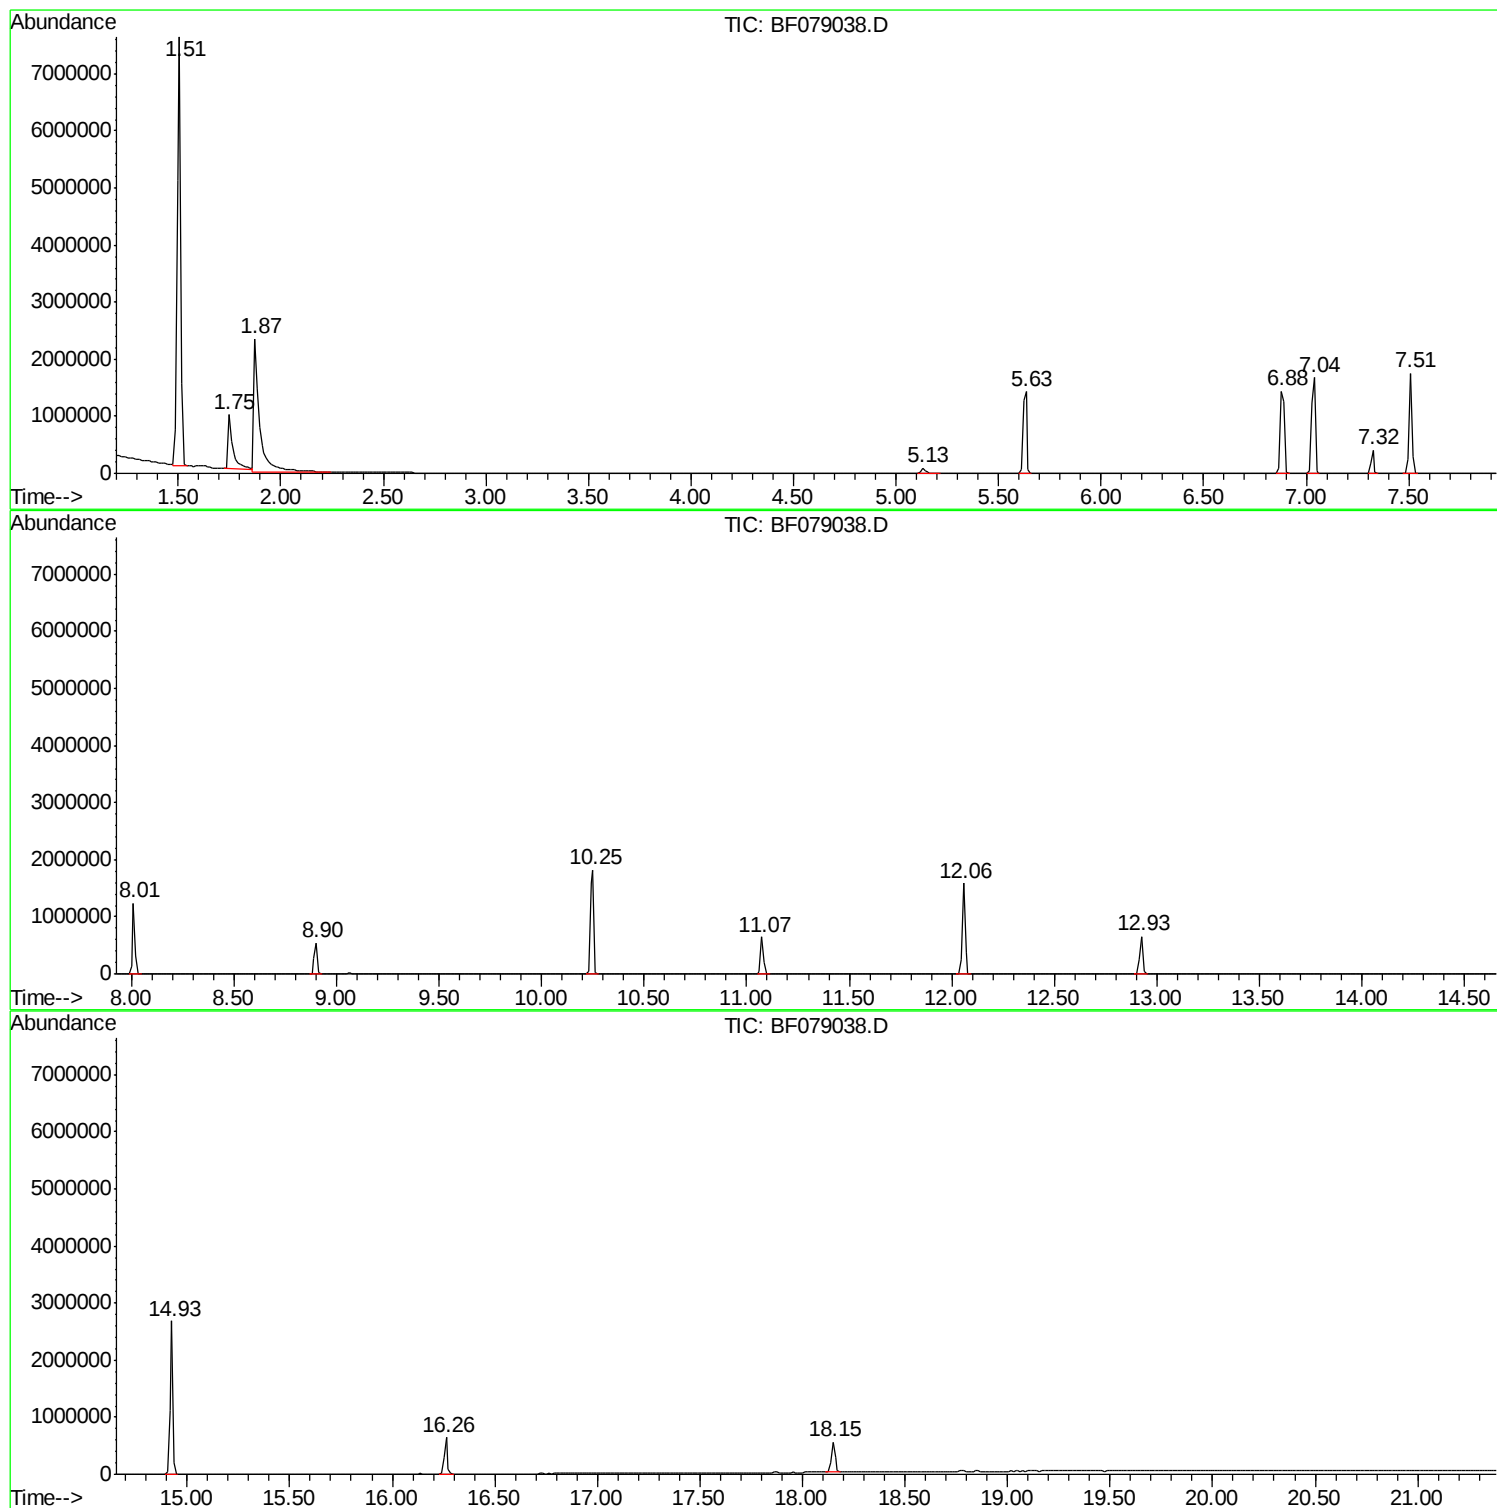

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079038.D
Acq On : 8 May 2015 15:24
Operator : TP/IZ
Sample : PB83243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83243BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.51	487.44 ng	9994080	1,4-Dichlorobenzene-d4	7.32

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	56
2		1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	9
3		N-Ethylformamide	73	C3H7NO	000627-45-2	9
4		1,3-Diaminoquanidine	89	CH7N5	004364-78-7	9
5		1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9

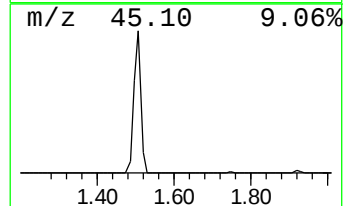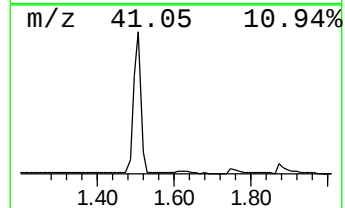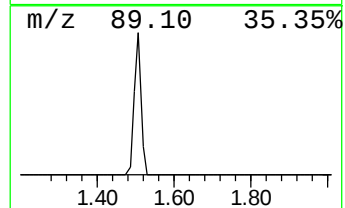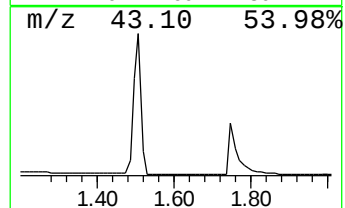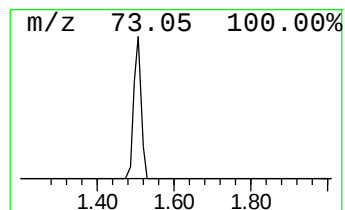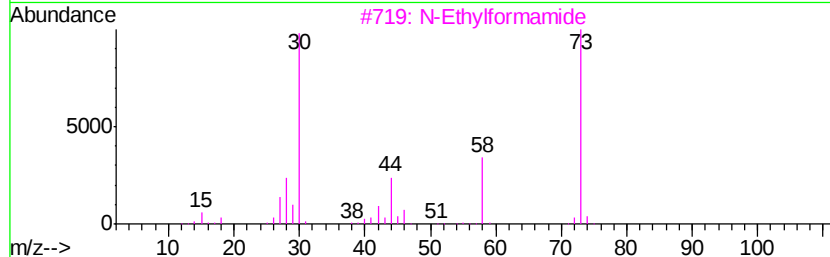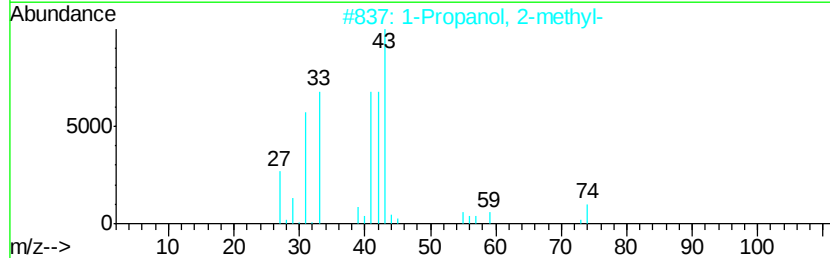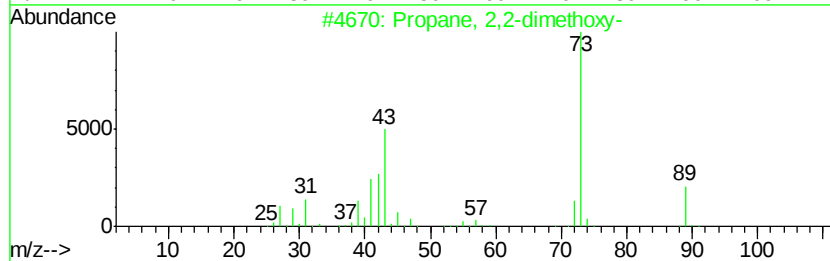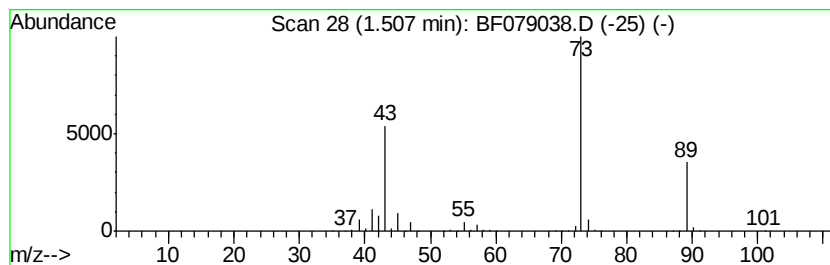

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079038.D
Acq On : 8 May 2015 15:24
Operator : TP/IZ
Sample : PB83243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83243BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.13	5.78 ng	118551	1,4-Dichlorobenzene-d4	7.32

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42
2			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4			2-Propanone, 1-(1-methylethoxy)-	116	C6H12O2	042781-12-4	9
5			5-Oxohexanenitrile	111	C6H9NO	010412-98-3	9

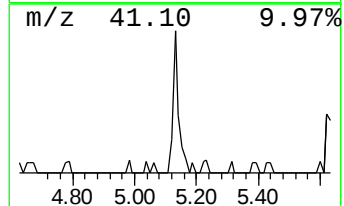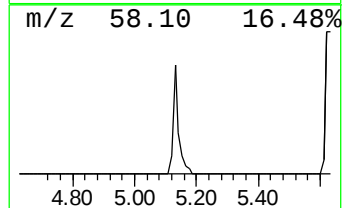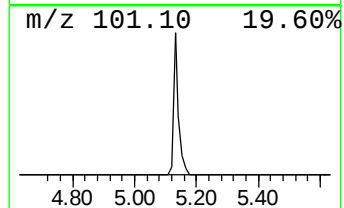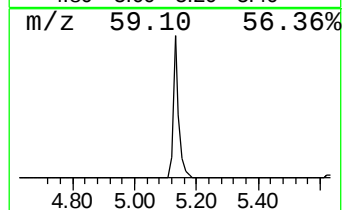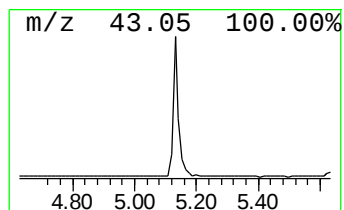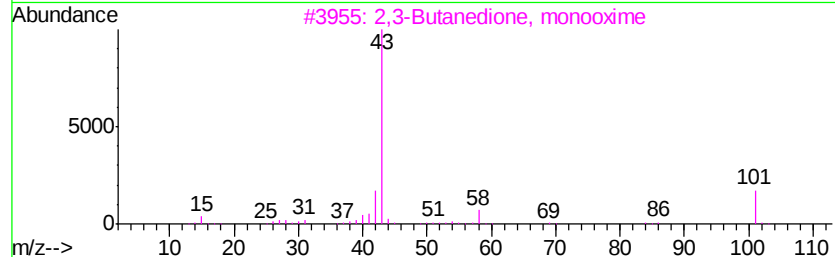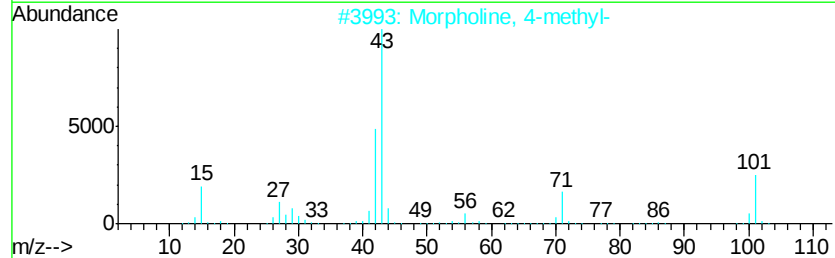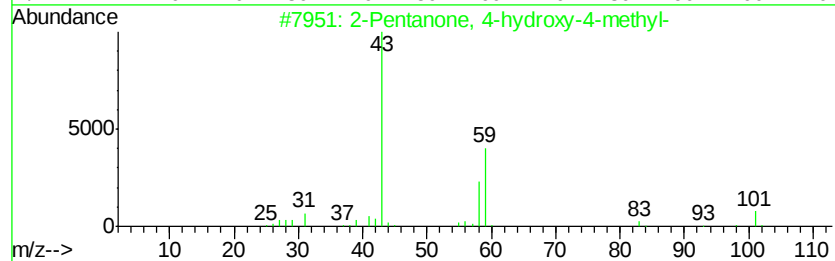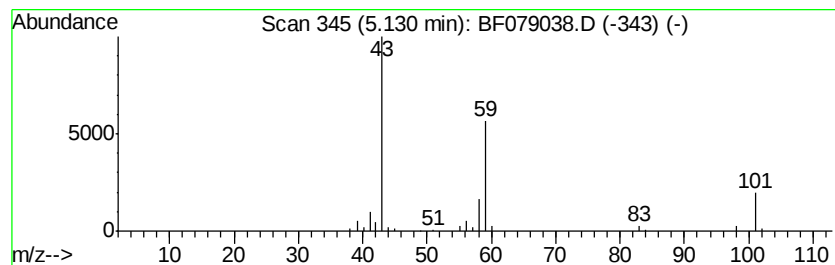

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050815\
Data File : BF079038.D
Acq On : 8 May 2015 15:24
Operator : TP/IZ
Sample : PB83243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83243BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown7.04 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	99.45 ng	2039160	1,4-Dichlorobenzene-d4	7.32

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3		Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4			Amphetaminil	250	C17H18N2	017590-01-1	12
5			5-Aminoindole	132	C8H8N2	005192-03-0	12

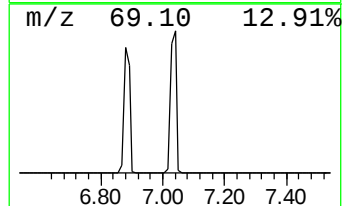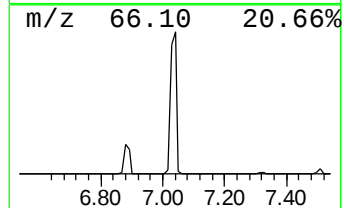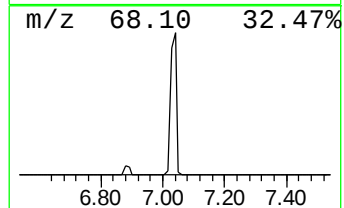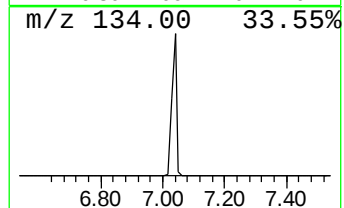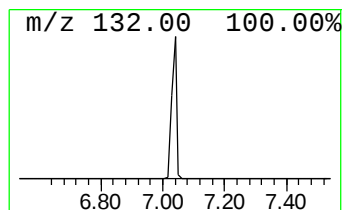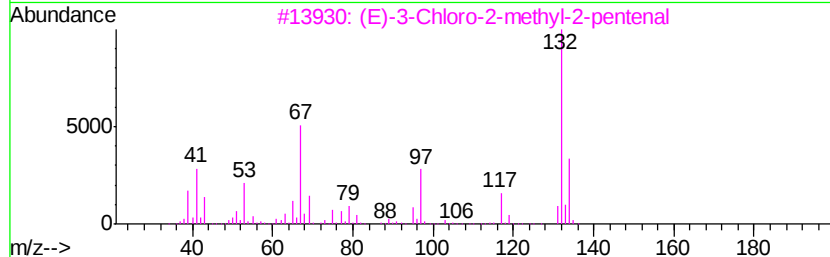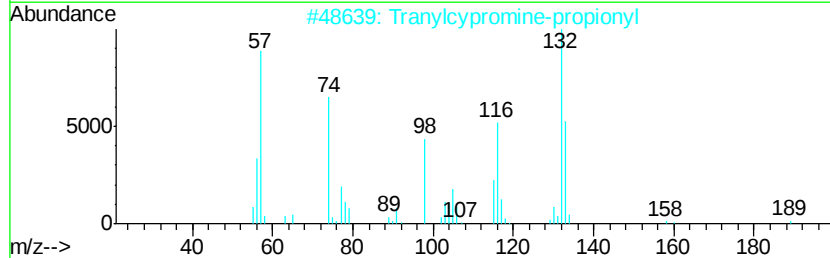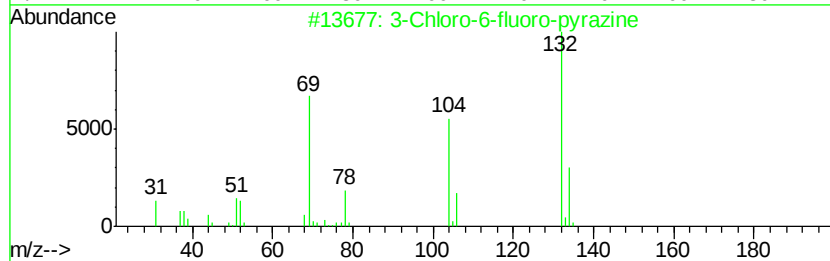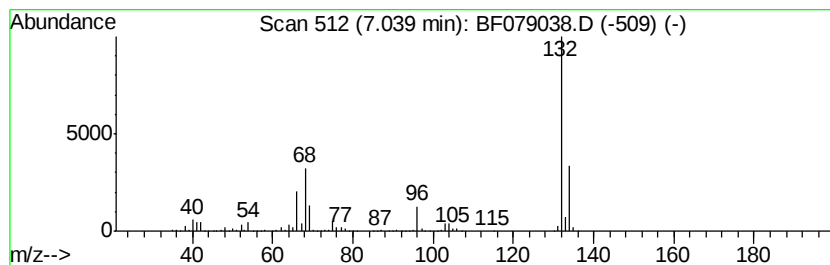

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079038.D
Acq On : 8 May 2015 15:24
Operator : TP/IZ
Sample : PB83243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83243BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-dime...	1.51	487.4	ng	9994080	1	7.32	410068	20.0
2-Pentanone, 4-hy...	5.13	5.8	ng	118551	1	7.32	410068	20.0
unknown7.04	7.04	99.5	ng	2039160	1	7.32	410068	20.0