

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
 Data File : BF079052.D
 Acq On : 8 May 2015 22:05
 Operator : TP/IZ
 Sample : PB83250BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83250BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.507	25	28	31	rVB	6907311	9323392	100.00%	29.786%
2	1.747	47	49	58	rBV	819687	1329852	14.26%	4.249%
3	1.873	58	60	97	rVB	1974941	3774471	40.48%	12.059%
4	5.622	386	388	391	rBV	1471505	1601442	17.18%	5.116%
5	6.879	496	498	500	rBV	1835972	1602430	17.19%	5.119%
6	7.027	509	511	514	rBV	1471546	1682371	18.04%	5.375%
7	7.325	534	537	539	rVB	380969	464941	4.99%	1.485%
8	7.508	551	553	555	rVB	1500139	1332704	14.29%	4.258%
9	8.010	594	597	599	rBV	1174871	1016493	10.90%	3.247%
10	8.891	672	674	677	rBV	474290	639577	6.86%	2.043%
11	10.239	790	792	795	rBV	2041496	1941677	20.83%	6.203%
12	11.074	862	865	868	rVB	772071	730942	7.84%	2.335%
13	12.057	948	951	953	rBV	1120959	1285130	13.78%	4.106%
14	12.914	1024	1026	1029	rBV2	652203	762814	8.18%	2.437%
15	14.914	1198	1201	1204	rBV	2298066	2253362	24.17%	7.199%
16	16.217	1312	1315	1317	rBV	751454	788047	8.45%	2.518%
17	17.977	1466	1469	1472	rBV	544619	771267	8.27%	2.464%




Sum of corrected areas: 31300912

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050815\
Data File : BF079052.D
Acq On : 8 May 2015 22:05
Operator : TP/IZ
Sample : PB83250BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83250BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

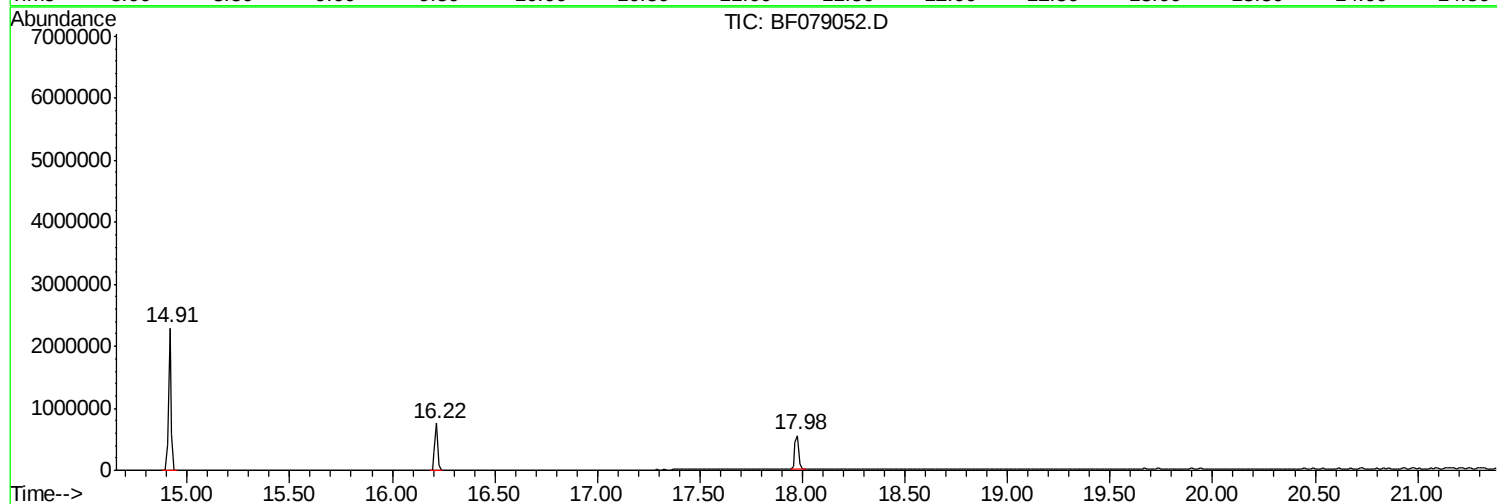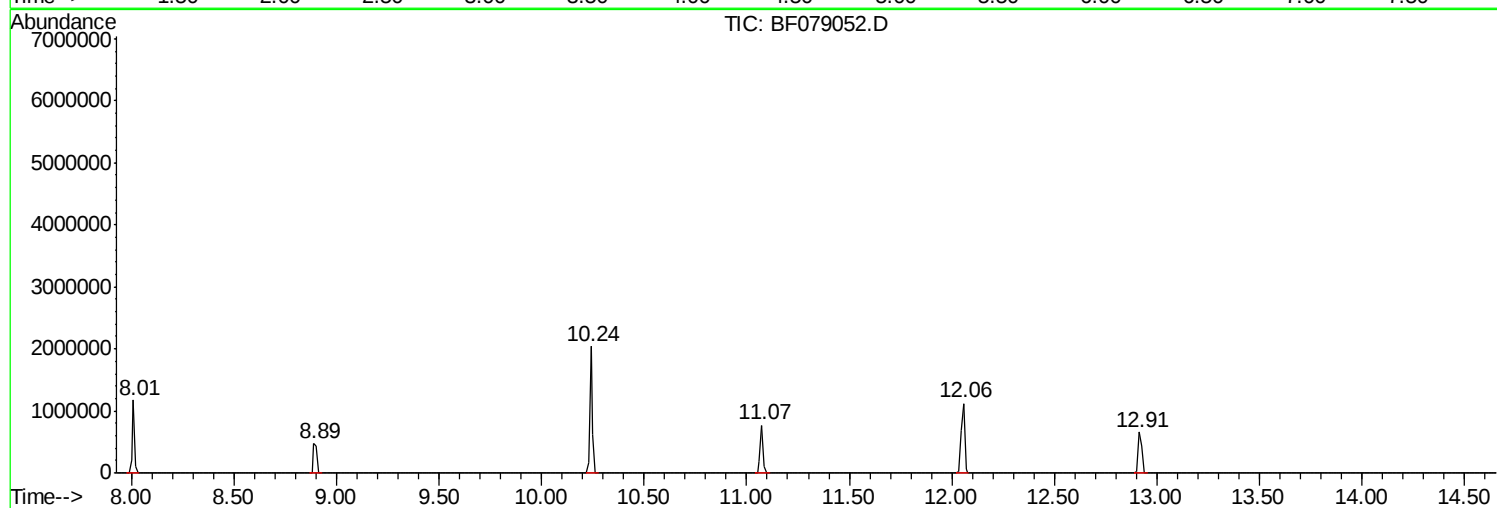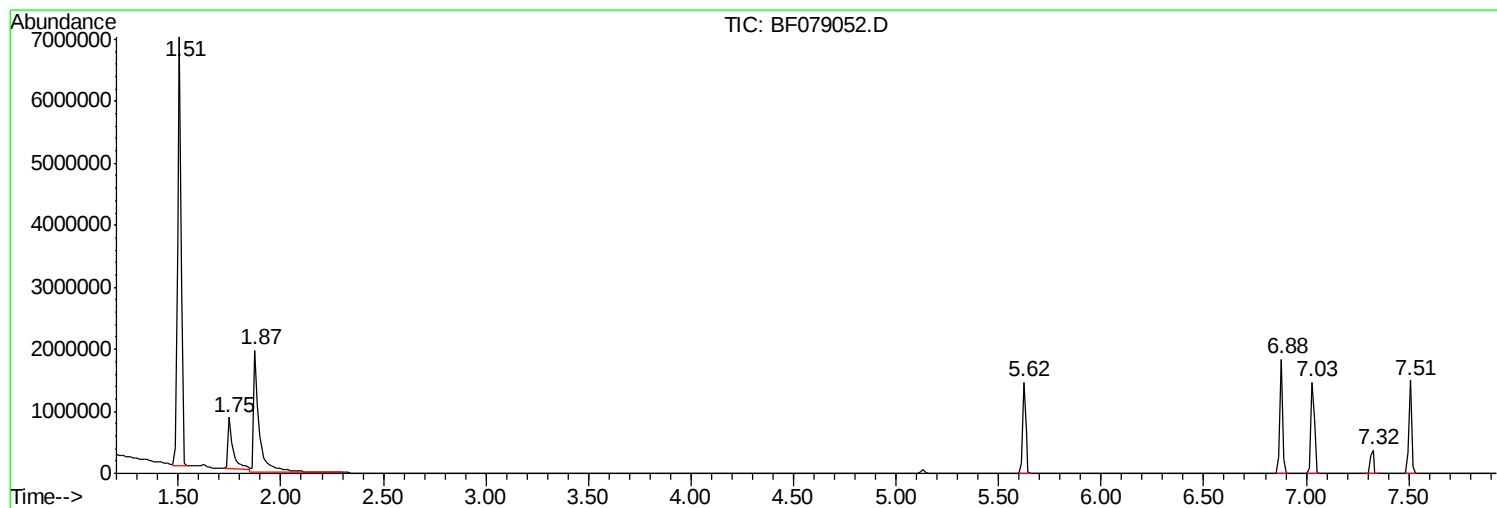

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079052.D
Acq On : 8 May 2015 22:05
Operator : TP/IZ
Sample : PB83250BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83250BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.51	401.06 ng	9323390	1,4-Dichlorobenzene-d4	7.32

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	56
2			N-Ethylformamide	73	C3H7NO	000627-45-2	9
3			1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	9
4			1,3-Diaminoquanidine	89	CH7N5	004364-78-7	9
5			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9

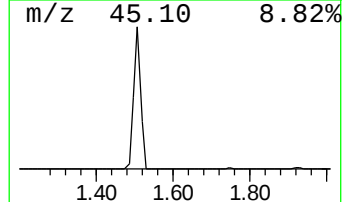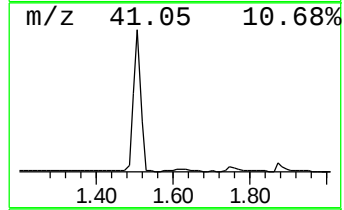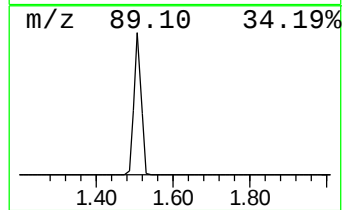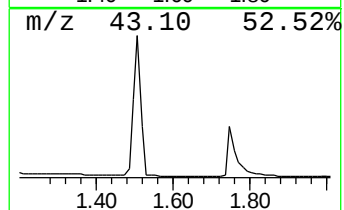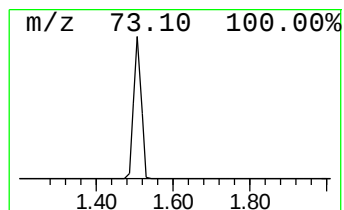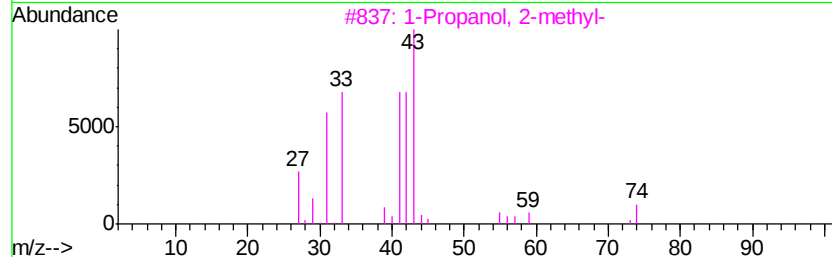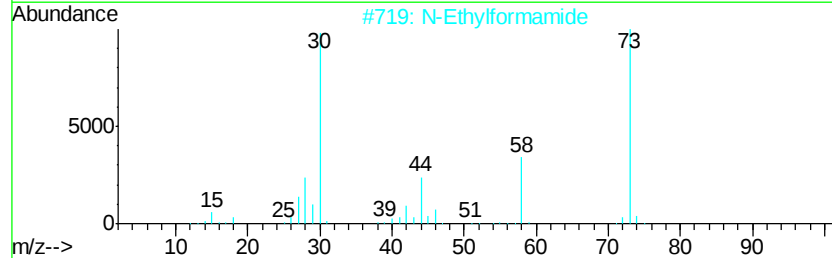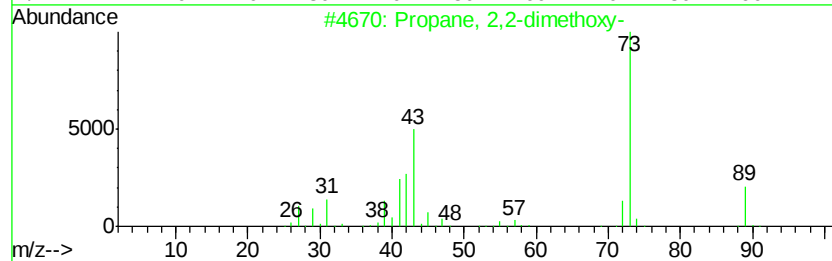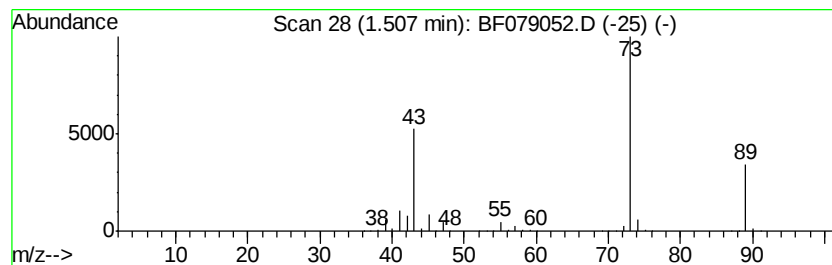

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079052.D
Acq On : 8 May 2015 22:05
Operator : TP/IZ
Sample : PB83250BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83250BL









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.03 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	72.37 ng	1682370	1,4-Dichlorobenzene-d4	7.32

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

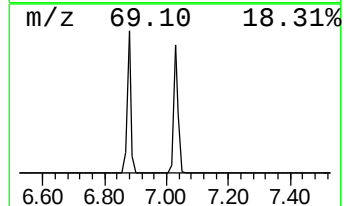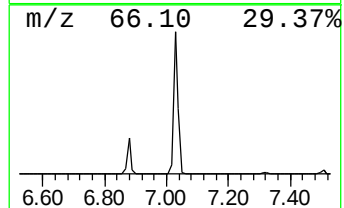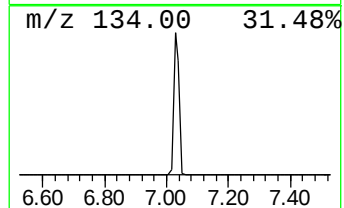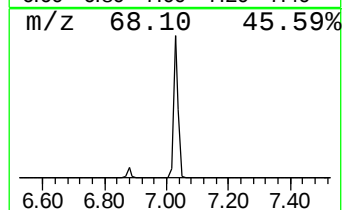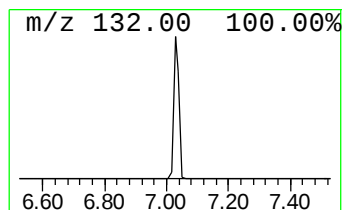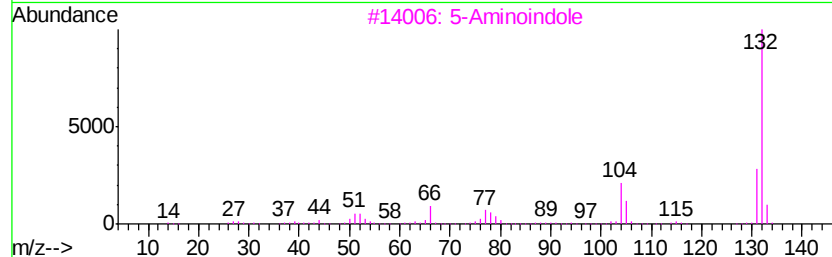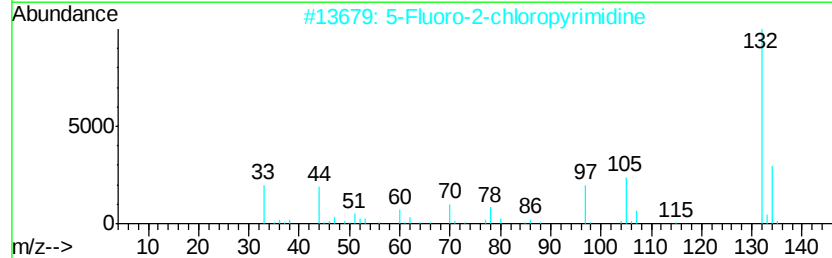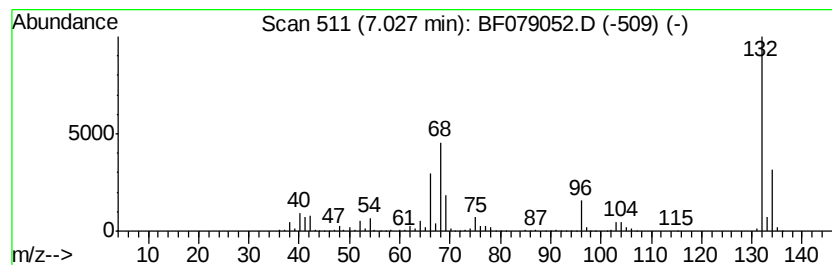

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050815\
Data File : BF079052.D
Acq On : 8 May 2015 22:05
Operator : TP/IZ
Sample : PB83250BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83250BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-dime...	1.51	401.1	ng	9323390	1	7.32	464941	20.0
unknown7.03	7.03	72.4	ng	1682370	1	7.32	464941	20.0