


Data Path : Z:\HPCHEM1\BNA F\Data\BF050815\
 Data File : BF079036.D
 Acq On : 8 May 2015 14:14
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

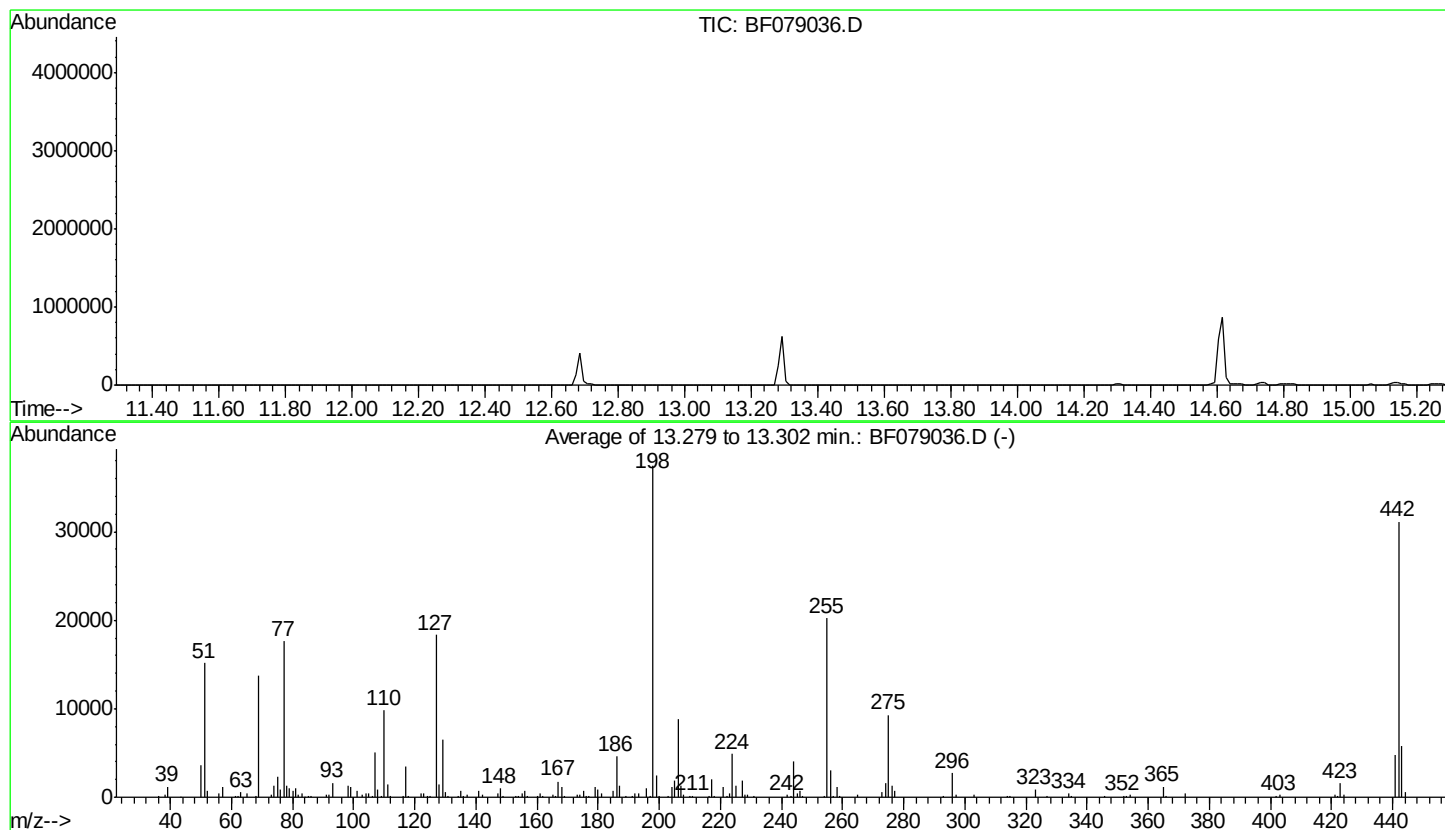

AutoFind: Scans 1058, 1059, 1060; Background Corrected with Scan 1055

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	15172	PASS
68	69	0.00	2	1.6	214	PASS
69	198	0.00	100	36.8	13774	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	18339	PASS
197	198	0.00	2	0.4	166	PASS
198	198	100	100	100.0	37450	PASS
199	198	5	9	6.6	2466	PASS
275	198	10	60	24.7	9261	PASS
365	198	1	100	3.1	1172	PASS
441	442	0.01	24	15.6	4840	PASS
442	198	50	100	83.0	31095	PASS
443	442	15	24	18.6	5770	PASS