


Data Path : Z:\HPCHEM1\BNA F\Data\BF050815\
 Data File : BF079060.D
 Acq On : 9 May 2015 3:18
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

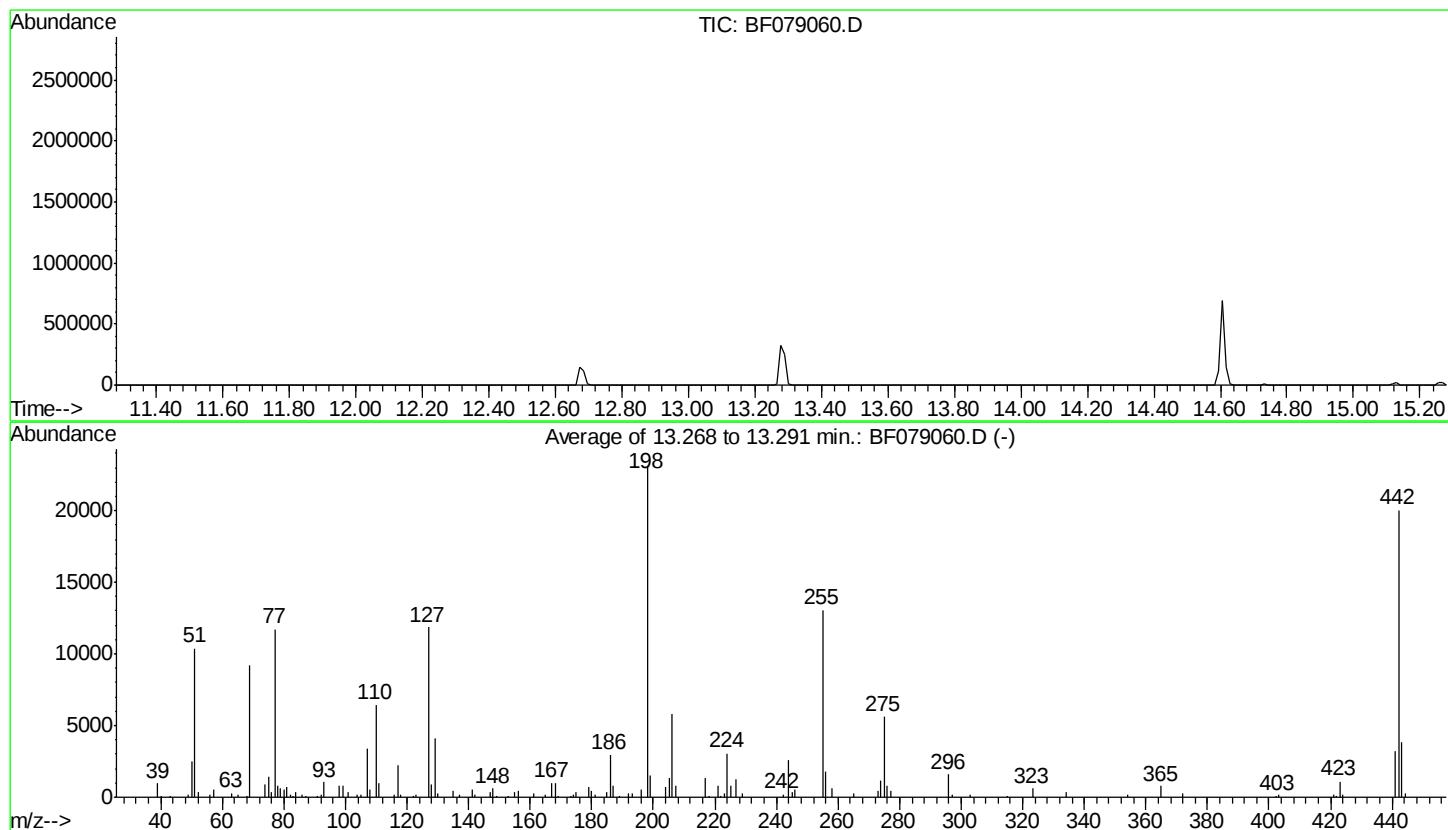

AutoFind: Scans 1057, 1058, 1059; Background Corrected with Scan 1054

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	10395	PASS
68	69	0.00	2	1.4	125	PASS
69	198	0.00	100	39.7	9190	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	11841	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23138	PASS
199	198	5	9	6.7	1543	PASS
275	198	10	60	24.2	5607	PASS
365	198	1	100	3.4	788	PASS
441	442	0.01	24	16.0	3206	PASS
442	198	50	100	86.5	20012	PASS
443	442	15	24	19.1	3820	PASS