
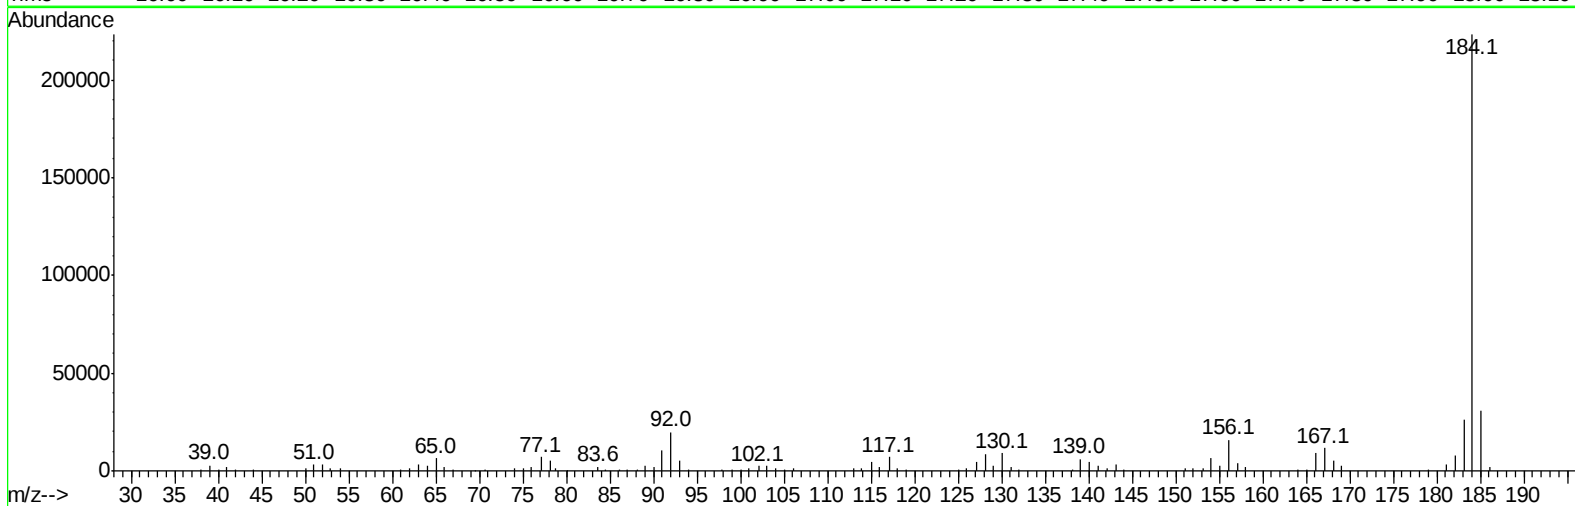


Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
Data File : BF094977.D
Acq On : 8 May 2017 11:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 12:59:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

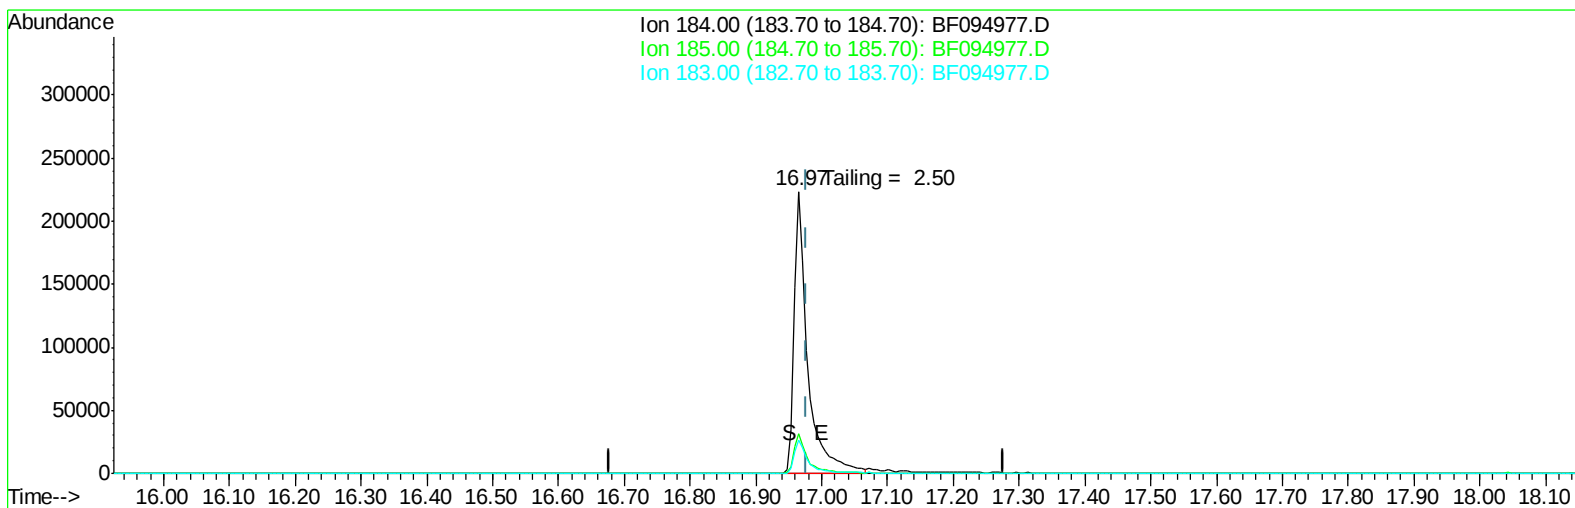

TIC: BF094977.D

(76) Benzidine



16.965min (-0.012) 0.00ng

response 333611

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.88#
183.00	12.20	11.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
Data File : BF094977.D
Acq On : 8 May 2017 11:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 12:59:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

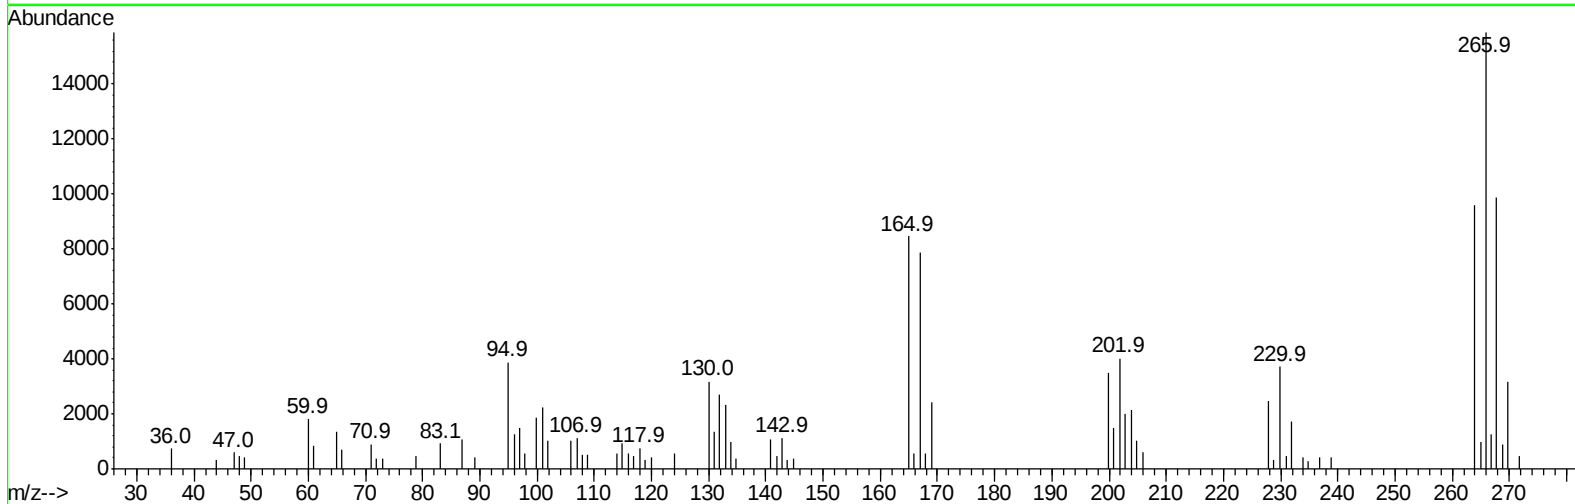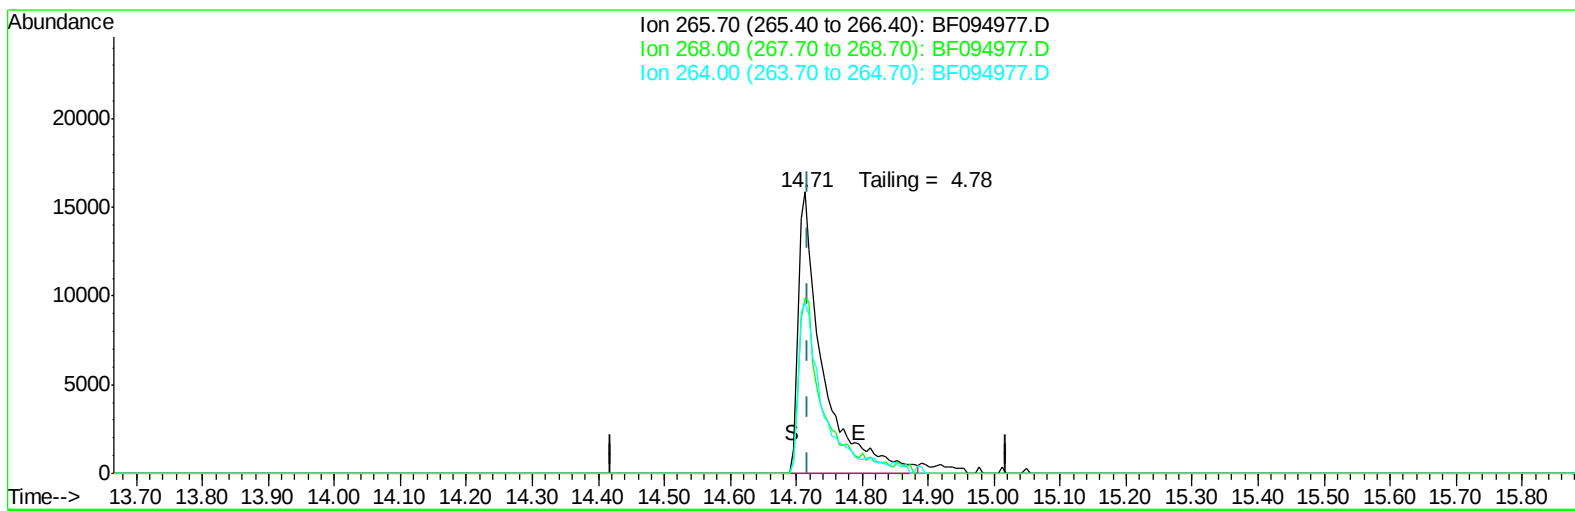

TIC: BF094977.D

(69) Pentachlorophenol (C)

14.712min (-0.006) 0.00ng

response 41519

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.12
264.00	64.60	60.33
0.00	0.00	0.00