
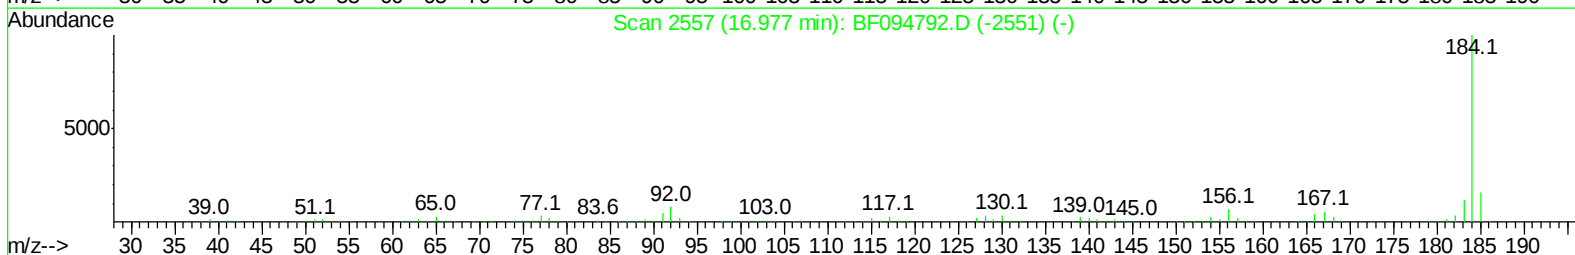
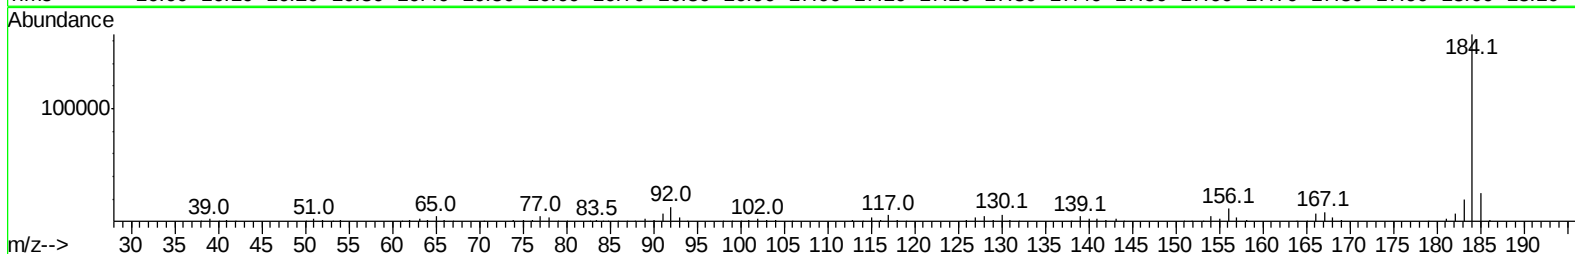


Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
Data File : BF094982.D
Acq On : 8 May 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 17:54:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

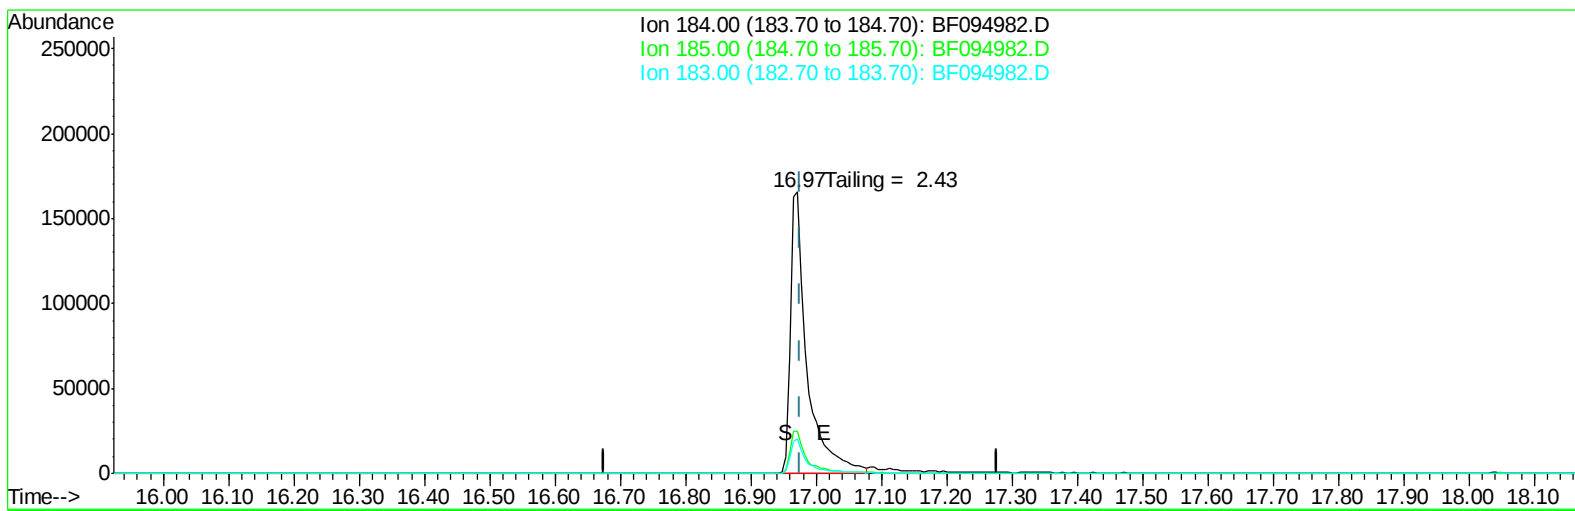

TIC: BF094982.D

(76) Benzidine




16.971min (-0.006) 0.00ng

response 302571

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.08#
183.00	12.20	12.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
Data File : BF094982.D
Acq On : 8 May 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 17:54:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

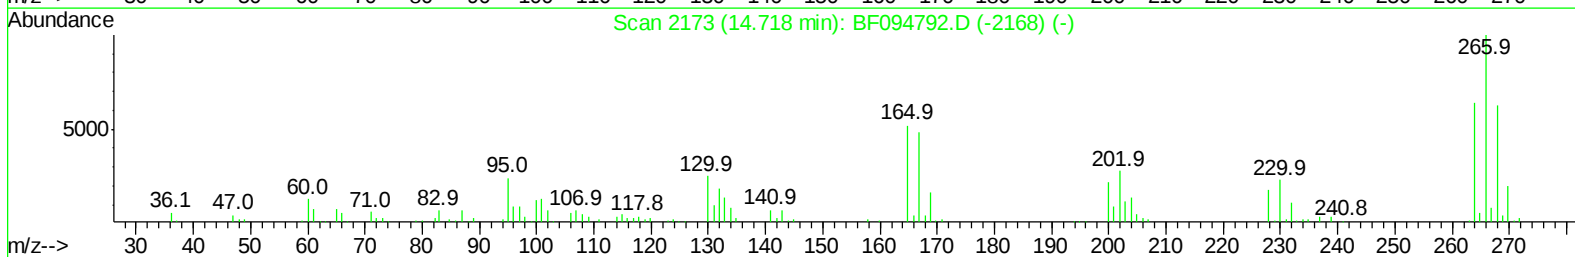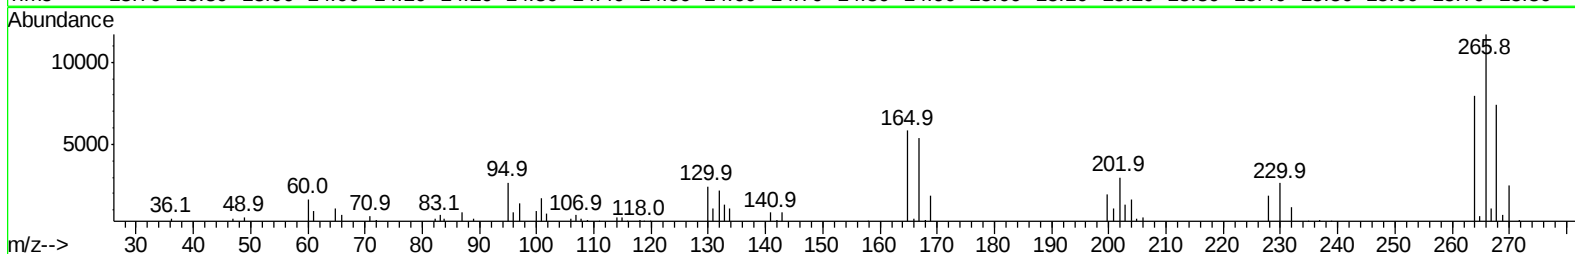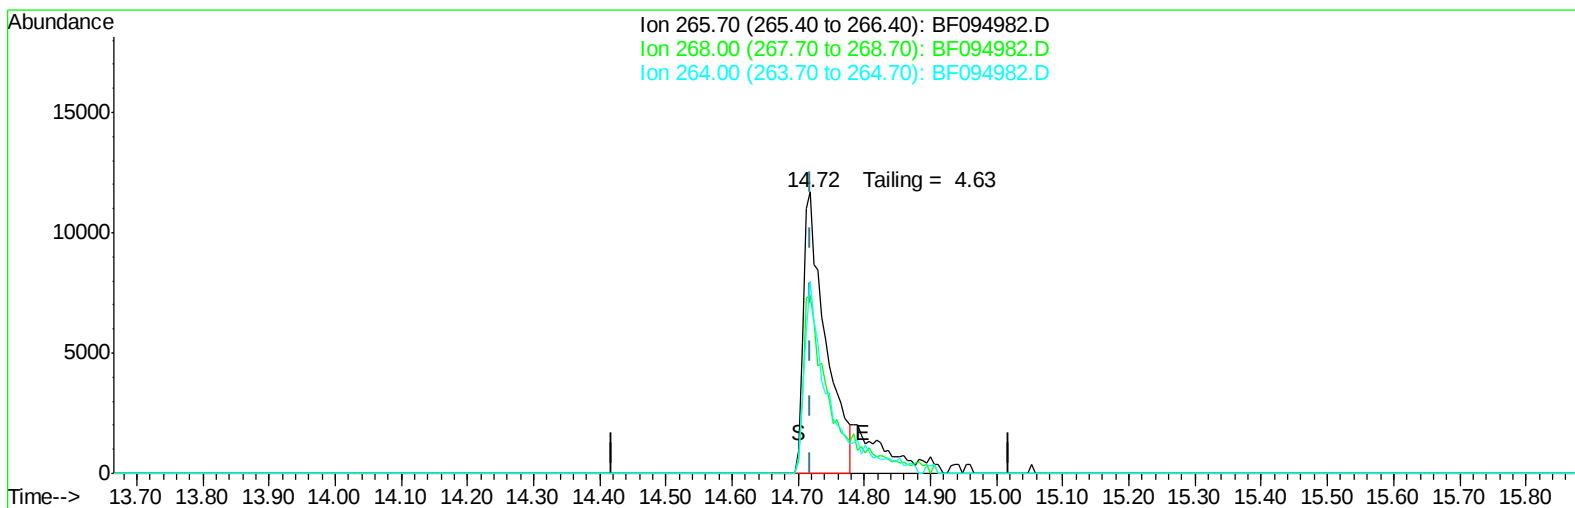

TIC: BF094982.D

(69) Pentachlorophenol (C)

14.718min (-0.000) 0.00ng

response 33659

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.40
264.00	64.60	68.31
0.00	0.00	0.00