
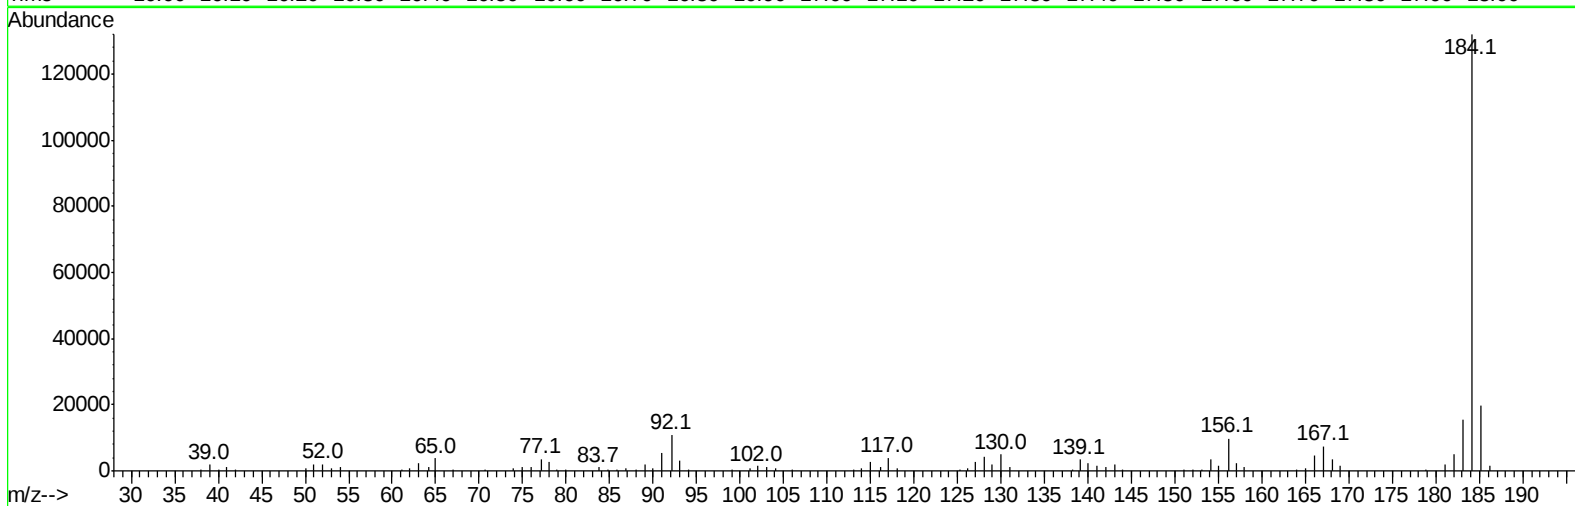


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050817\
Data File : BF095005.D
Acq On : 9 May 2017 5:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 09:20:55 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

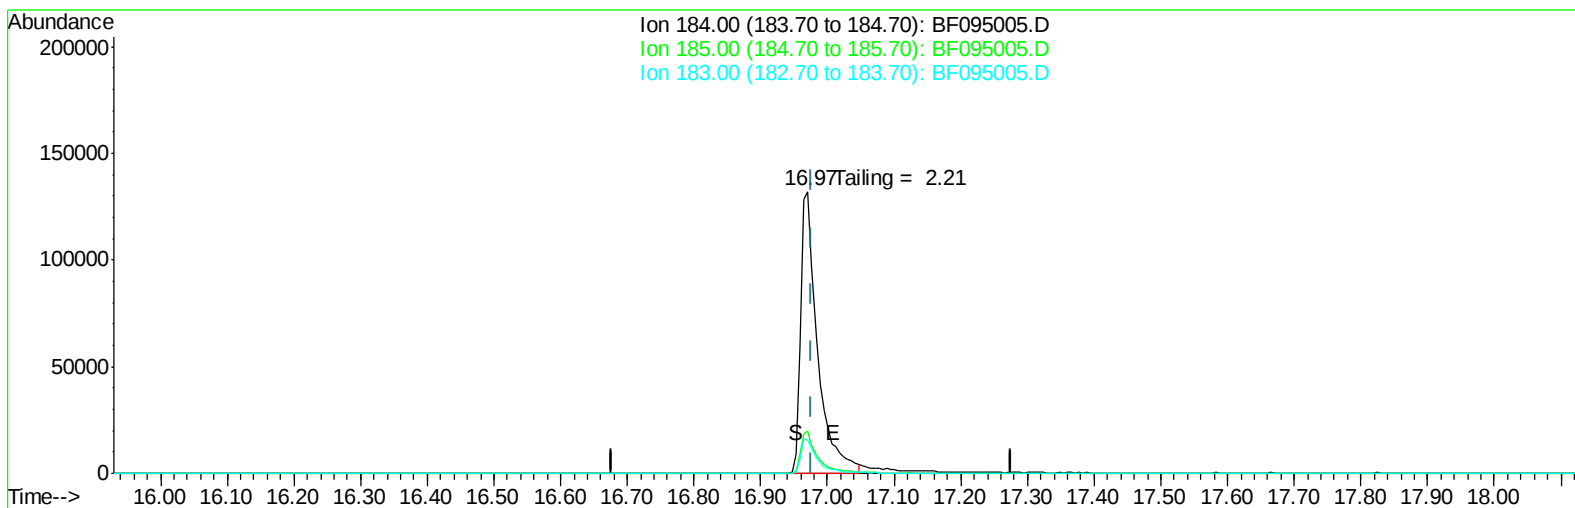

TIC: BF095005.D

(76) Benzidine



16.971min (-0.006) 0.00ng

response 237625

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.95#
183.00	12.20	11.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050817\
Data File : BF095005.D
Acq On : 9 May 2017 5:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 09:20:55 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

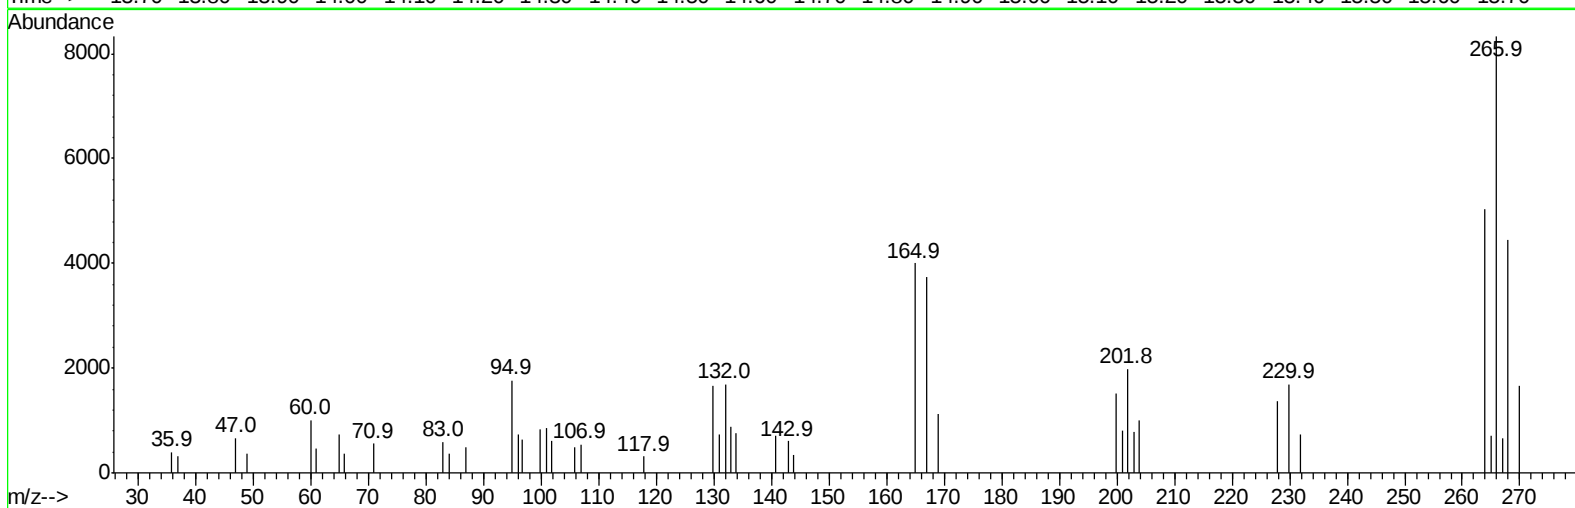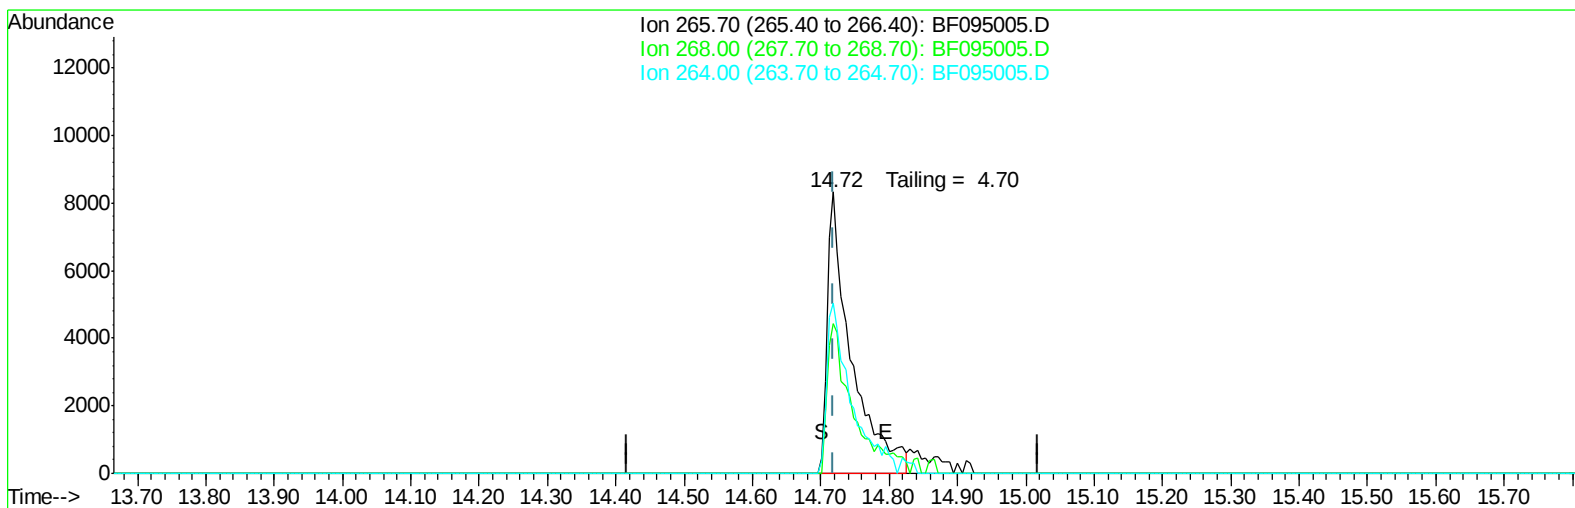

TIC: BF095005.D

(69) Pentachlorophenol (C)

14.718min (-0.000) 0.00ng

response 19452

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	53.26
264.00	64.60	60.37
0.00	0.00	0.00