


Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
 Data File : BF094977.D
 Acq On : 8 May 2017 11:52
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

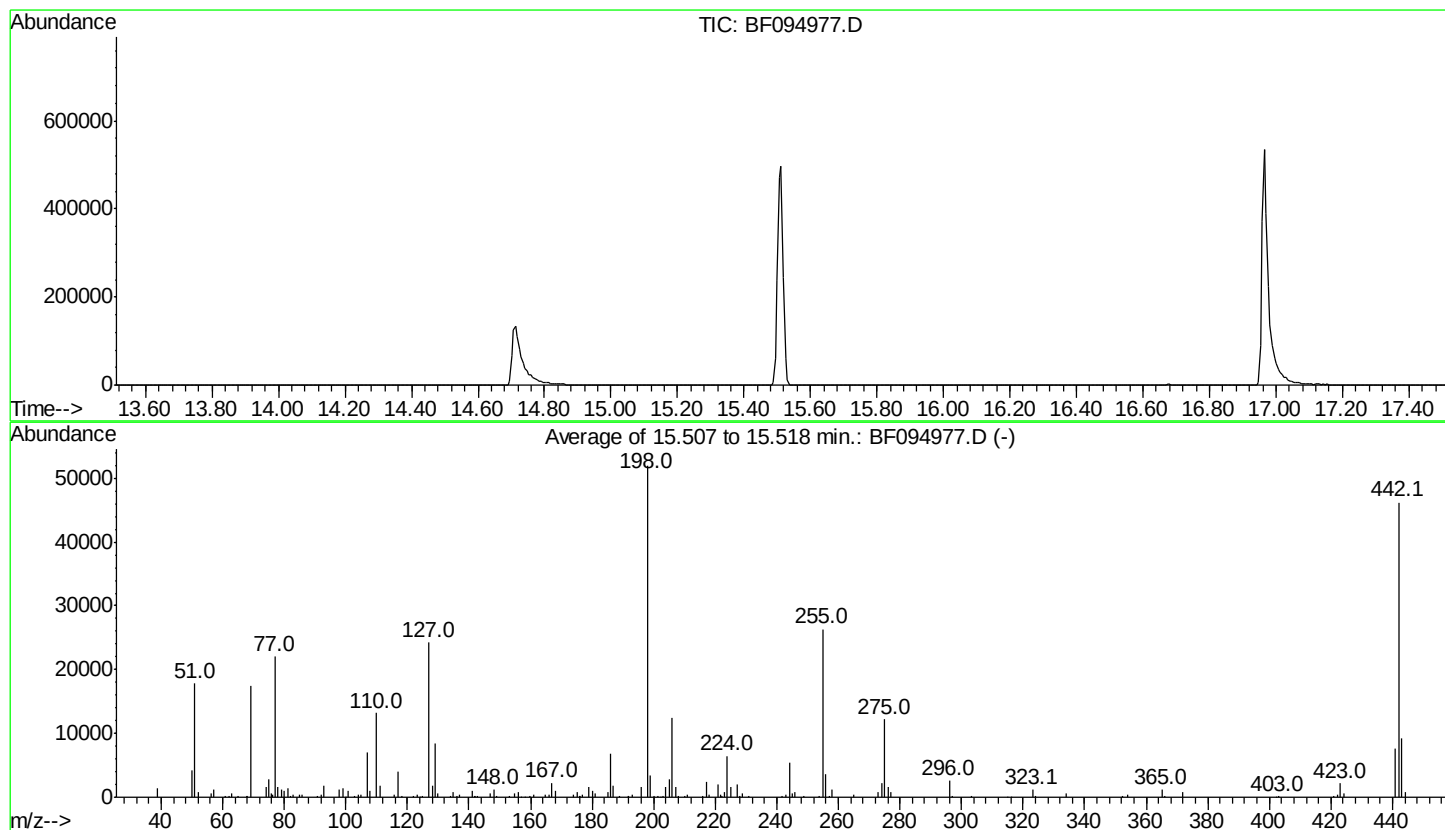

AutoFind: Scans 2307, 2308, 2309; Background Corrected with Scan 2301

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	17825	PASS
68	69	0.00	2	0.9	159	PASS
69	198	0.00	100	33.7	17531	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	24227	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51965	PASS
199	198	5	9	6.8	3512	PASS
275	198	10	60	23.4	12181	PASS
365	198	1	100	2.2	1164	PASS
441	442	0.01	24	16.5	7618	PASS
442	198	50	100	88.9	46194	PASS
443	442	15	24	20.0	9247	PASS