


Data Path : Z:\HPCHEM1\BNA F\Data\BF050817\
 Data File : BF095005.D
 Acq On : 9 May 2017 5:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

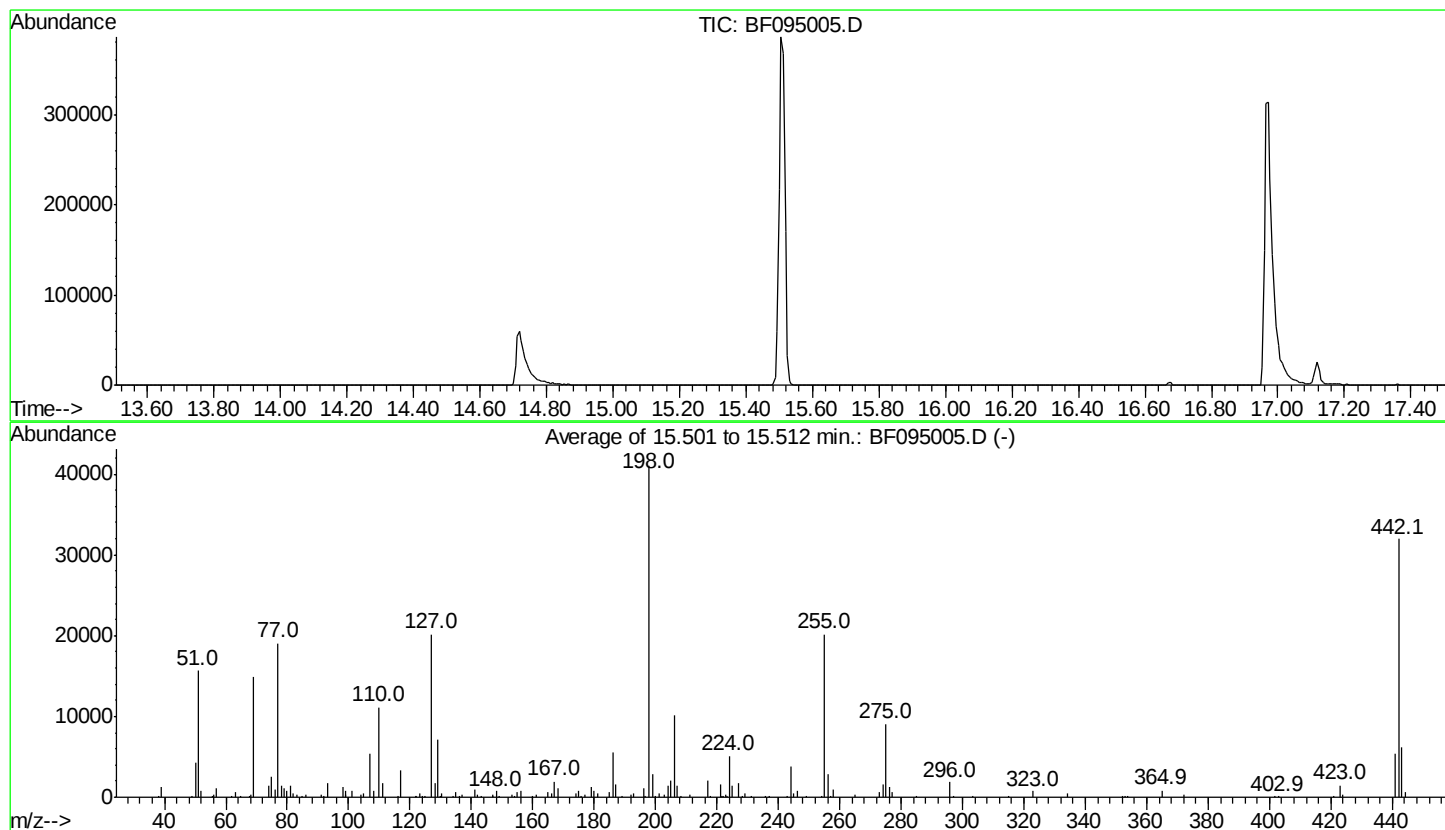

AutoFind: Scans 2306, 2307, 2308; Background Corrected with Scan 2301

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	15669	PASS
68	69	0.00	2	1.7	247	PASS
69	198	0.00	100	36.3	14898	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.2	20174	PASS
197	198	0.00	2	0.4	150	PASS
198	198	100	100	100.0	41034	PASS
199	198	5	9	6.9	2838	PASS
275	198	10	60	22.1	9078	PASS
365	198	1	100	2.1	868	PASS
441	442	0.01	24	16.7	5348	PASS
442	198	50	100	77.9	31947	PASS
443	442	15	24	19.5	6223	PASS