
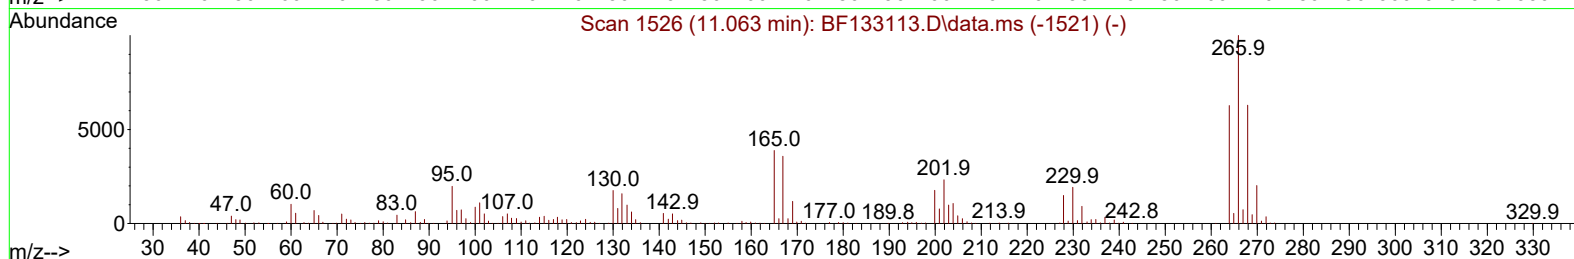
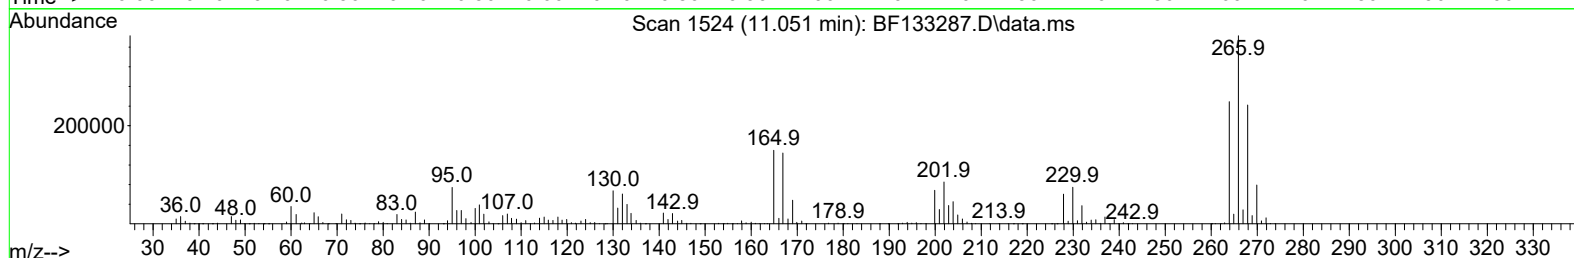


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133287.D
Acq On : 08 May 2023 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 06:50:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

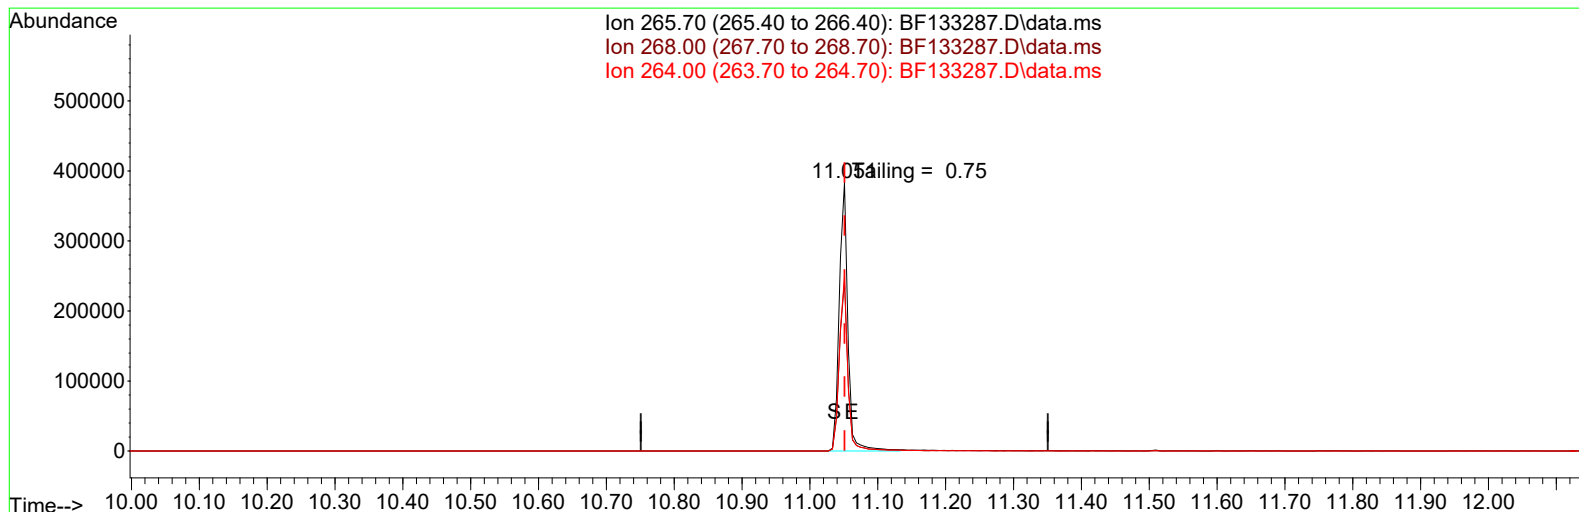

TIC: BF133287.D\data.ms

(70) Pentachlorophenol (C)




11.051min (0.000) 283401.45 ng

response 338705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.15
264.00	63.30	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133287.D
Acq On : 08 May 2023 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 06:50:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

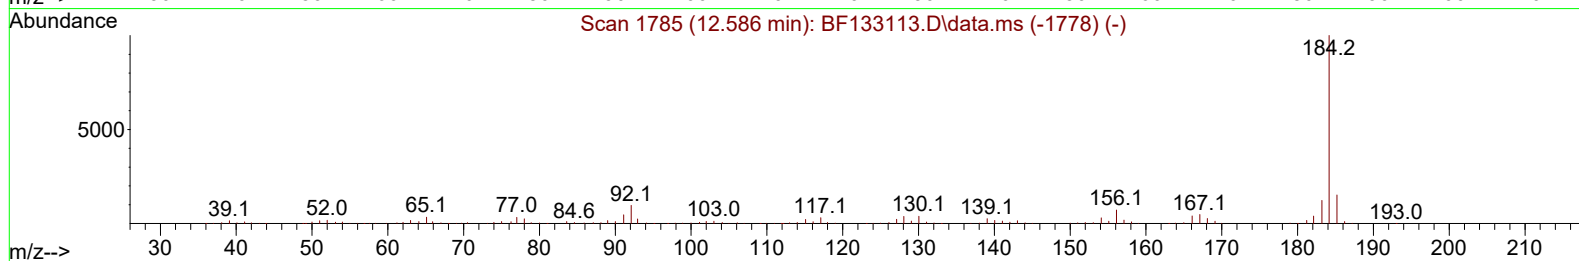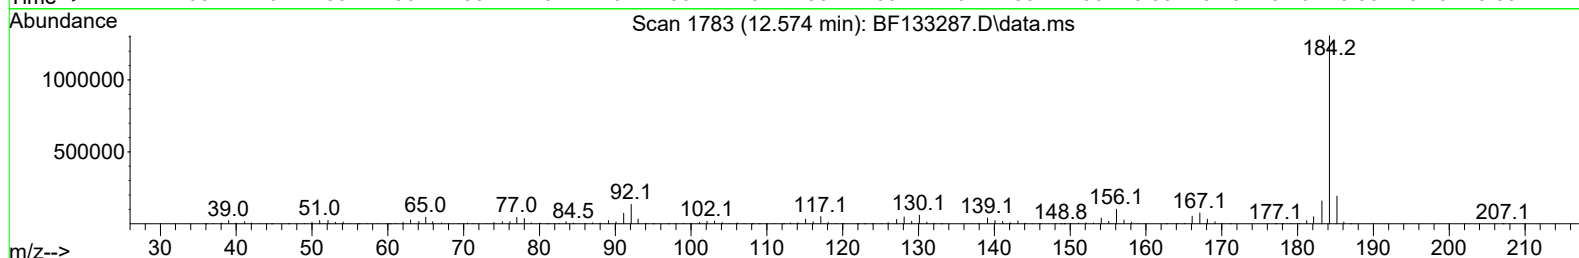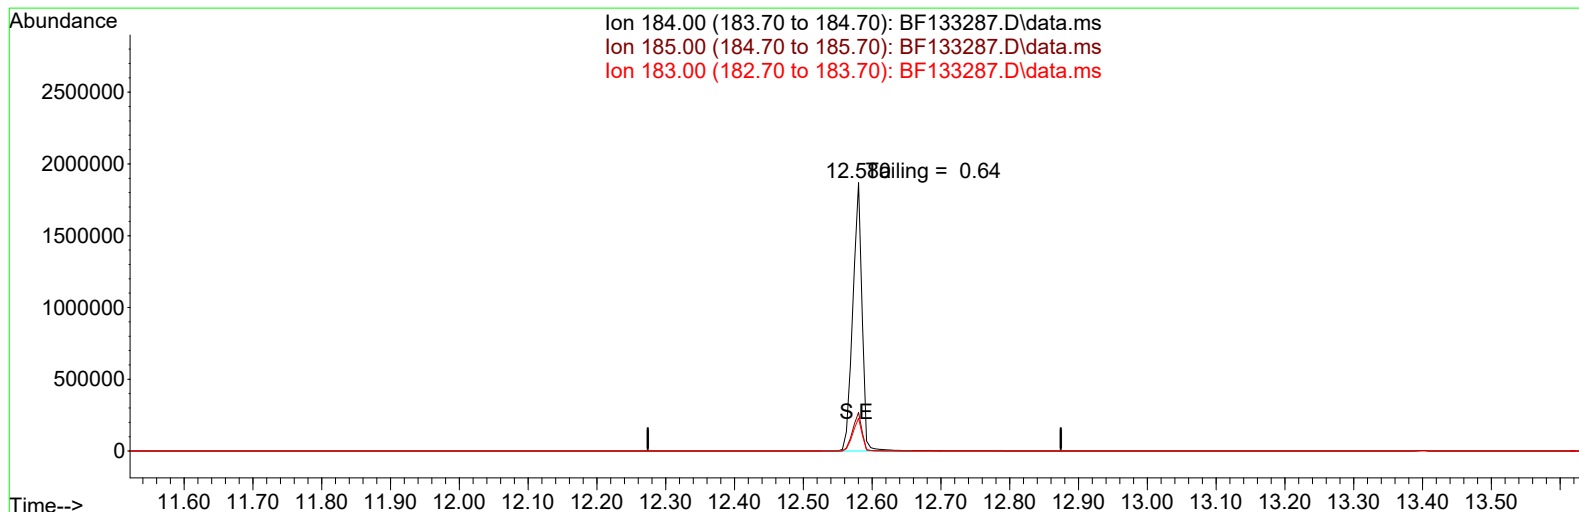

TIC: BF133287.D\data.ms

(77) Benzidine

12.574min (-12.574) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	19.30	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00