

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
 Data File : BF133297.D
 Acq On : 08 May 2023 16:24
 Operator : CG\JU
 Sample : 02567-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 EB-2023-29-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.916	477	481	492	rVB	412198	565905	7.03%	1.152%
2	5.340	548	553	556	rBV	4669225	4876251	60.57%	9.930%
3	6.363	722	727	730	rBV	3774833	3482042	43.25%	7.091%
4	6.722	784	788	791	rBV	2631990	2045315	25.40%	4.165%
5	7.292	879	885	888	rBV	4744986	5389527	66.94%	10.975%
6	8.004	1002	1006	1009	rBV	3277326	2747545	34.13%	5.595%
7	9.086	1185	1190	1193	rBV	7373956	8051185	100.00%	16.395%
8	9.757	1300	1304	1307	rBV	3615536	3035553	37.70%	6.181%
9	10.551	1434	1439	1442	rBV	3937450	4152023	51.57%	8.455%
10	11.239	1552	1556	1559	rBV	3579095	2996849	37.22%	6.103%
11	11.310	1562	1568	1571	rVB2	85987	81901	1.02%	0.167%
12	12.833	1821	1827	1830	rBV	6540133	7831545	97.27%	15.948%
13	13.874	2000	2004	2007	rBV	2302880	1938969	24.08%	3.948%
14	13.968	2015	2020	2030	rBV	141017	152155	1.89%	0.310%
15	15.292	2239	2245	2250	rBV	1481806	1761285	21.88%	3.587%




Sum of corrected areas: 49108050

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133297.D
Acq On : 08 May 2023 16:24
Operator : CG\JU
Sample : 02567-03
Misc :
ALS Vial : 12 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
EB-2023-29-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

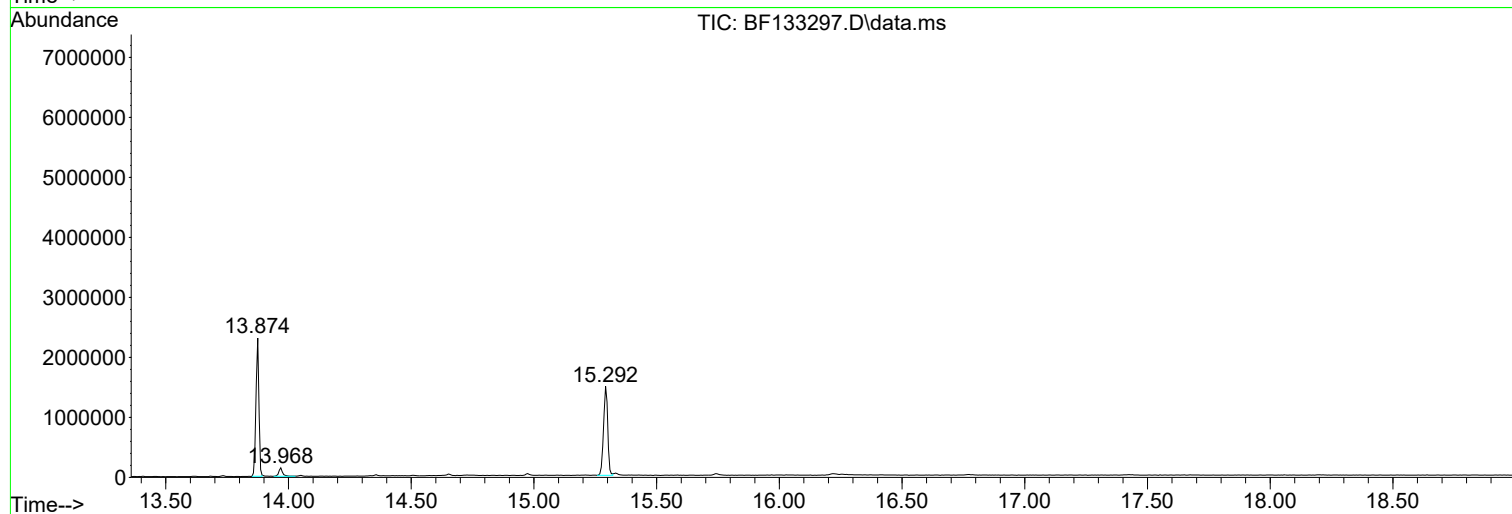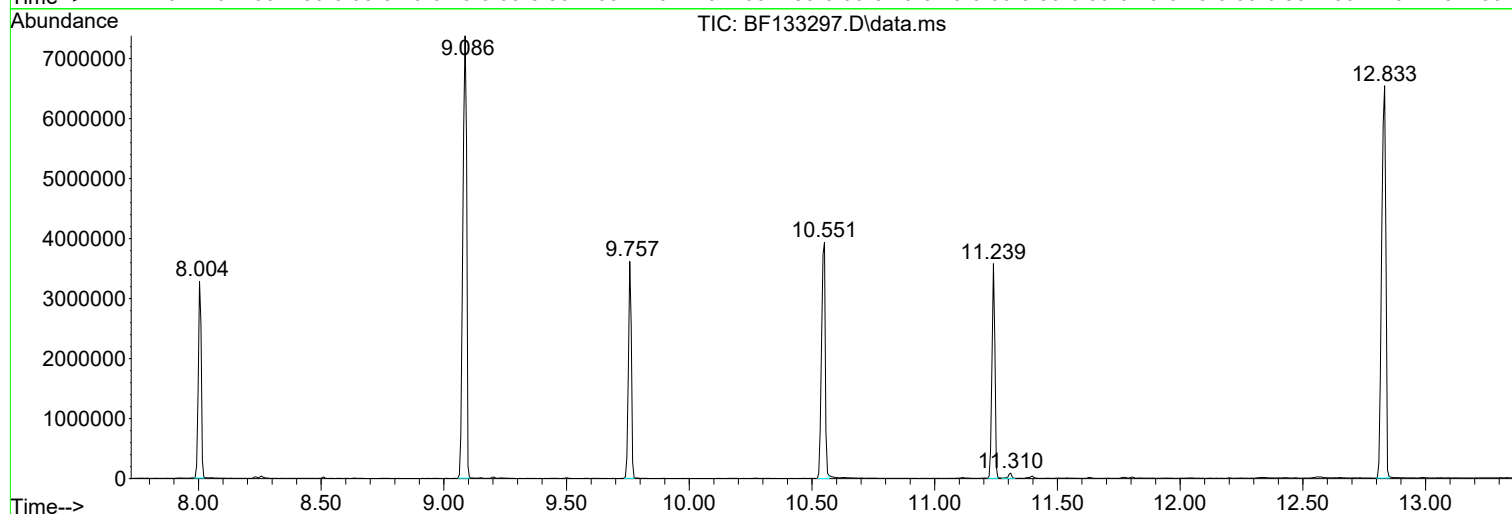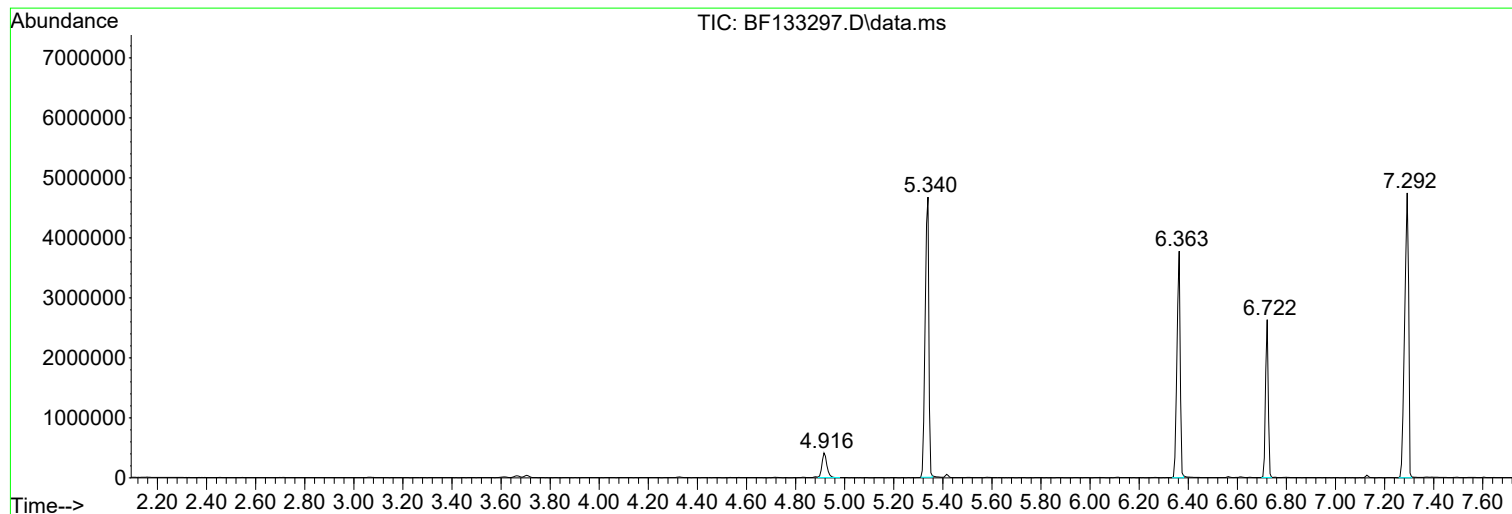

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133297.D
Acq On : 08 May 2023 16:24
Operator : CG\JU
Sample : 02567-03
Misc :
ALS Vial : 12 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
EB-2023-29-04










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.916	5.53 ng	565905	1,4-Dichlorobenzene-d4	6.722

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9		
4	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	9		
5	5-Oxohexanenitrile	111	C6H9NO	010412-98-3	9		

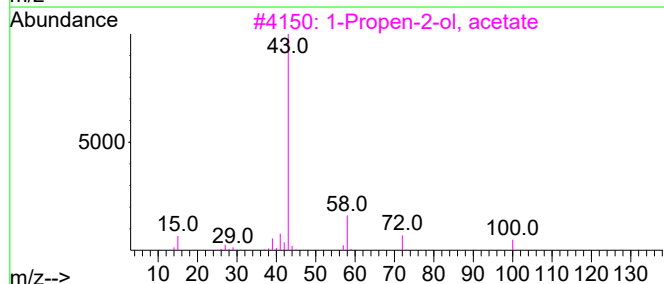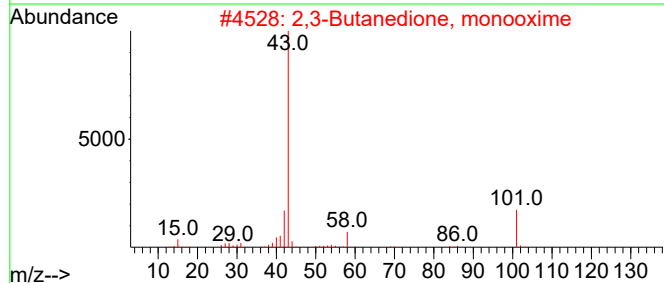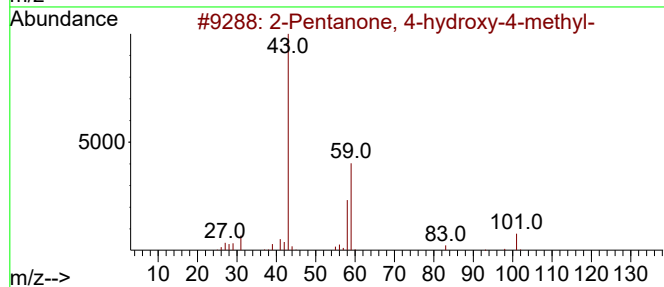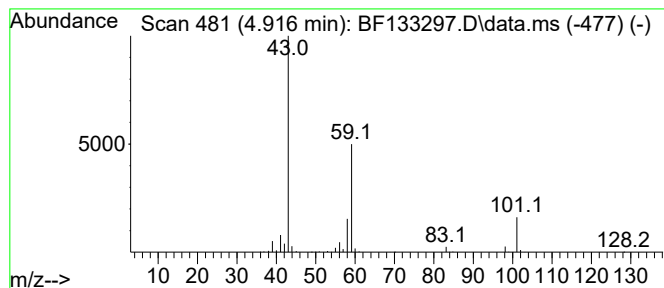

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133297.D
Acq On : 08 May 2023 16:24
Operator : CG\JU
Sample : 02567-03
Misc :
ALS Vial : 12 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
EB-2023-29-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.916	5.5	ng	565905	1	6.722	2045320	20.0