

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050823\  
 Data File : BF133300.D  
 Acq On : 08 May 2023 18:02  
 Operator : CG\JU  
 Sample : 02659-01  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 STEPS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133300.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.257       | 364           | 369         | 377          | rBV      | 566938         | 697837        | 18.02%          | 2.303%        |
| 2         | 4.916       | 474           | 481         | 484          | rBV      | 2655207        | 3473113       | 89.67%          | 11.462%       |
| 3         | 5.328       | 547           | 551         | 555          | rBV      | 2189985        | 2066289       | 53.35%          | 6.819%        |
| 4         | 5.728       | 615           | 619         | 622          | rBV      | 72618          | 60333         | 1.56%           | 0.199%        |
| 5         | 6.363       | 722           | 727         | 730          | rBV      | 3176569        | 3041725       | 78.53%          | 10.038%       |
| 6         | 6.722       | 784           | 788         | 791          | rBV      | 1418821        | 1218361       | 31.45%          | 4.021%        |
| 7         | 7.287       | 879           | 884         | 887          | rBV      | 2295146        | 2111849       | 54.52%          | 6.969%        |
| 8         | 8.004       | 1002          | 1006        | 1009         | rBV      | 2177374        | 1662292       | 42.92%          | 5.486%        |
| 9         | 9.081       | 1185          | 1189        | 1192         | rBV      | 4955812        | 3873378       | 100.00%         | 12.782%       |
| 10        | 9.757       | 1300          | 1304        | 1307         | rBV      | 2174187        | 1836733       | 47.42%          | 6.061%        |
| 11        | 10.463      | 1421          | 1424        | 1428         | rBV      | 1174859        | 1006855       | 25.99%          | 3.323%        |
| 12        | 10.539      | 1434          | 1437        | 1442         | rBV      | 310860         | 258557        | 6.68%           | 0.853%        |
| 13        | 10.669      | 1456          | 1459        | 1464         | rBV2     | 35879          | 48784         | 1.26%           | 0.161%        |
| 14        | 10.775      | 1474          | 1477        | 1481         | rVB      | 200118         | 154998        | 4.00%           | 0.512%        |
| 15        | 11.239      | 1552          | 1556        | 1559         | rBV      | 1973143        | 1806387       | 46.64%          | 5.961%        |
| 16        | 12.822      | 1821          | 1825        | 1829         | rBV      | 3997061        | 3711305       | 95.82%          | 12.248%       |
| 17        | 13.369      | 1915          | 1918        | 1922         | rBV      | 125199         | 109789        | 2.83%           | 0.362%        |
| 18        | 13.404      | 1922          | 1924        | 1927         | rVV2     | 64662          | 51182         | 1.32%           | 0.169%        |
| 19        | 13.733      | 1975          | 1980        | 1988         | rBV      | 212834         | 341945        | 8.83%           | 1.128%        |
| 20        | 13.869      | 1999          | 2003        | 2007         | rBV      | 1346596        | 1173334       | 30.29%          | 3.872%        |
| 21        | 13.963      | 2015          | 2019        | 2025         | rVB      | 244497         | 262079        | 6.77%           | 0.865%        |
| 22        | 14.051      | 2031          | 2034        | 2037         | rVB      | 58774          | 50060         | 1.29%           | 0.165%        |
| 23        | 14.357      | 2082          | 2086        | 2089         | rBV      | 56088          | 62971         | 1.63%           | 0.208%        |
| 24        | 15.245      | 2233          | 2237        | 2240         | rBV2     | 51079          | 62095         | 1.60%           | 0.205%        |
| 25        | 15.286      | 2240          | 2244        | 2249         | rVV      | 897014         | 1030101       | 26.59%          | 3.399%        |
| 26        | 16.198      | 2395          | 2399        | 2411         | rVB3     | 69541          | 129922        | 3.35%           | 0.429%        |




Sum of corrected areas: 30302274

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050823\  
Data File : BF133300.D  
Acq On : 08 May 2023 18:02  
Operator : CG\JU  
Sample : 02659-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
STEPS

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

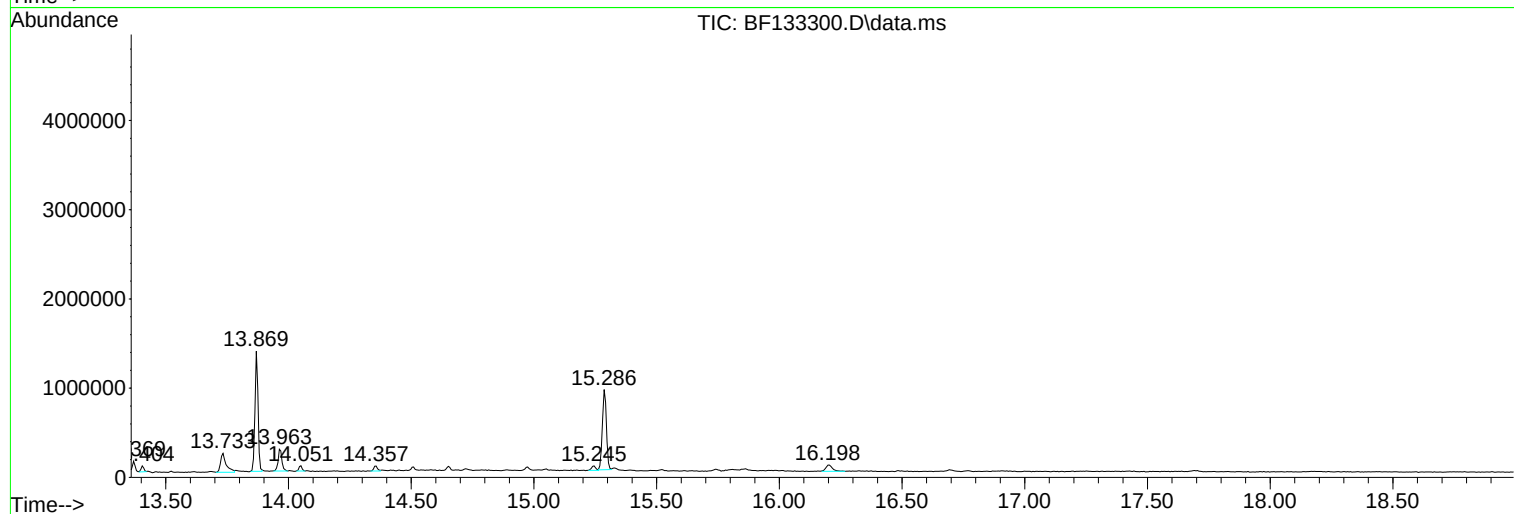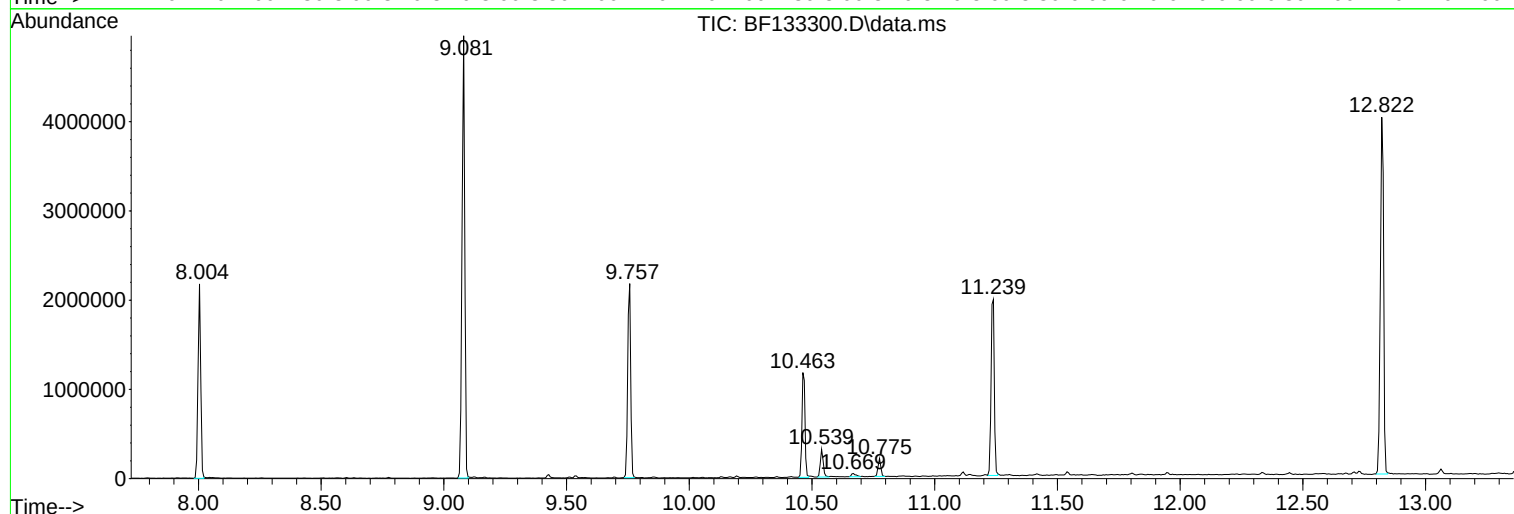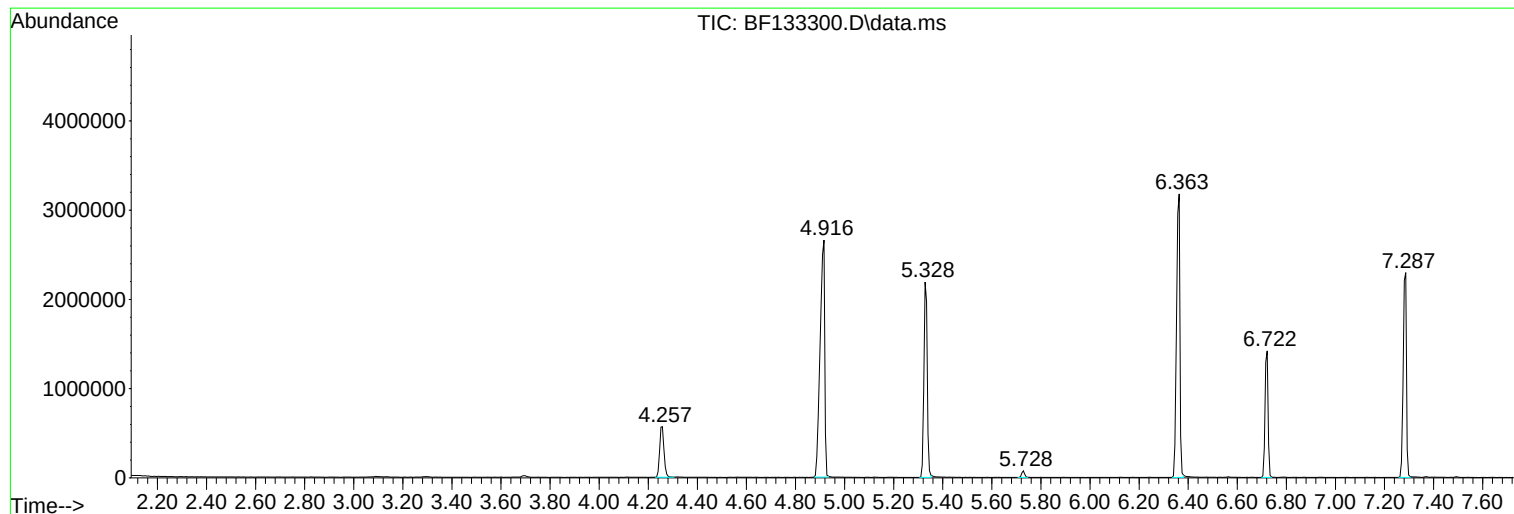

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050823\  
Data File : BF133300.D  
Acq On : 08 May 2023 18:02  
Operator : CG\JU  
Sample : 02659-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
STEPS

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050823\  
Data File : BF133300.D  
Acq On : 08 May 2023 18:02  
Operator : CG\JU  
Sample : 02659-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
STEPS

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|