

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
 Data File : BF133301.D
 Acq On : 08 May 2023 18:35
 Operator : CG\JU
 Sample : 02659-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LARGE-PAD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.251	364	368	378	rBV	354811	435703	11.72%	1.661%
2	4.910	474	480	483	rBV	1926243	2344451	63.07%	8.937%
3	5.328	547	551	555	rBV	2619458	2419206	65.08%	9.222%
4	5.728	616	619	625	rBV	69270	59785	1.61%	0.228%
5	6.357	722	726	742	rBV	2931117	2932495	78.89%	11.179%
6	6.722	784	788	791	rBV	1327074	1129789	30.39%	4.307%
7	7.287	879	884	887	rBV	2275677	2028341	54.57%	7.732%
8	8.004	1002	1006	1009	rBV	2036868	1521032	40.92%	5.798%
9	9.081	1185	1189	1192	rBV	4797696	3717030	100.00%	14.169%
10	9.757	1300	1304	1307	rBV	1935452	1652388	44.45%	6.299%
11	10.463	1421	1424	1428	rBV	299776	245456	6.60%	0.936%
12	10.539	1433	1437	1447	rBV	829870	710107	19.10%	2.707%
13	10.869	1490	1493	1497	rBV	65344	56151	1.51%	0.214%
14	11.233	1552	1555	1559	rBV	1767457	1554139	41.81%	5.924%
15	12.822	1821	1825	1828	rBV	3458993	2970771	79.92%	11.325%
16	13.733	1977	1980	1989	rVB2	107702	180745	4.86%	0.689%
17	13.869	2000	2003	2010	rVB	1023535	893197	24.03%	3.405%
18	13.963	2016	2019	2026	rVB	249549	265670	7.15%	1.013%
19	15.286	2240	2244	2249	rBV	866025	1003283	26.99%	3.824%
20	16.362	2423	2427	2436	rVB6	58146	113375	3.05%	0.432%




Sum of corrected areas: 26233114

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133301.D
Acq On : 08 May 2023 18:35
Operator : CG\JU
Sample : 02659-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LARGE-PAD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

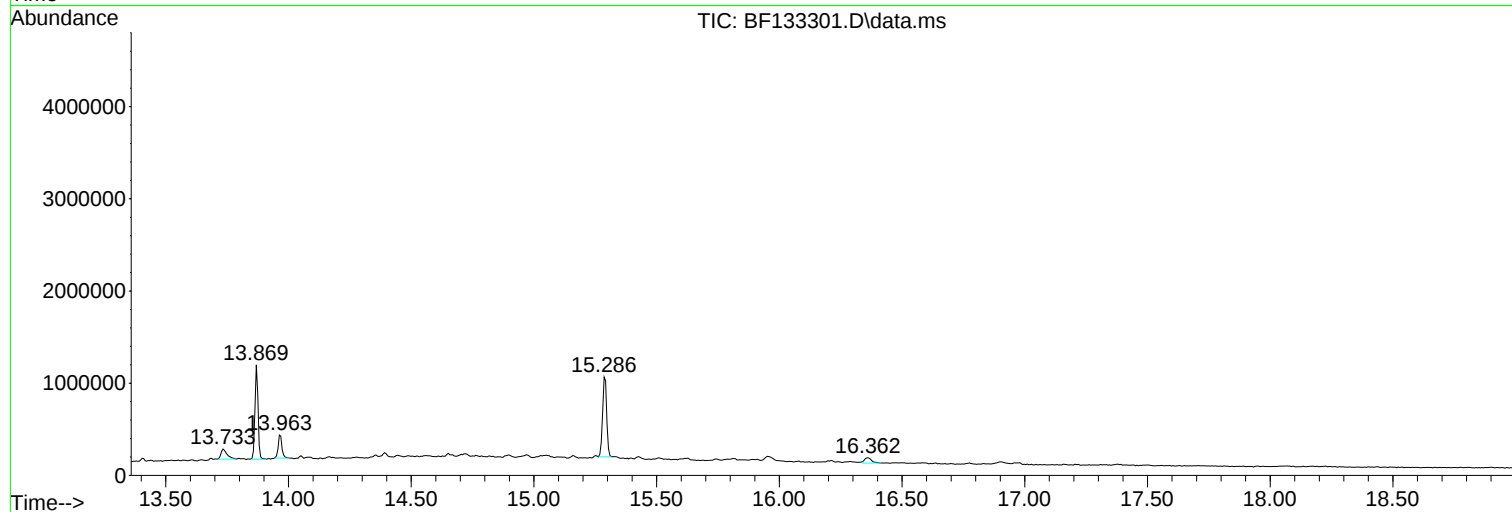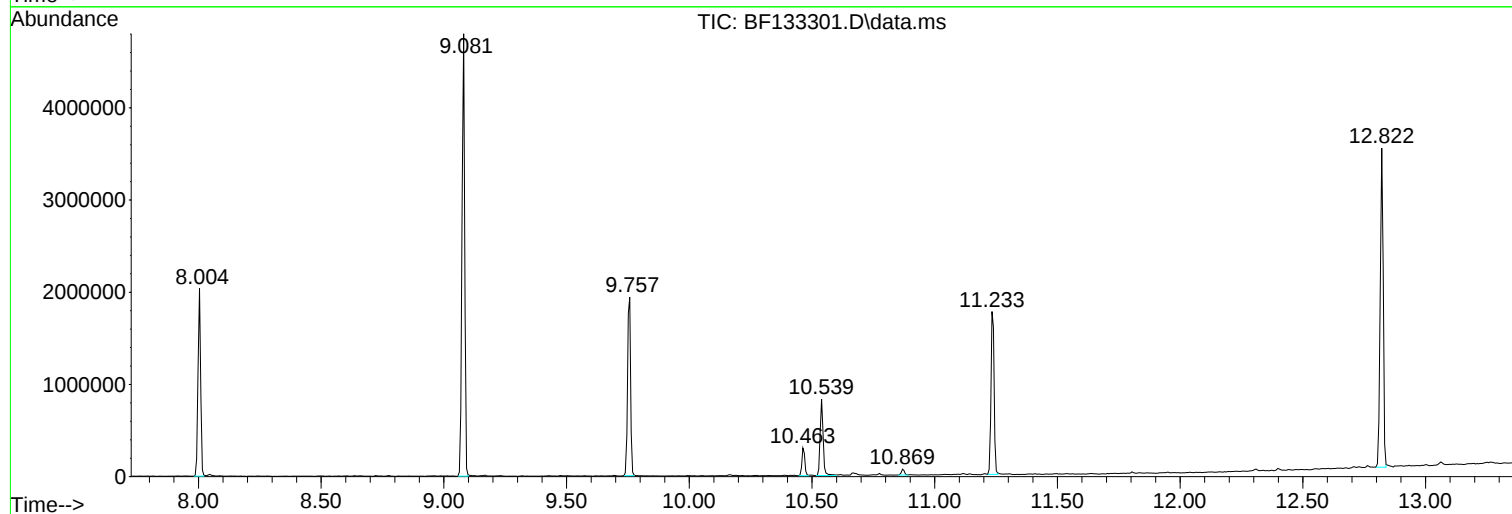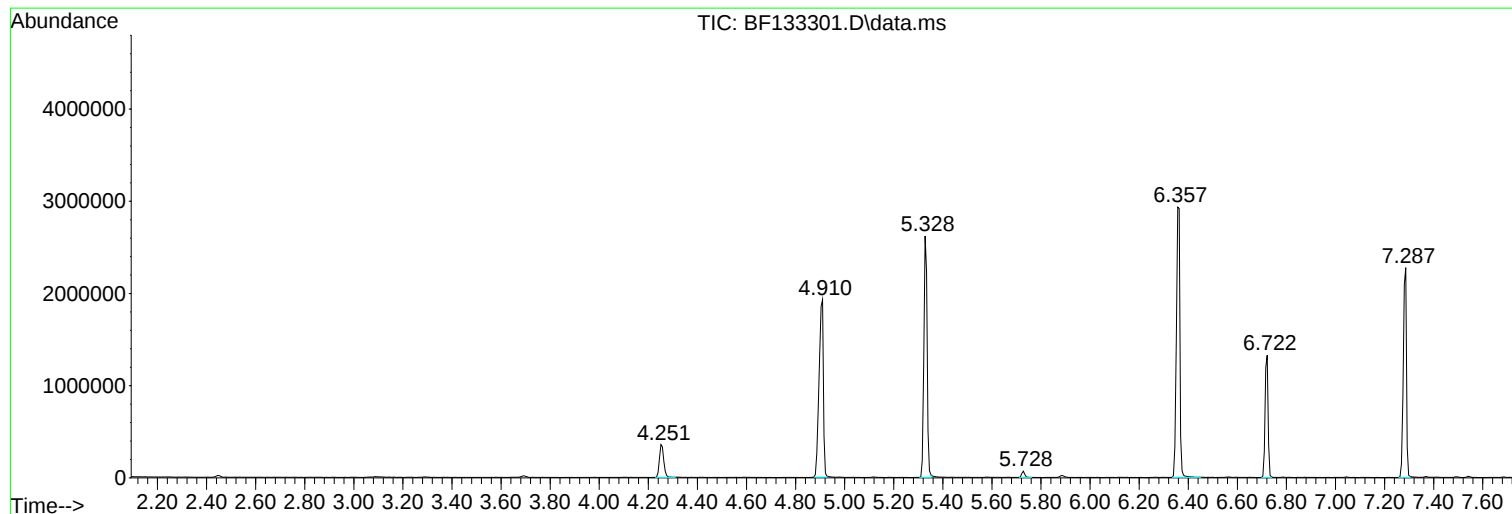

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133301.D
Acq On : 08 May 2023 18:35
Operator : CG\JU
Sample : 02659-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LARGE-PAD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133301.D
Acq On : 08 May 2023 18:35
Operator : CG\JU
Sample : 02659-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LARGE-PAD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------