
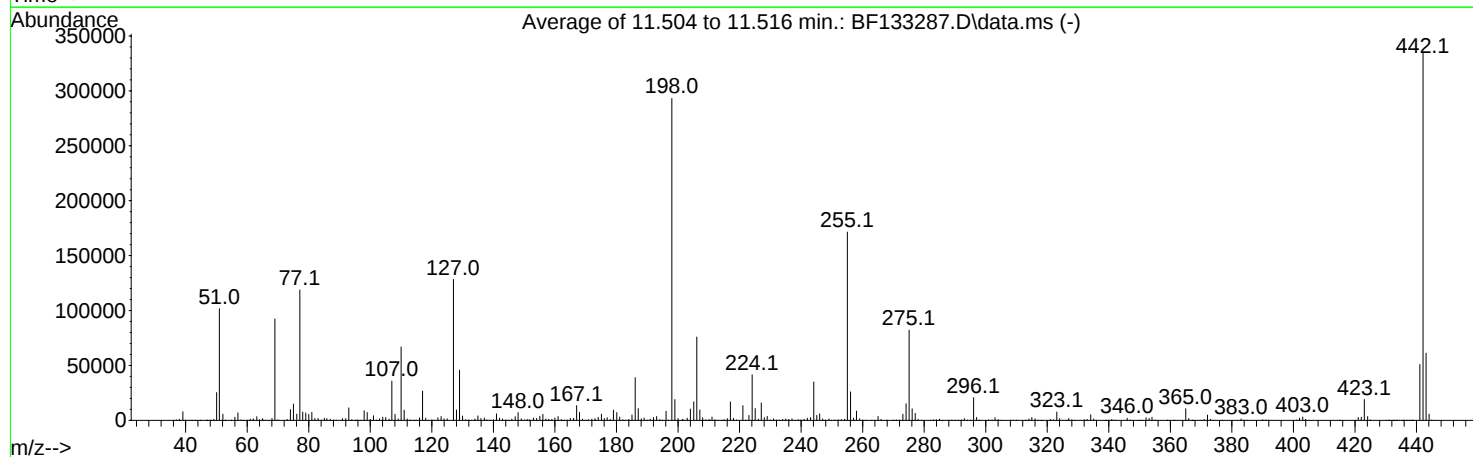


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
 Data File : BF133287.D
 Acq On : 08 May 2023 10:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 09 04:59:36 2023

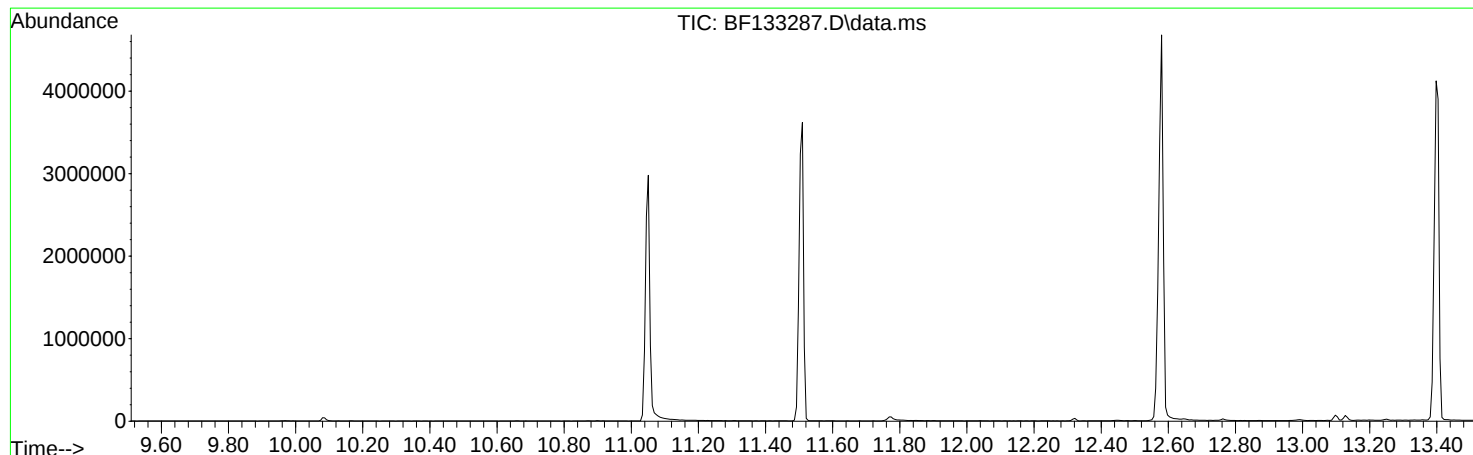

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	101747	PASS
68	69	0.00	2	1.8	1697	PASS
69	198	0.00	100	31.5	92439	PASS
70	69	0.00	2	0.6	512	PASS
127	198	10	80	43.8	128328	PASS
197	198	0.00	2	0.1	227	PASS
198	198	100	100	100.0	293157	PASS
199	198	5	9	6.5	18949	PASS
275	198	10	60	28.0	82219	PASS
365	198	1	100	3.6	10583	PASS
441	198	0.01	100	17.3	50824	PASS
442	442	50	100	100.0	334933	PASS
443	442	15	24	18.3	61267	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2023	BNA_F	<u>BF133287.D</u>
Compound Name	Response	Retention Time
DDT	786529	13.404
DDD	18740	13.098
DDE	2438	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21178	807707	2.62

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
Data File : BF133287.D
Acq On : 08 May 2023 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 09 06:50:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

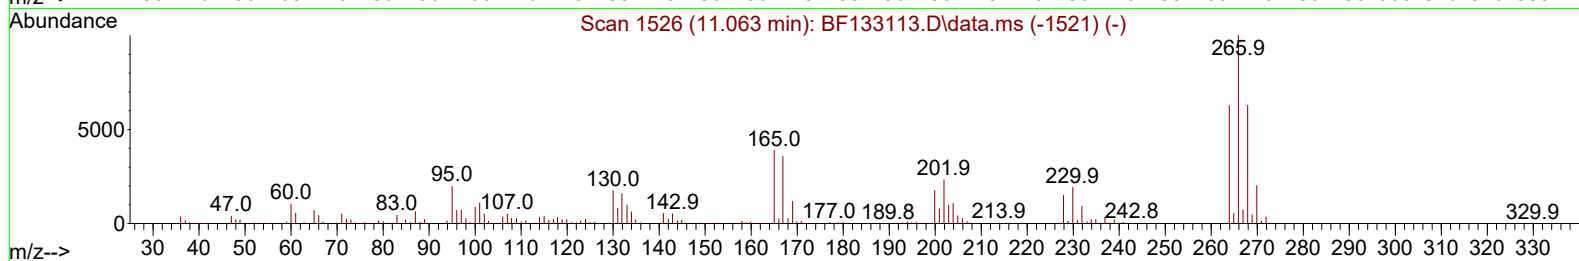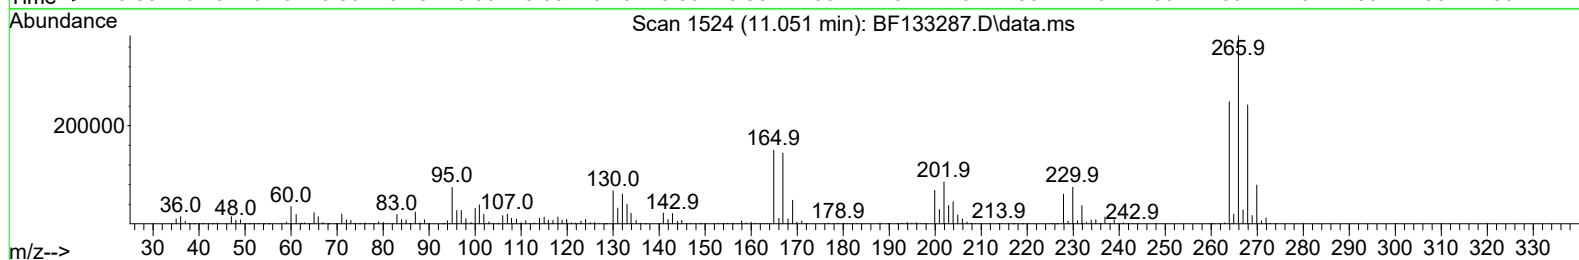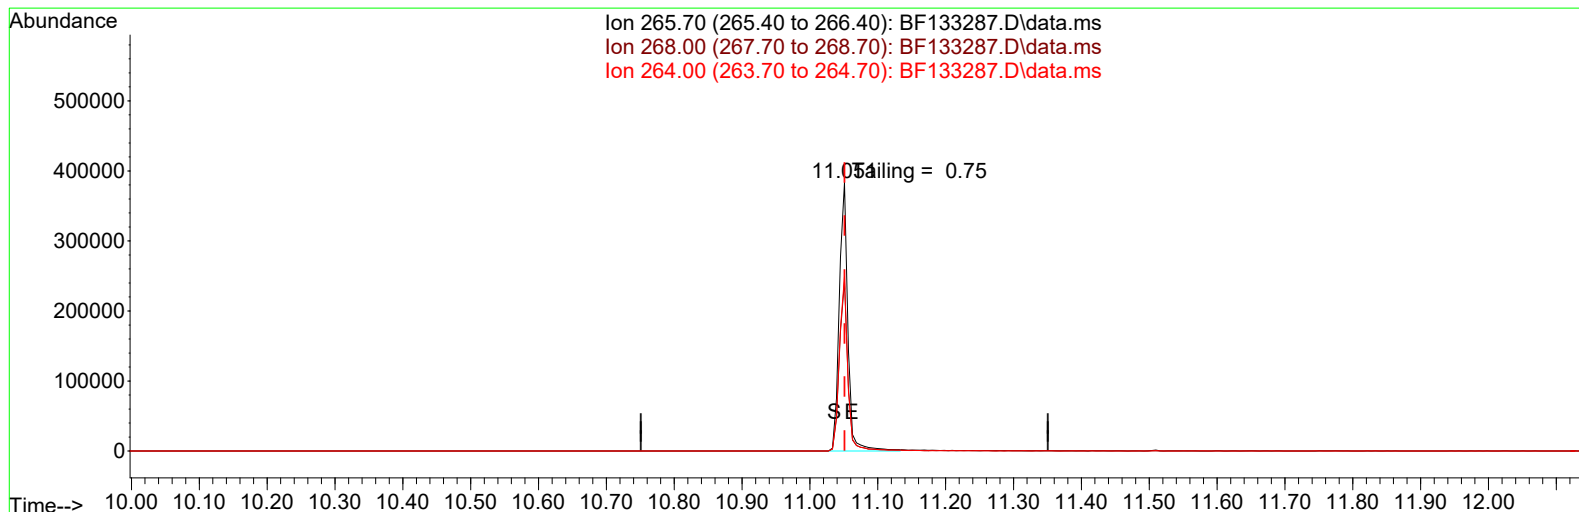

TIC: BF133287.D\data.ms

(70) Pentachlorophenol (C)

11.051min (0.000) 283401.45 ng




response 338705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.15
264.00	63.30	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050823\
 Data File : BF133287.D
 Acq On : 08 May 2023 10:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 09 06:50:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 04:59:36 2023
 Response via : Initial Calibration

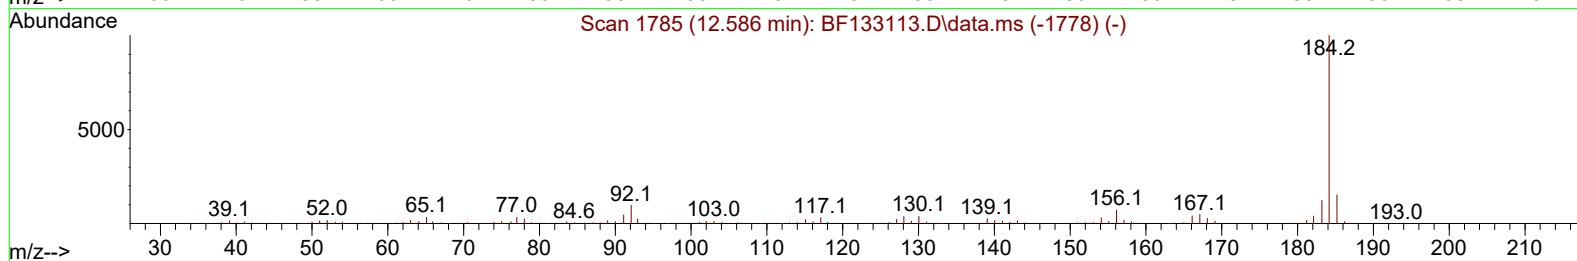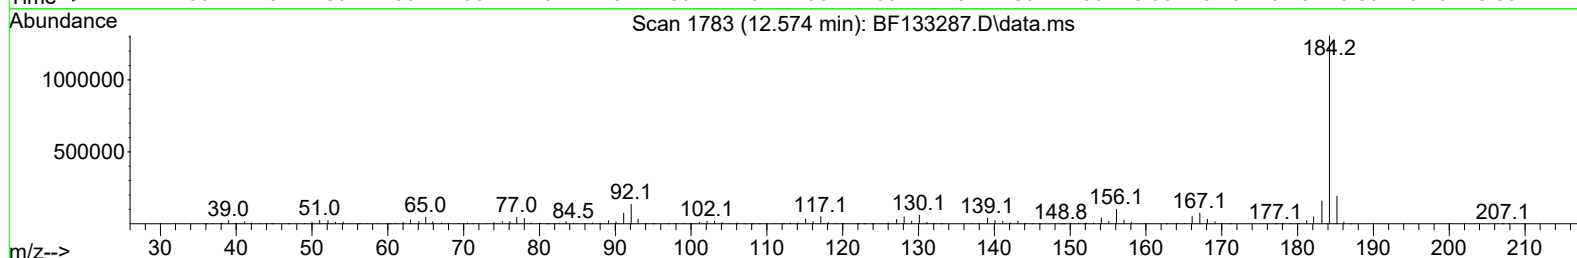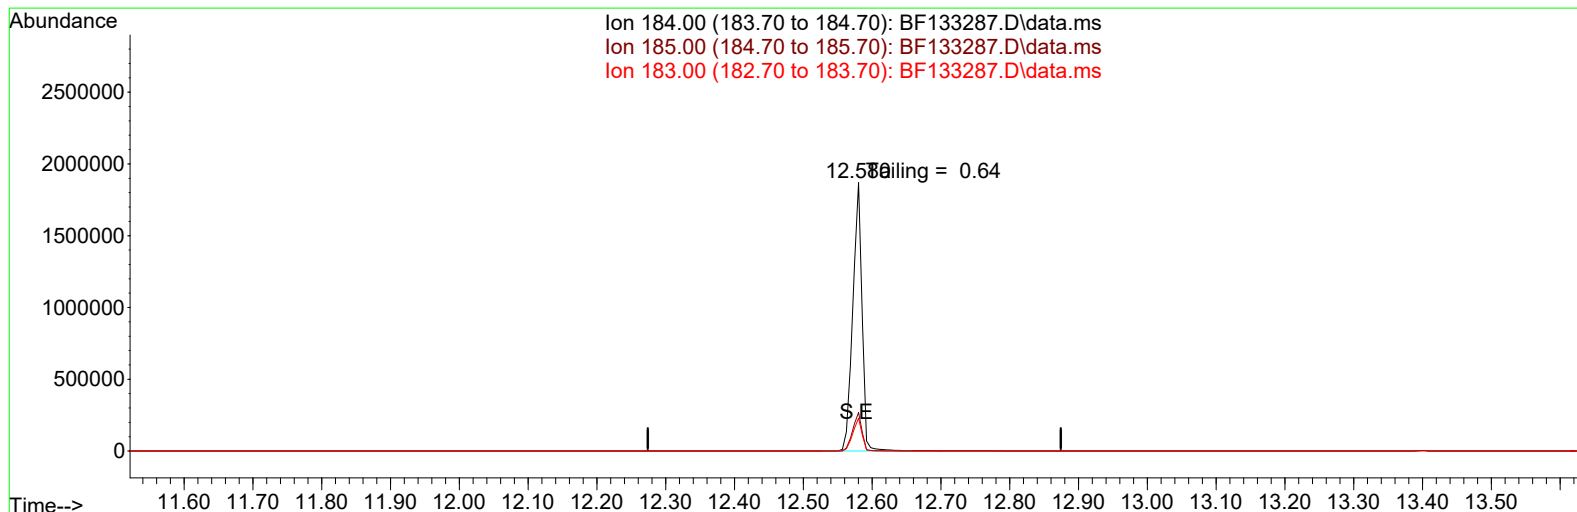

TIC: BF133287.D\data.ms

(77) Benzidine

12.574min (-12.574) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	19.30	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00