
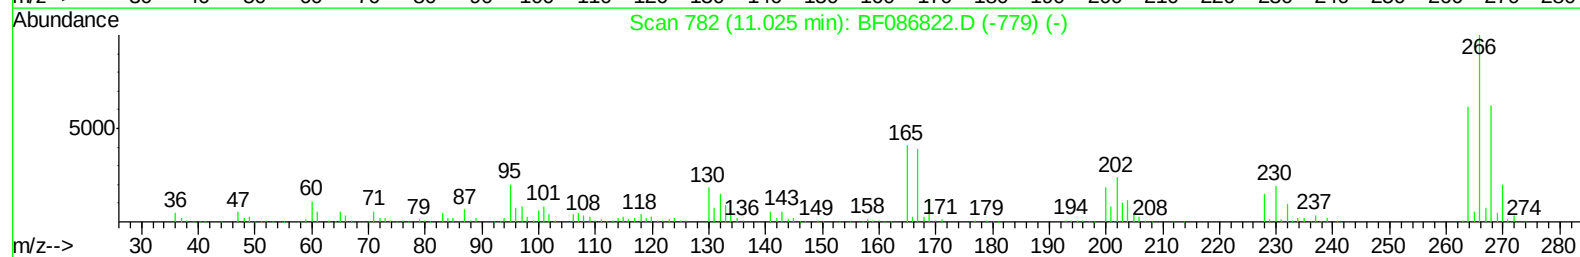
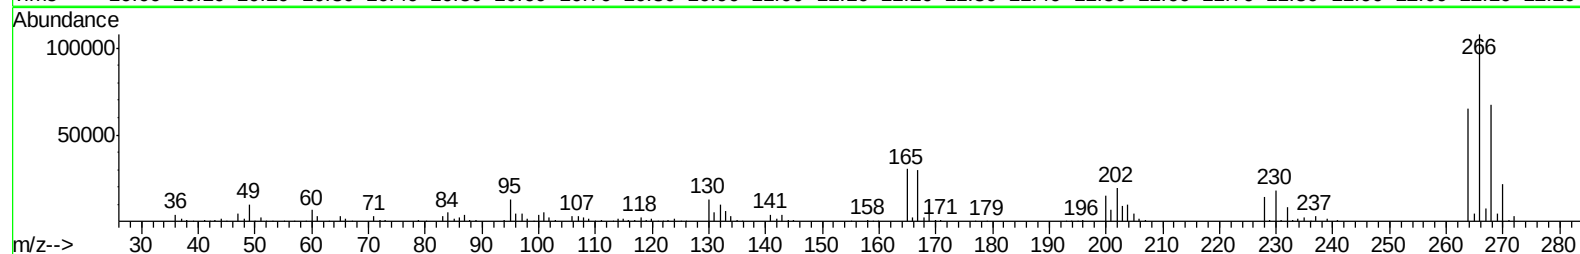


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050916\
Data File : BF086816.D
Acq On : 9 May 2016 10:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 16:13:15 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 16:04:56 2016
Response via : Initial Calibration

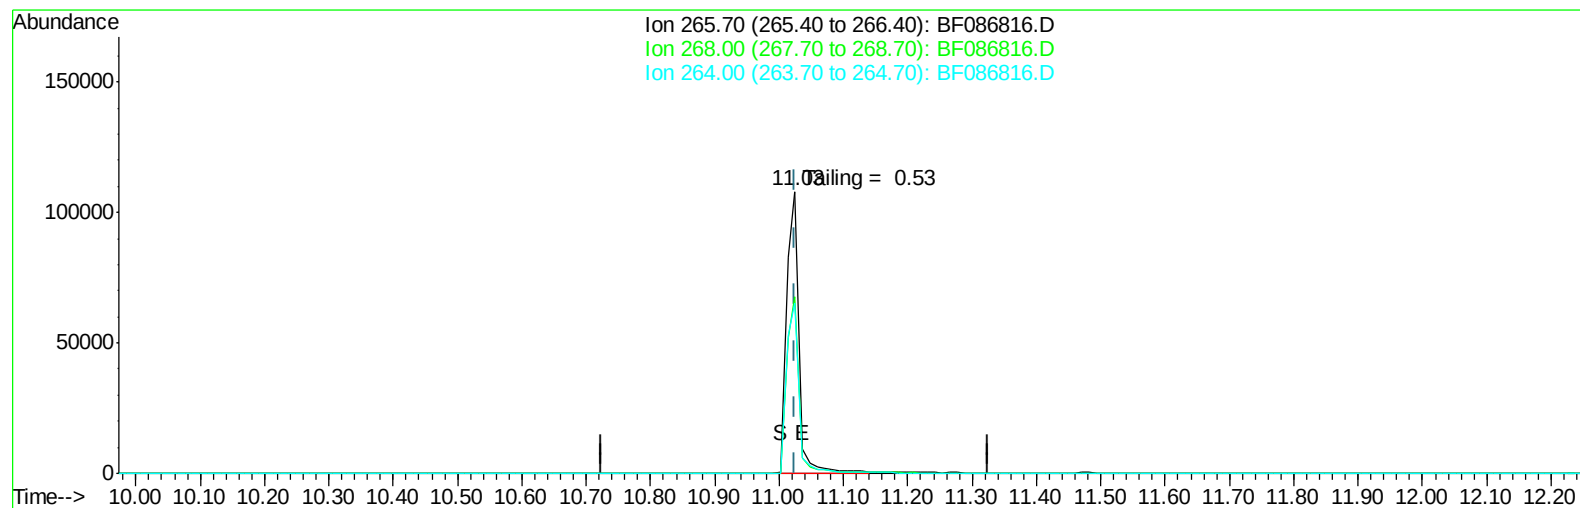

TIC: BF086816.D

(69) Pentachlorophenol (C)




11.025min (+0.000) 35800.91ng

response 150566

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.60
264.00	66.10	60.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050916\
Data File : BF086816.D
Acq On : 9 May 2016 10:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 16:13:15 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 16:04:56 2016
Response via : Initial Calibration

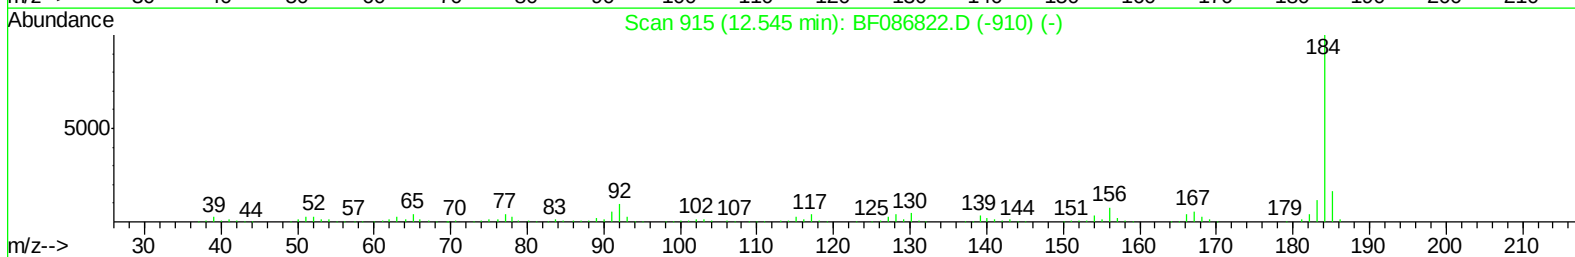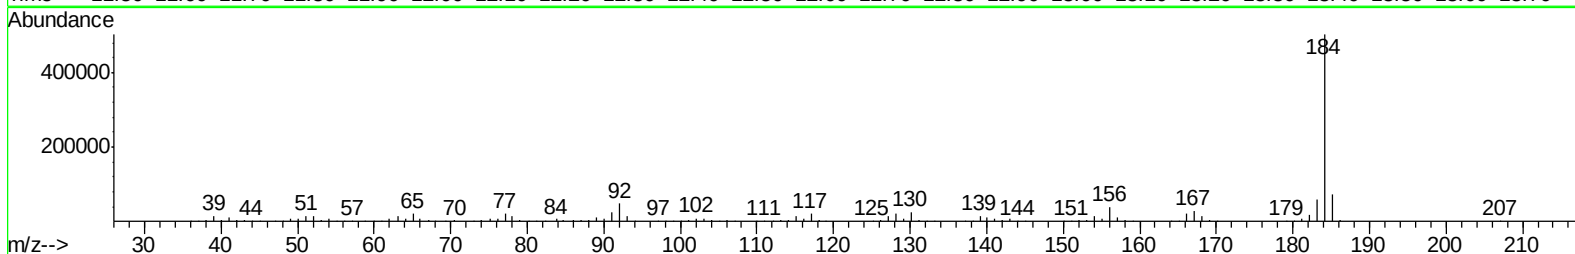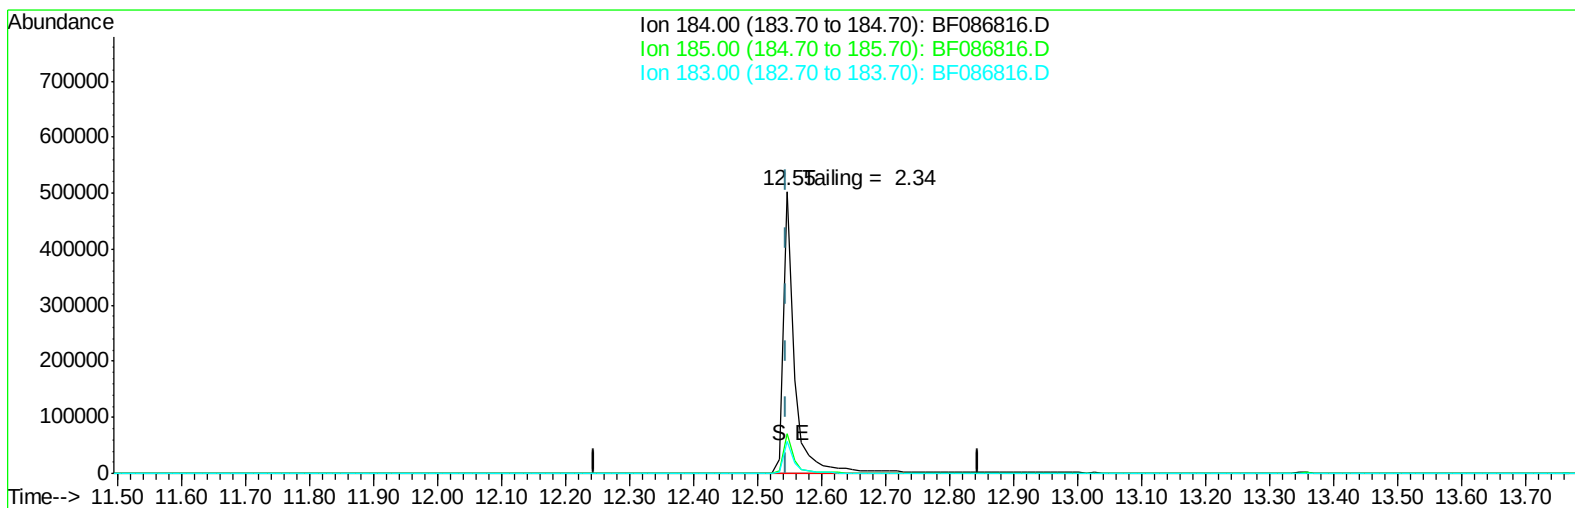

TIC: BF086816.D

(76) Benzidine

12.545min (+0.000) 75786.99ng

response 616331

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.20
183.00	12.20	11.56
0.00	0.00	0.00