

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
 Data File : BF086840.D
 Acq On : 10 May 2016 00:28
 Operator : UM/SJ
 Sample : H2895-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP7-7.5FT

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.853	240	242	250	rBV	253343	446480	9.64%	1.131%
2	5.287	278	280	283	rBV	3436975	3906963	84.33%	9.900%
3	6.350	370	373	375	rBV	4324642	4632717	100.00%	11.740%
4	6.464	381	383	385	rBV	4436366	4600798	99.31%	11.659%
5	6.693	400	403	405	rBV	779259	1025543	22.14%	2.599%
6	6.842	414	416	419	rBV	3217452	3103774	67.00%	7.865%
7	7.265	450	453	455	rBV	2860095	3386529	73.10%	8.582%
8	7.973	513	515	518	rBV	1435848	1372926	29.64%	3.479%
9	9.059	607	610	612	rBV	2753980	4030778	87.01%	10.214%
10	9.448	642	644	647	rBV	418020	578570	12.49%	1.466%
11	9.722	666	668	671	rBV	1682168	1587470	34.27%	4.023%
12	10.168	703	707	708	rBV	47756	70171	1.51%	0.178%
13	10.511	734	737	740	rBV	2913488	3156110	68.13%	7.998%
14	10.636	746	748	755	rVB	82836	115925	2.50%	0.294%
15	11.082	783	787	788	rBV	41779	46887	1.01%	0.119%
16	11.196	795	797	800	rBV	1185305	1619734	34.96%	4.104%
17	11.745	843	845	847	rBV	63930	76182	1.64%	0.193%
18	12.785	933	936	938	rBV	3524087	3228542	69.69%	8.181%
19	13.825	1025	1027	1030	rBV	1406321	1448590	31.27%	3.671%
20	15.197	1145	1147	1150	rBV	768774	1027745	22.18%	2.604%


Sum of corrected areas: 39462434

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
Data File : BF086840.D
Acq On : 10 May 2016 00:28
Operator : UM/SJ
Sample : H2895-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP7-7.5FT

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

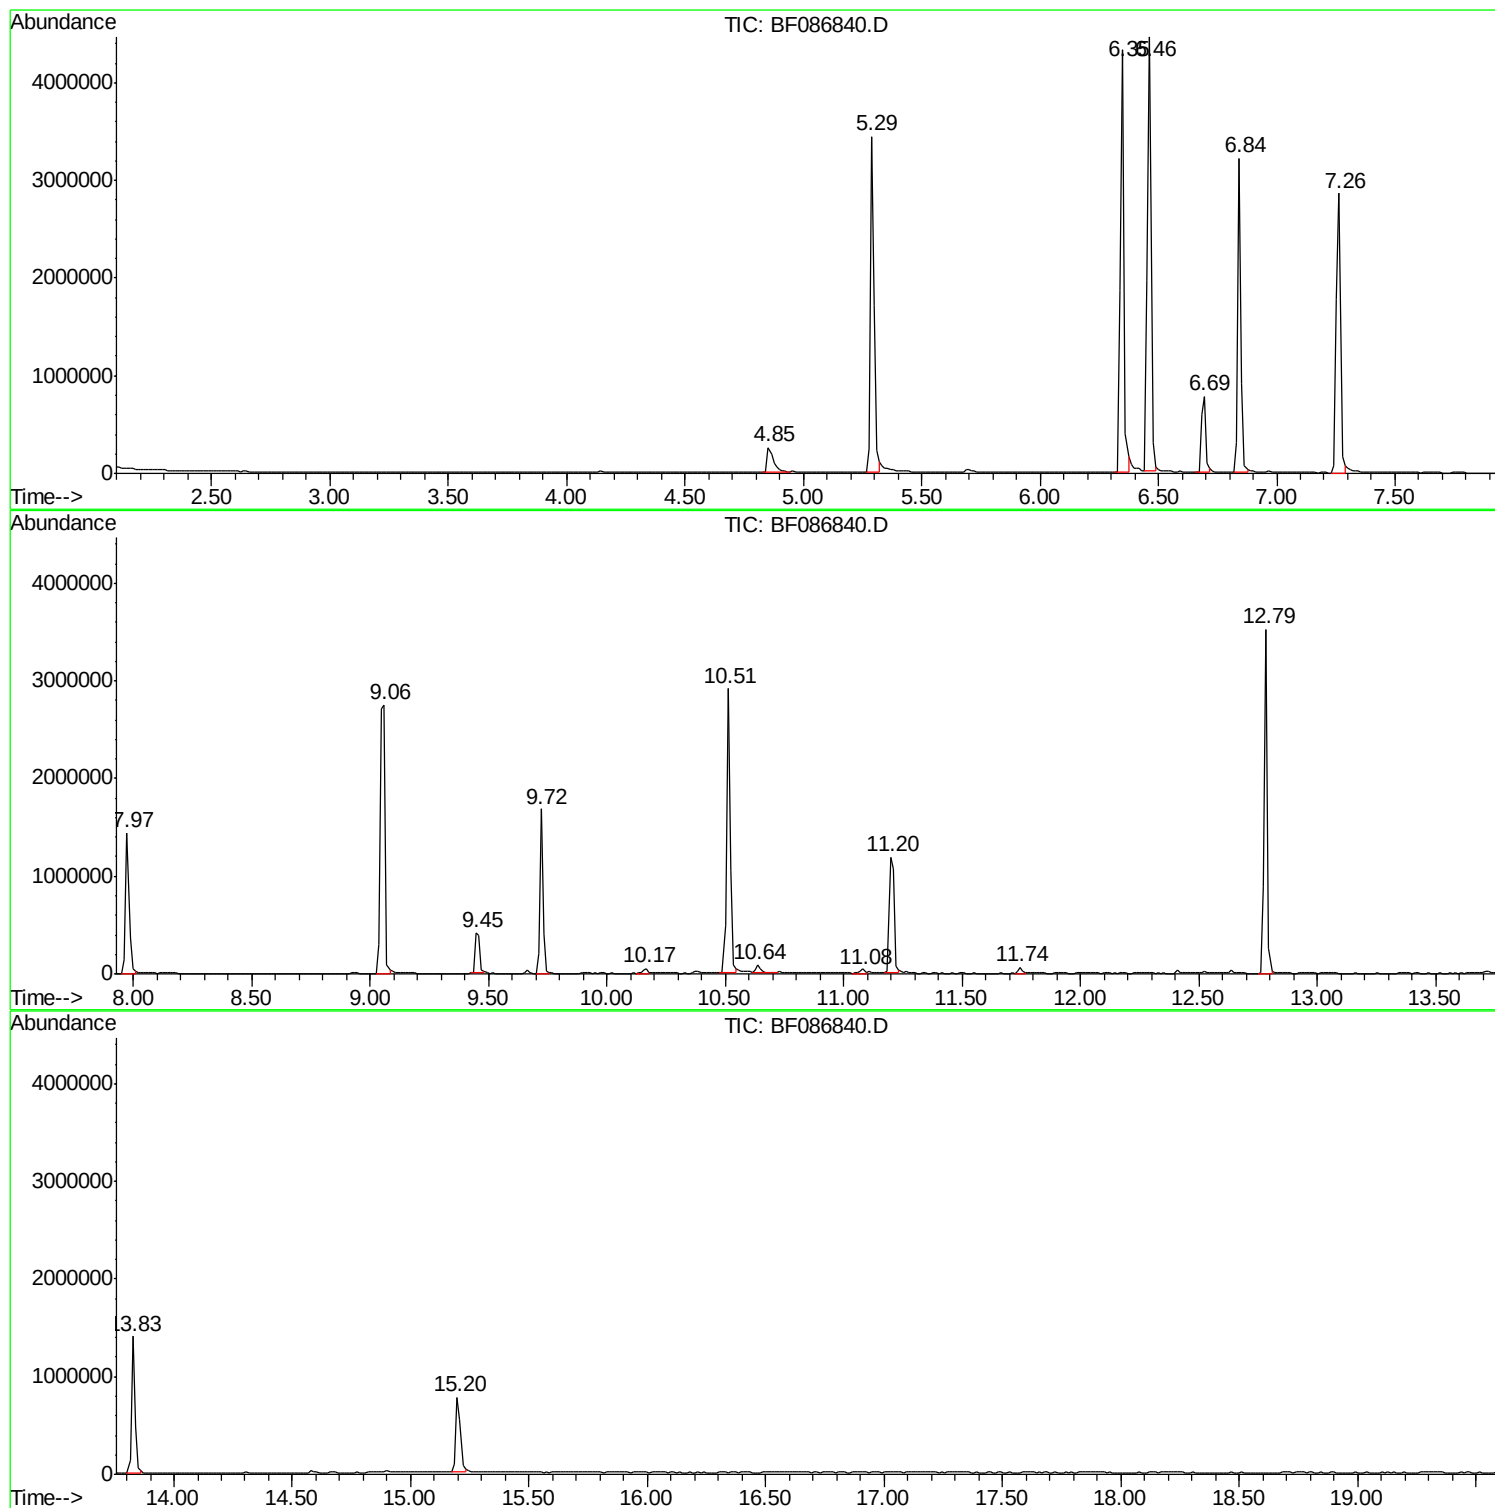

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
Data File : BF086840.D
Acq On : 10 May 2016 00:28
Operator : UM/SJ
Sample : H2895-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP7-7.5FT










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.85	8.71 ng	446480	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4			Diacetamide	101	C4H7NO2	000625-77-4	9
5			Butane	58	C4H10	000106-97-8	9

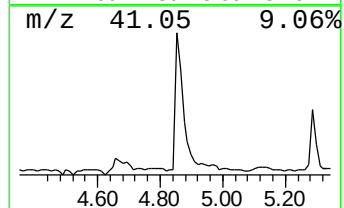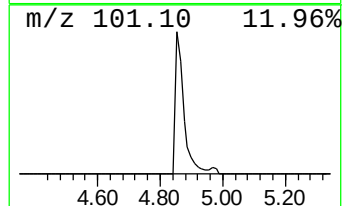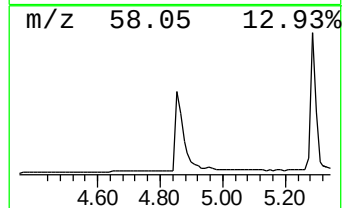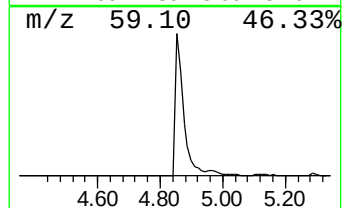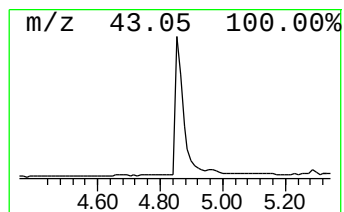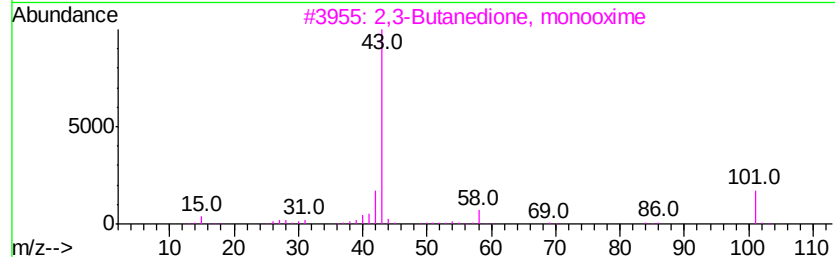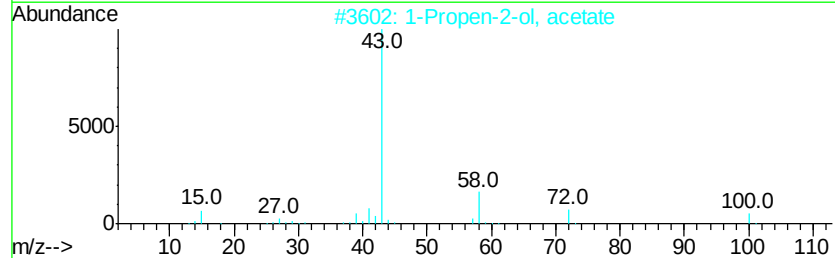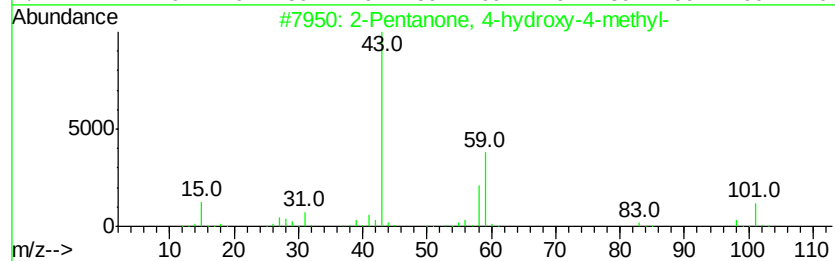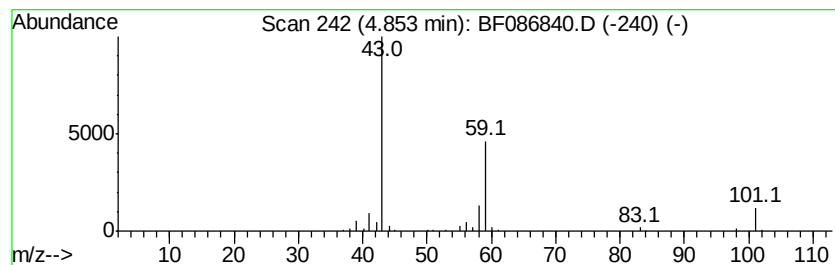

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
Data File : BF086840.D
Acq On : 10 May 2016 00:28
Operator : UM/SJ
Sample : H2895-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP7-7.5FT










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	89.72 ng	4600800	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
5			(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10

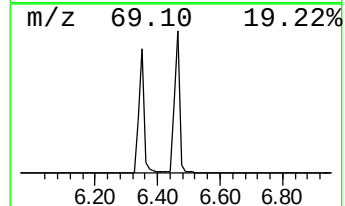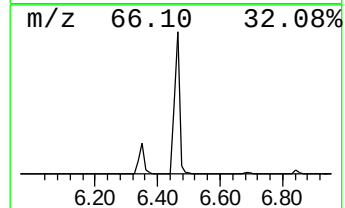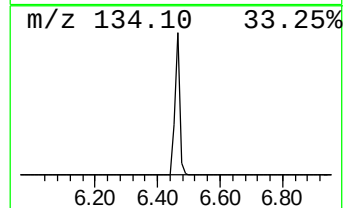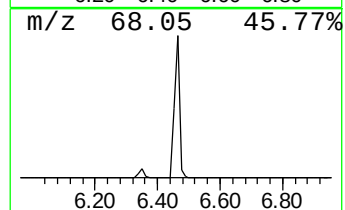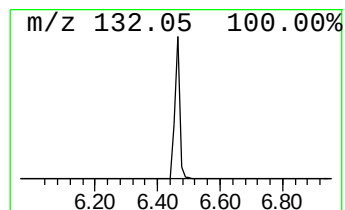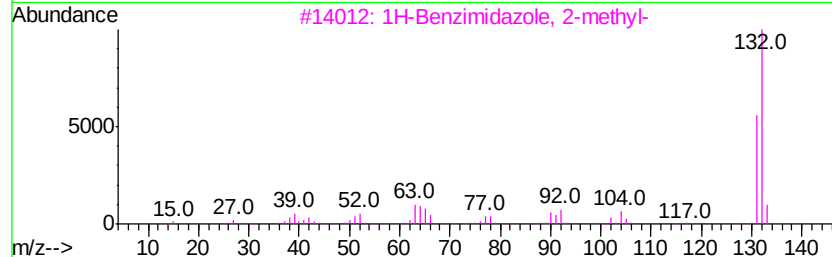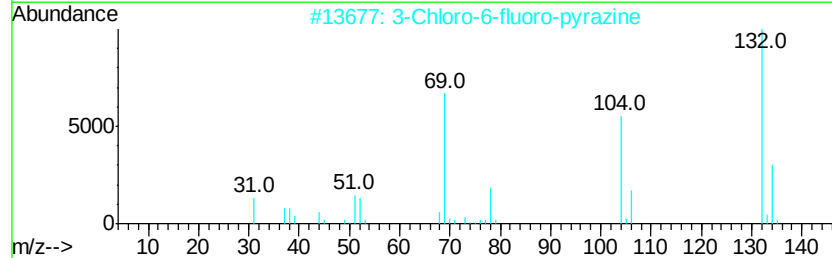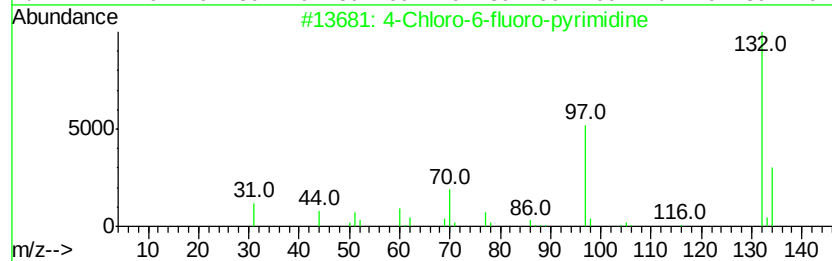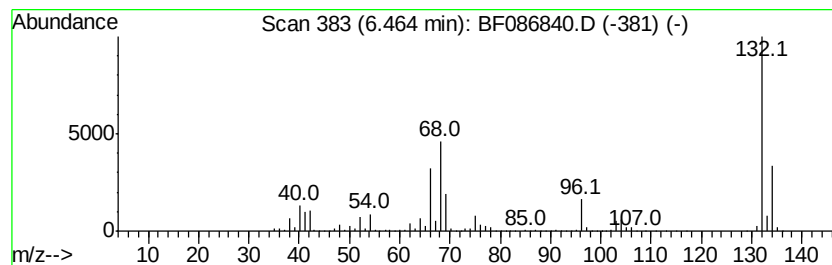

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
Data File : BF086840.D
Acq On : 10 May 2016 00:28
Operator : UM/SJ
Sample : H2895-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP7-7.5FT

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.85	8.7	ng	446480	1	6.69	1025540	20.0
unknown6.46	6.46	89.7	ng	4600800	1	6.69	1025540	20.0