


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050916\
 Data File : BF086827.D
 Acq On : 9 May 2016 17:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 16:04:56 2016

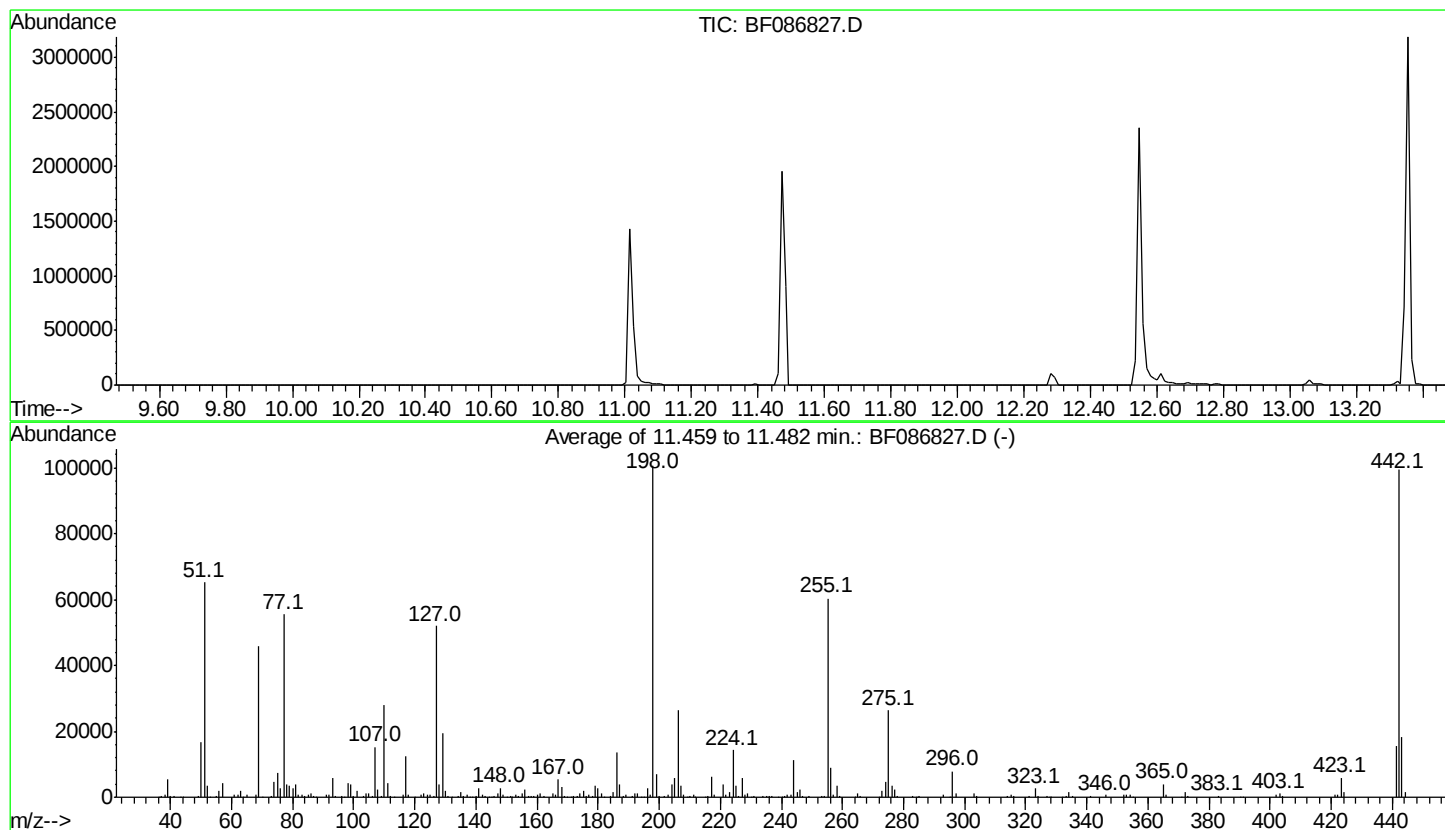

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.8	65198	PASS
68	69	0.00	2	1.5	697	PASS
69	198	0.00	100	45.4	45715	PASS
70	69	0.00	2	0.4	175	PASS
127	198	10	80	51.6	51964	PASS
197	198	0.00	2	0.8	835	PASS
198	198	100	100	100.0	100680	PASS
199	198	5	9	6.8	6856	PASS
275	198	10	60	26.2	26412	PASS
365	198	1	100	4.0	4061	PASS
441	442	0.01	24	15.7	15610	PASS
442	198	50	100	98.8	99489	PASS
443	442	15	24	18.3	18192	PASS