


Data Path : Z:\HPCHEM1\BNA F\Data\BF050917\
 Data File : BF095024.D
 Acq On : 9 May 2017 16:07
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

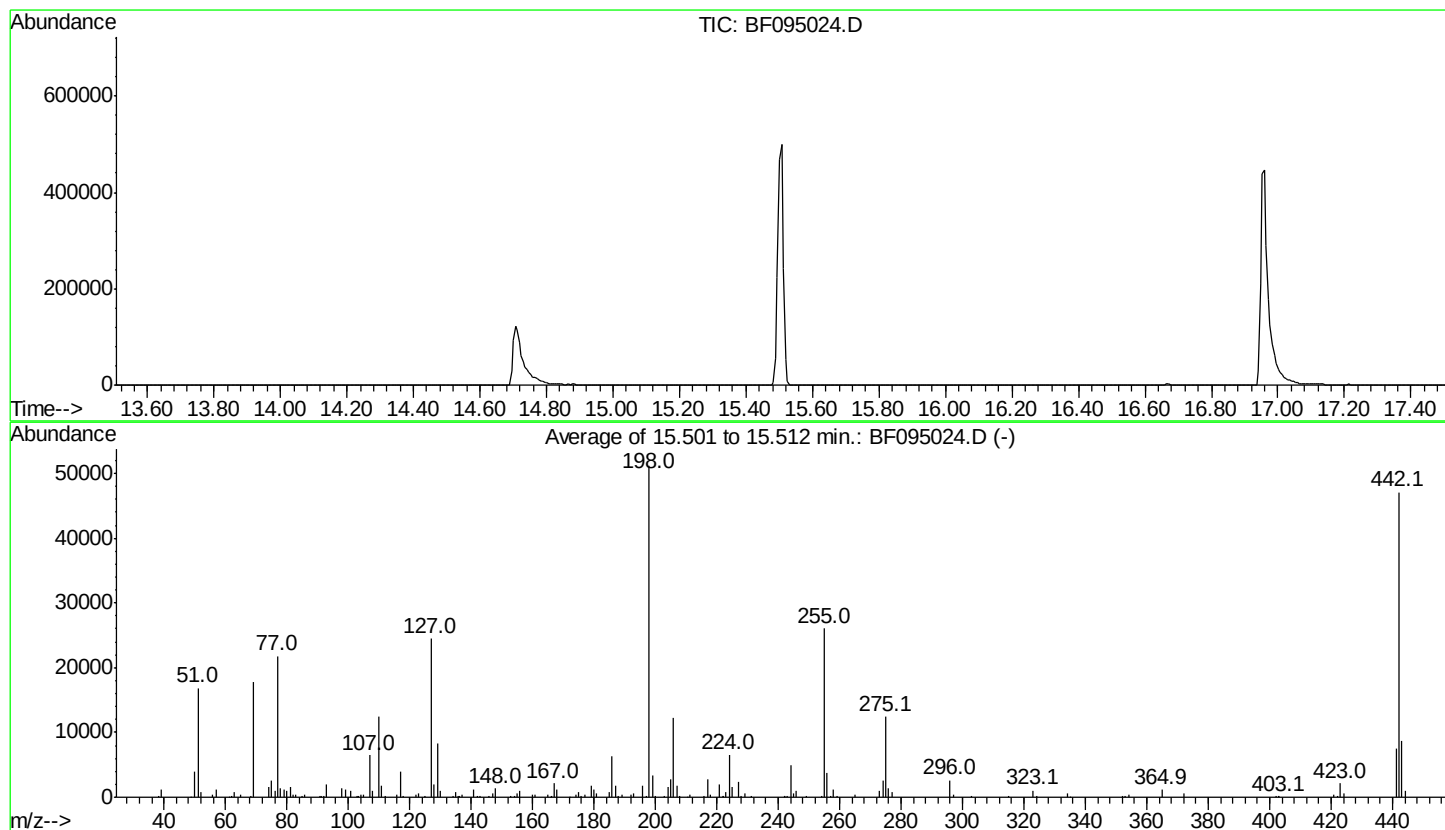

AutoFind: Scans 2306, 2307, 2308; Background Corrected with Scan 2300

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	16887	PASS
68	69	0.00	2	0.9	157	PASS
69	198	0.00	100	34.8	17833	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	24457	PASS
197	198	0.00	2	0.6	293	PASS
198	198	100	100	100.0	51197	PASS
199	198	5	9	6.4	3296	PASS
275	198	10	60	24.2	12403	PASS
365	198	1	100	2.3	1168	PASS
441	442	0.01	24	16.1	7585	PASS
442	198	50	100	92.0	47096	PASS
443	442	15	24	18.4	8675	PASS