

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
 Data File : BF128151.D
 Acq On : 09 May 2022 16:12
 Operator : CG\JU
 Sample : PB144686BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144686BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	546	550	553	rBV	2196468	2135842	48.94%	9.736%
2	6.516	714	719	722	rBV	1968179	2192444	50.24%	9.994%
3	6.893	779	783	786	rBV	685606	600898	13.77%	2.739%
4	7.457	873	879	882	rBV	1970548	2149921	49.26%	9.800%
5	8.175	996	1001	1004	rBV	819806	833409	19.10%	3.799%
6	9.251	1177	1184	1187	rBV	3519117	3821610	87.57%	17.420%
7	9.934	1294	1300	1303	rBV	1069764	985304	22.58%	4.491%
8	10.728	1428	1435	1438	rBV	1842380	1782028	40.83%	8.123%
9	11.428	1547	1554	1557	rBV	1144949	1070361	24.53%	4.879%
10	13.016	1819	1824	1827	rBV	4051826	4364077	100.00%	19.892%
11	14.069	1999	2003	2007	rBV	1114291	1007929	23.10%	4.594%
12	14.163	2013	2019	2025	rVB	60578	65649	1.50%	0.299%
13	15.569	2252	2258	2264	rBV	745283	929134	21.29%	4.235%




Sum of corrected areas: 21938606

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128151.D
Acq On : 09 May 2022 16:12
Operator : CG\JU
Sample : PB144686BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144686BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

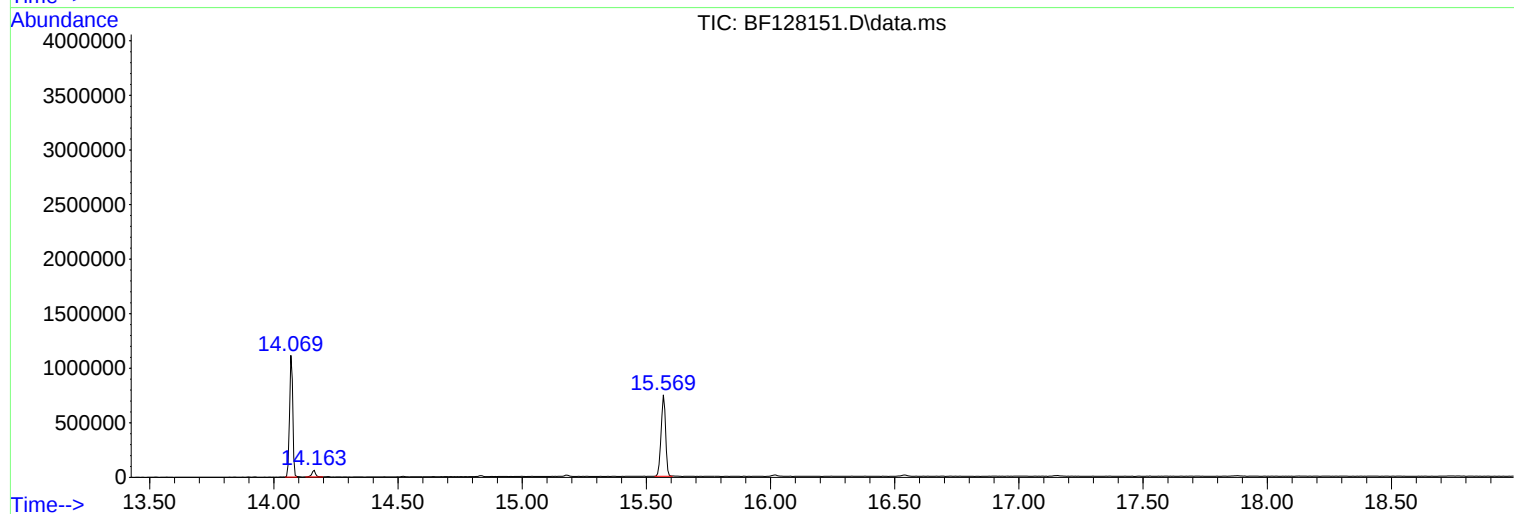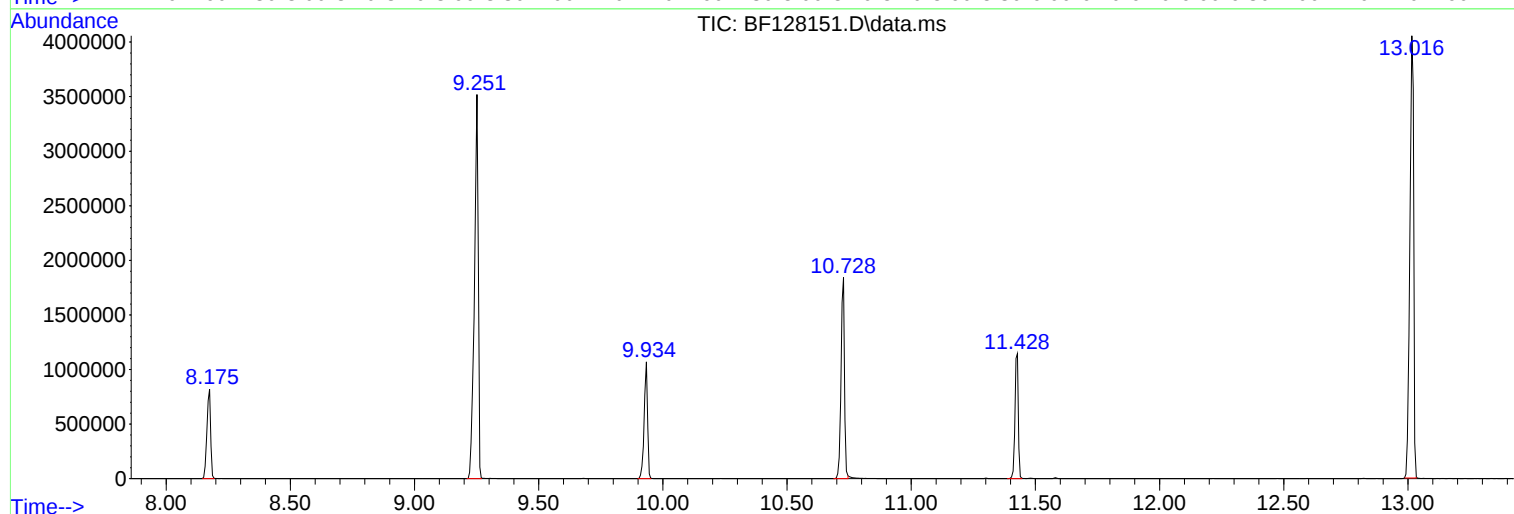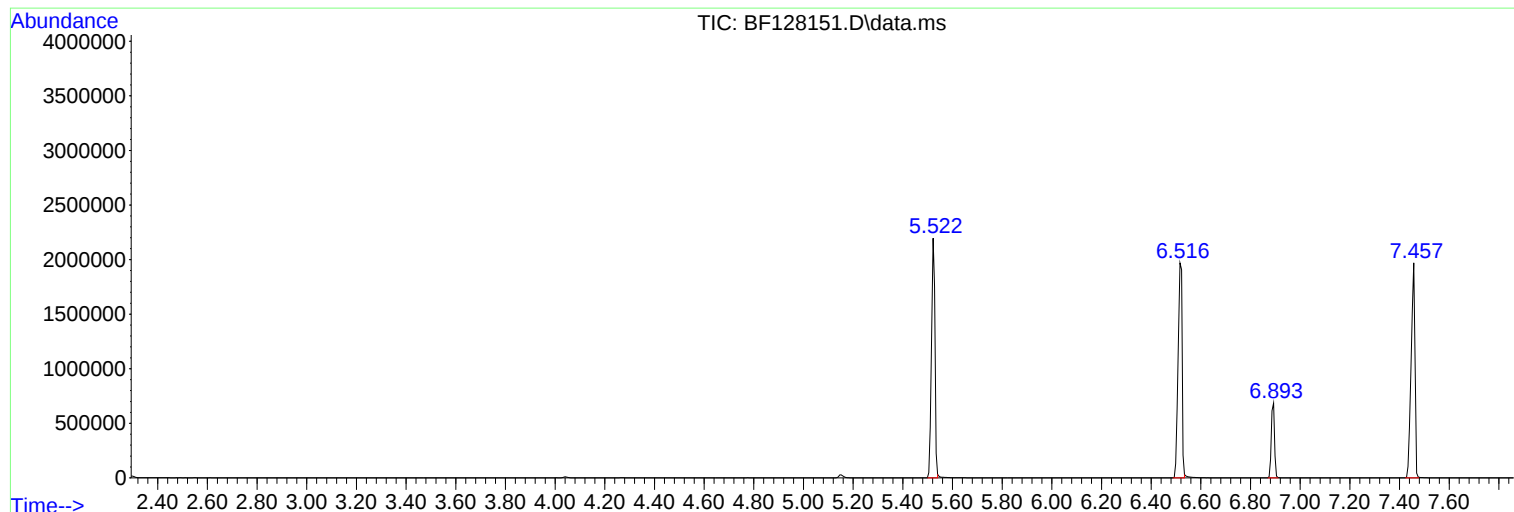

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128151.D
Acq On : 09 May 2022 16:12
Operator : CG\JU
Sample : PB144686BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144686BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128151.D
Acq On : 09 May 2022 16:12
Operator : CG\JU
Sample : PB144686BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144686BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------