

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
 Data File : BF128154.D
 Acq On : 09 May 2022 17:50
 Operator : CG\JU
 Sample : N2741-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	543	547	559	rBV	904975	782821	25.48%	5.461%
2	6.510	715	718	725	rBV	597289	509737	16.59%	3.556%
3	6.892	779	783	786	rBV	484376	424036	13.80%	2.958%
4	7.457	874	879	882	rBV	1739065	1608719	52.36%	11.223%
5	8.175	997	1001	1004	rBV	701235	561459	18.28%	3.917%
6	9.251	1179	1184	1187	rBV	3231572	2839127	92.41%	19.806%
7	9.345	1198	1200	1207	rVB	45608	41155	1.34%	0.287%
8	9.933	1296	1300	1303	rBV	806570	665701	21.67%	4.644%
9	10.722	1430	1434	1438	rBV	1473908	1393894	45.37%	9.724%
10	10.822	1448	1451	1460	rVB	38890	43868	1.43%	0.306%
11	11.422	1549	1553	1557	rBV	845121	723982	23.57%	5.051%
12	11.933	1636	1640	1647	rBV	42131	54929	1.79%	0.383%
13	13.016	1819	1824	1827	rBV	3224399	3072205	100.00%	21.432%
14	13.927	1975	1979	1989	rVB8	19282	41153	1.34%	0.287%
15	14.068	1999	2003	2007	rBV	818439	693422	22.57%	4.837%
16	14.163	2014	2019	2025	rBV	261866	270026	8.79%	1.884%
17	15.563	2252	2257	2264	rBV	475612	608142	19.79%	4.243%




Sum of corrected areas: 14334376

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128154.D
Acq On : 09 May 2022 17:50
Operator : CG\JU
Sample : N2741-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

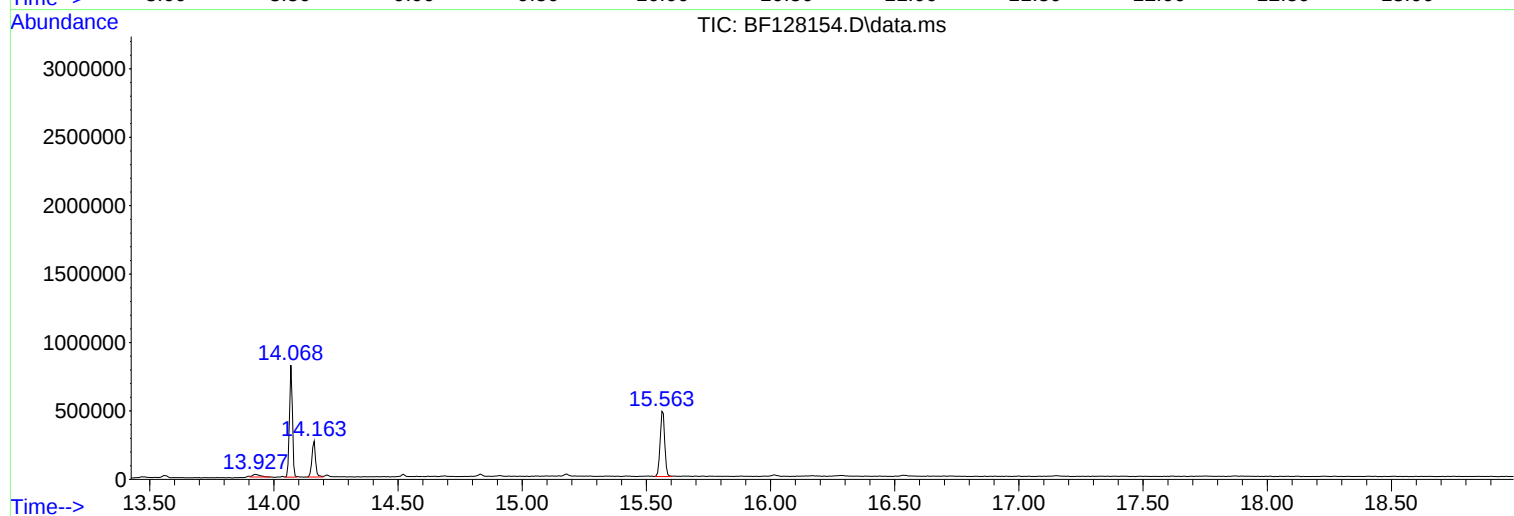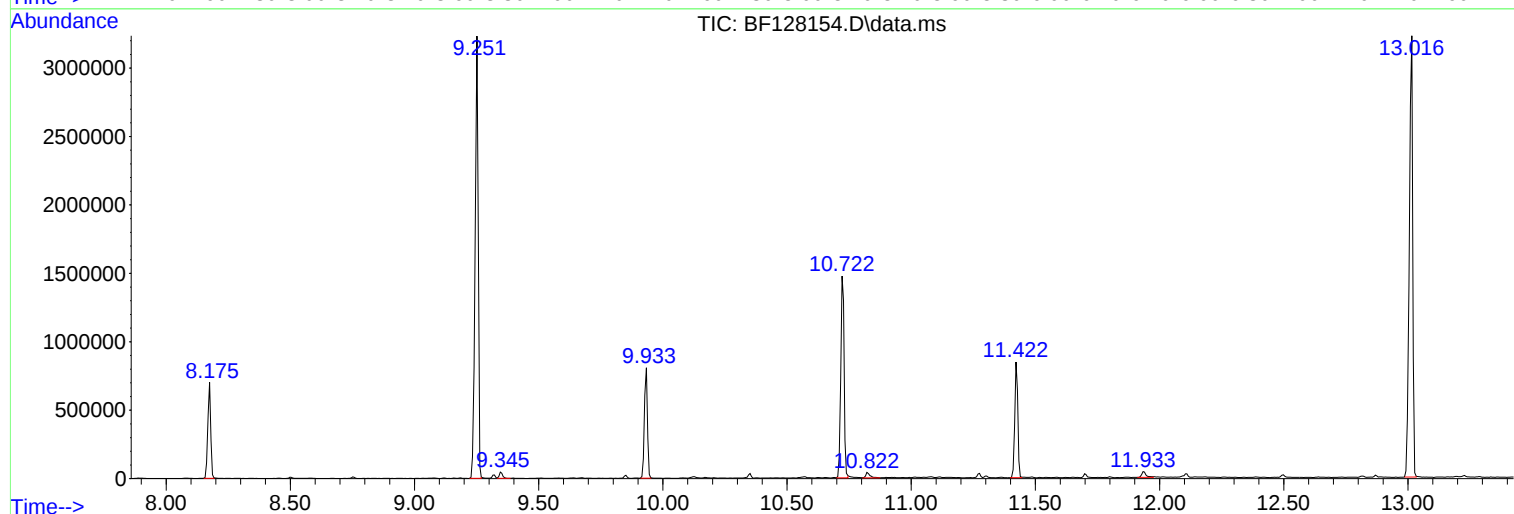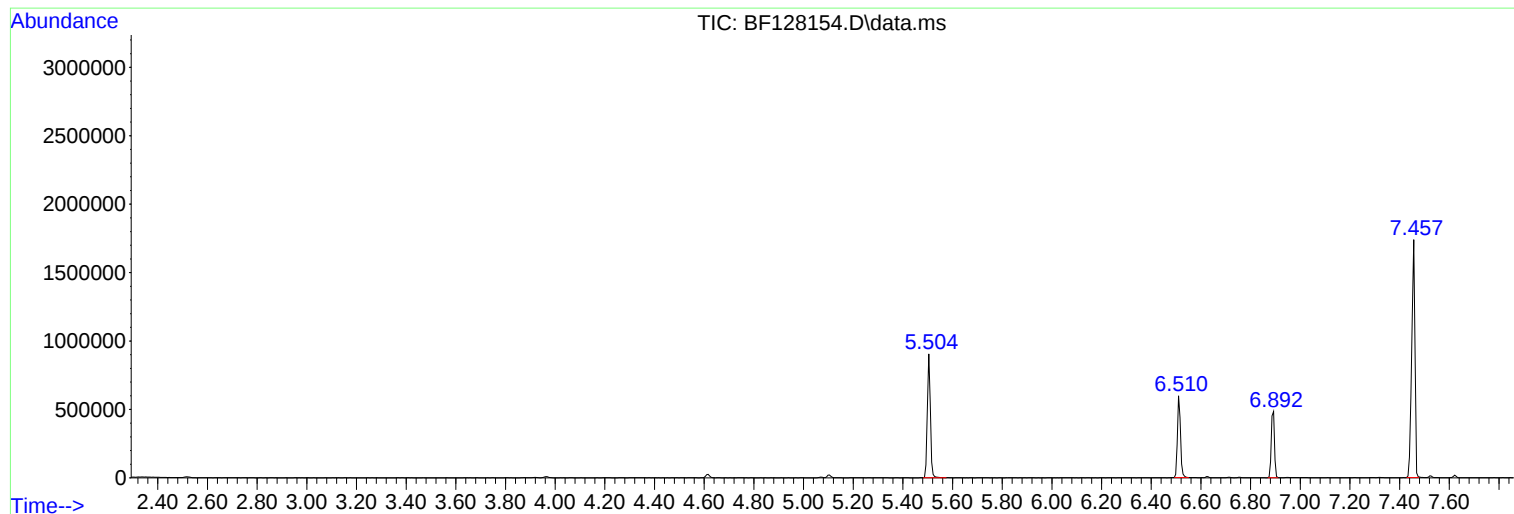

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128154.D
Acq On : 09 May 2022 17:50
Operator : CG\JU
Sample : N2741-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.163	7.79 ng	270026	Chrysene-d12	14.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	50
4			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	39
5			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19NO3Si	072101-35-0	37

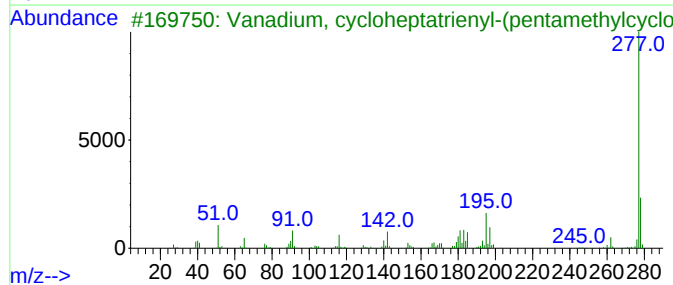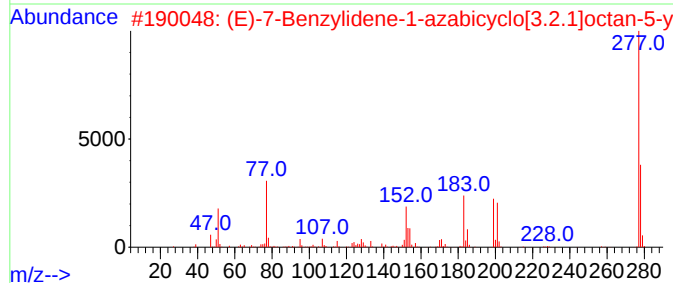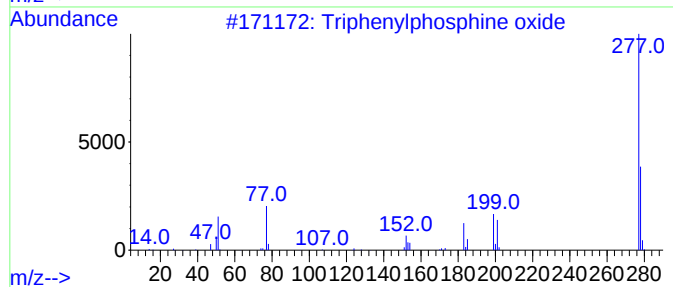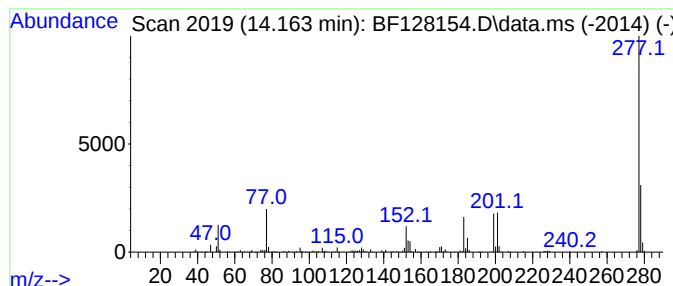

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128154.D
Acq On : 09 May 2022 17:50
Operator : CG\JU
Sample : N2741-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.163	7.8	ng	270026	5	14.069	693422	20.0