


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
 Data File : BF128140.D
 Acq On : 09 May 2022 10:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 15:30:11 2022

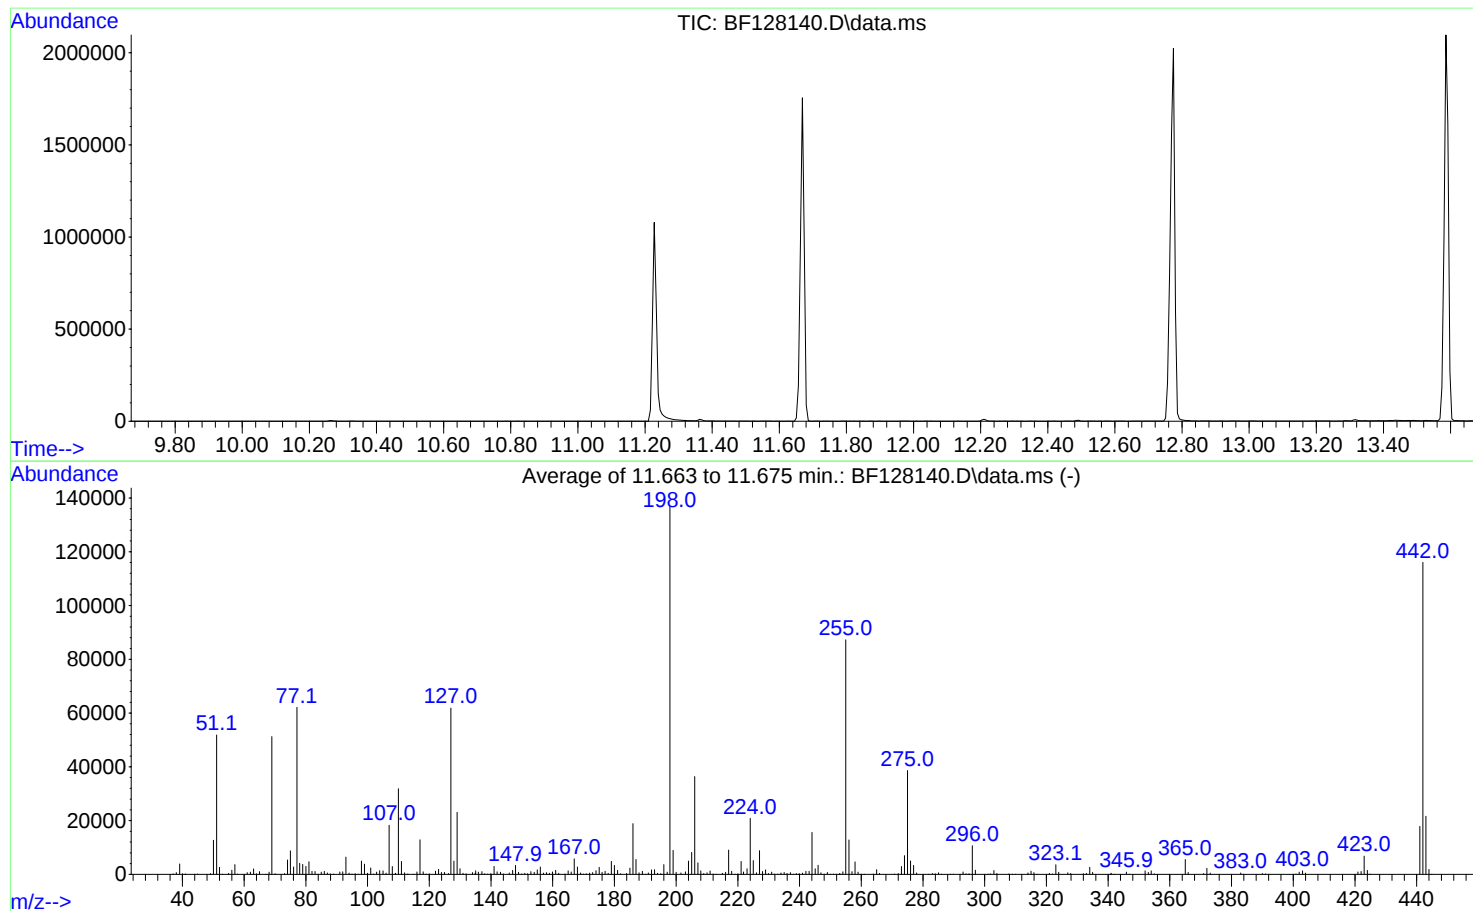




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	51819	PASS
68	69	0.00	2	1.7	866	PASS
69	198	0.00	100	37.5	51267	PASS
70	69	0.00	2	0.5	249	PASS
127	198	10	80	45.2	61845	PASS
197	198	0.00	2	0.6	819	PASS
198	198	100	100	100.0	136824	PASS
199	198	5	9	6.5	8942	PASS
275	198	10	60	28.2	38635	PASS
365	198	1	100	4.1	5567	PASS
441	198	0.01	100	13.1	17866	PASS
442	442	50	100	100.0	116051	PASS
443	442	15	24	18.6	21614	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
Data File : BF128140.D
Acq On : 09 May 2022 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 09 13:12:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 13:08:24 2022
Response via : Initial Calibration

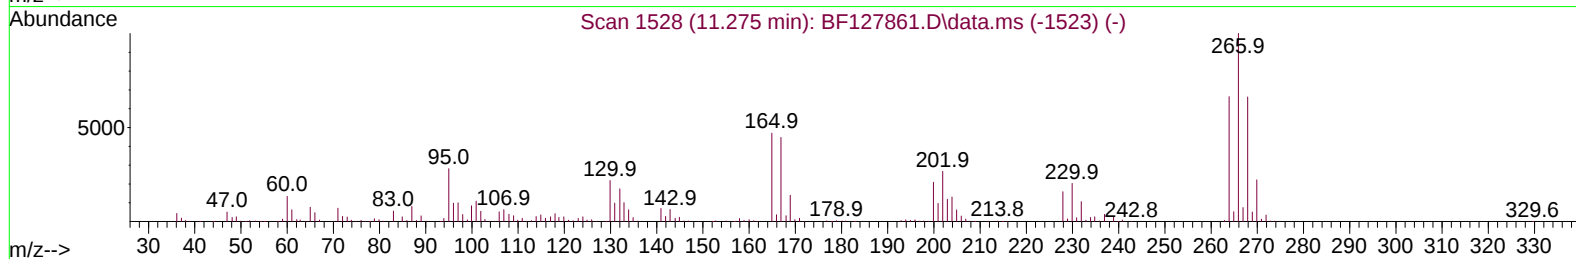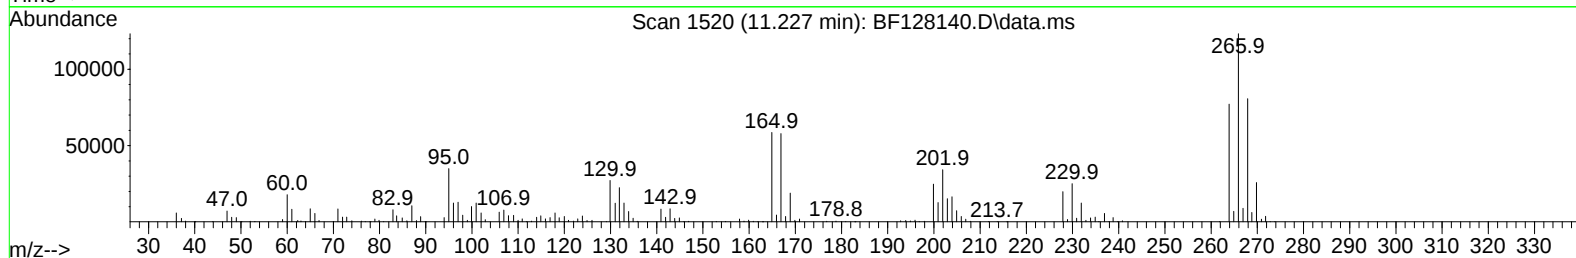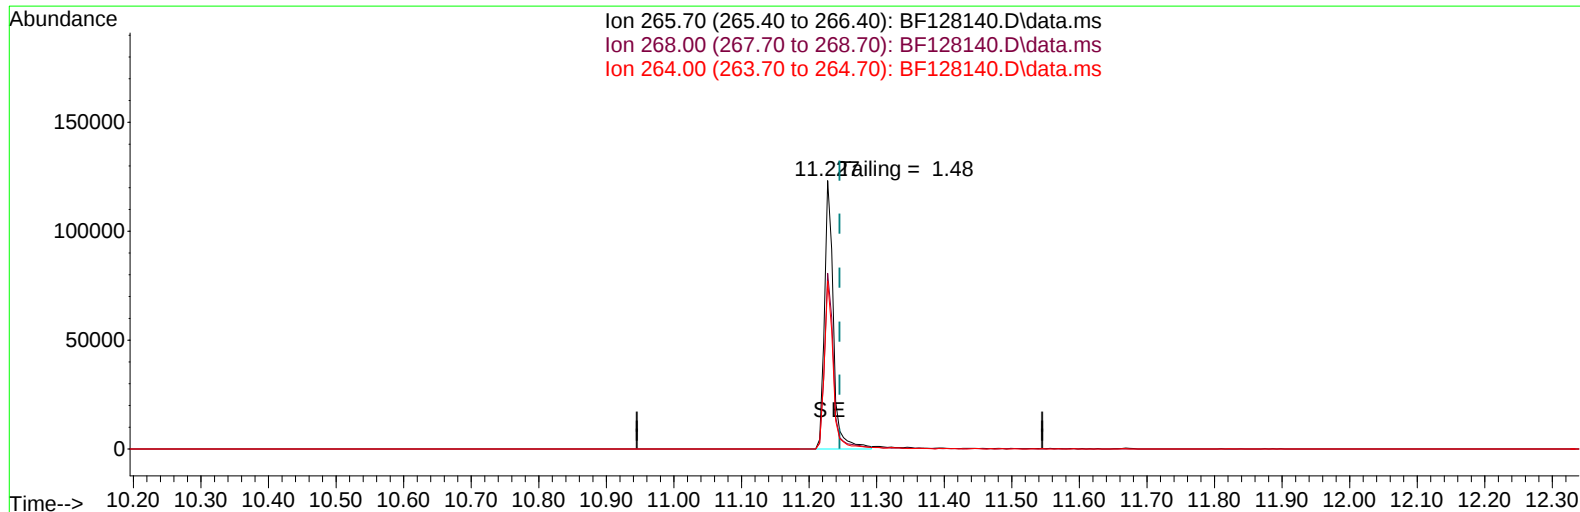

TIC: BF128140.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.018) 26203.54 ng




response 115051

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.45
264.00	66.40	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050922\
 Data File : BF128140.D
 Acq On : 09 May 2022 10:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 09 13:12:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 13:08:24 2022
 Response via : Initial Calibration

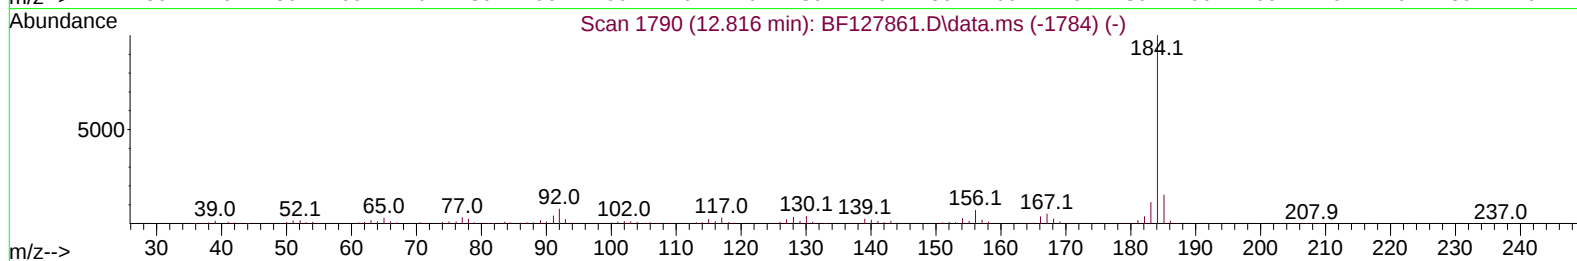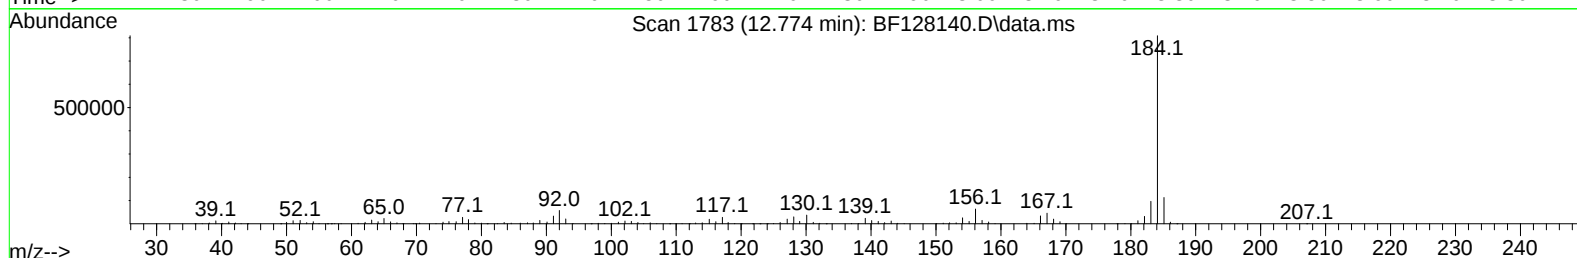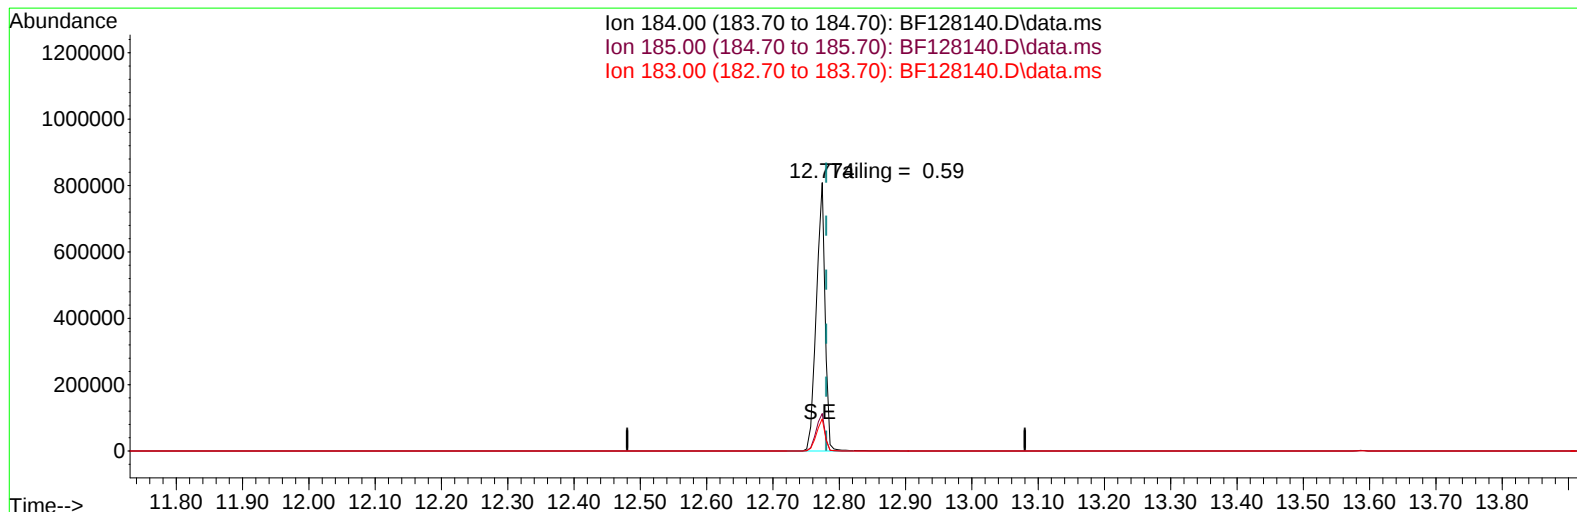

TIC: BF128140.D\data.ms

(77) Benzidine

12.774min (-0.006) 0.00 ng

response 745157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.94
183.00	11.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/9/2022	BNA_F	<u>BF128140.D</u>
Compound Name	Response	Retention Time
DDT	359809	13.58
DDD	691	13.28
DDE	271	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
962	360771	0.27

Instrument :
BNA_F
ClientSampleId :
DFTPP