
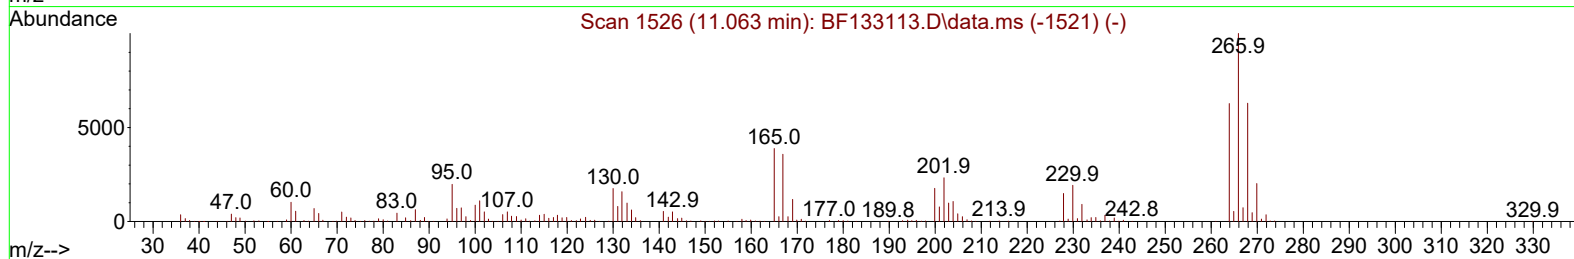
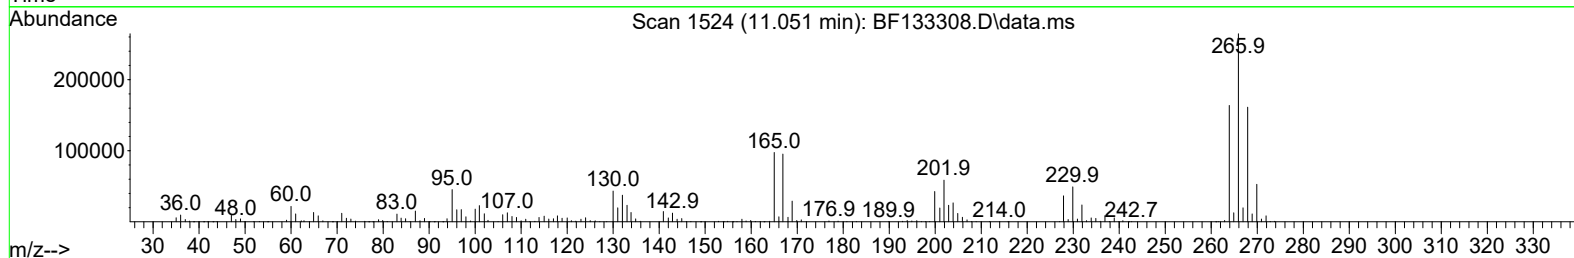


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133308.D
Acq On : 09 May 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 05:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

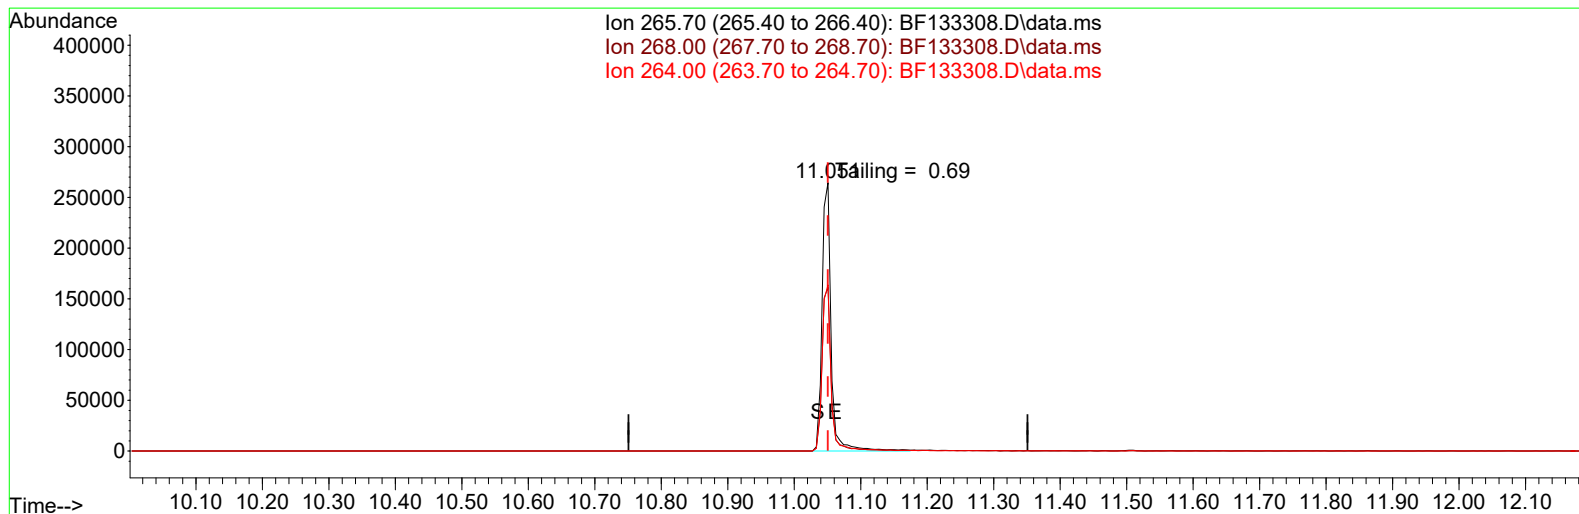

TIC: BF133308.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.000) 497745.26 ng

response 252133

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	60.93
264.00	63.30	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133308.D
Acq On : 09 May 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 05:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

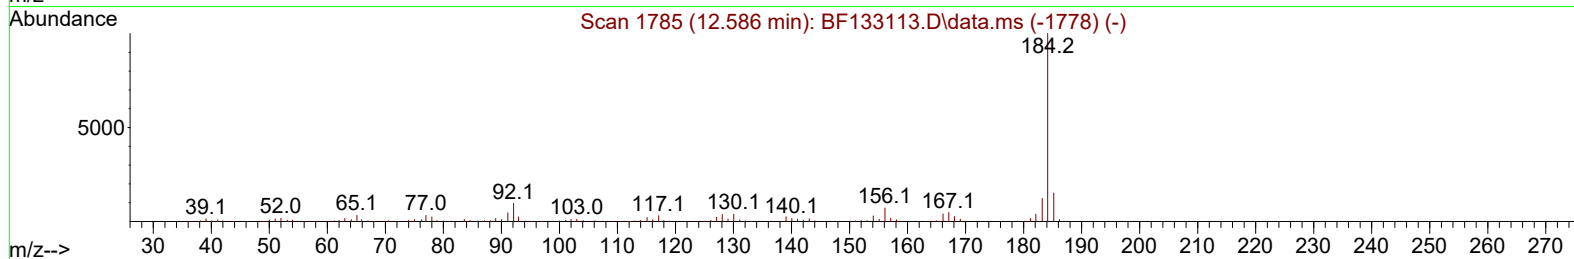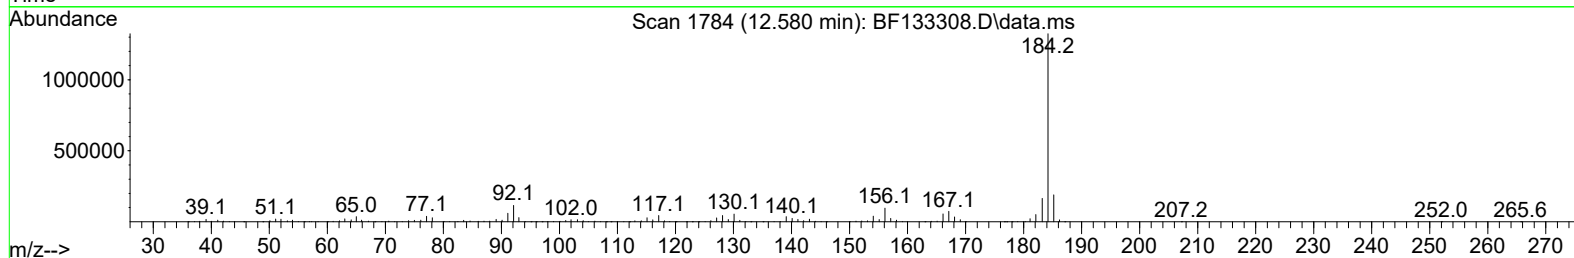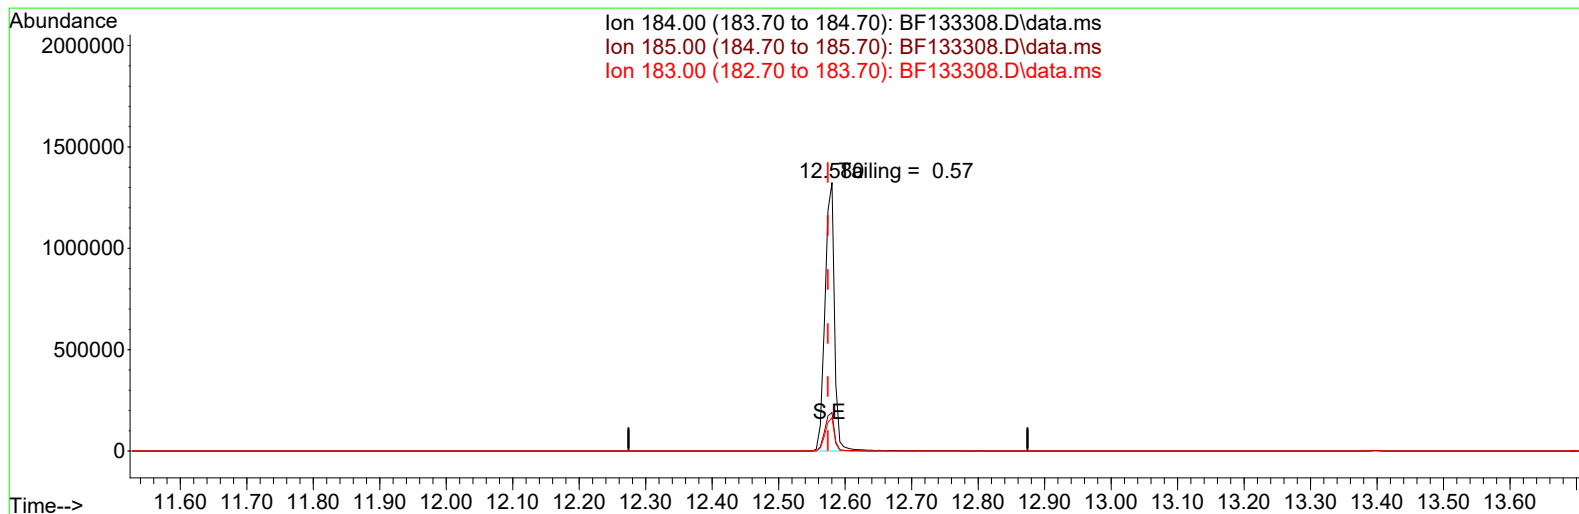

TIC: BF133308.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 0.00 ng

response 1313324

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.34#
183.00	11.70	12.40
0.00	0.00	0.00