

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
 Data File : BF133310.D
 Acq On : 09 May 2023 10:46
 Operator : CG\JU
 Sample : PB152628BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB152628BL

Quant Time: May 10 01:44:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 04:59:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.722	152	242848	20.000	ng	0.00
21) Naphthalene-d8	8.004	136	1011619	20.000	ng	0.00
39) Acenaphthene-d10	9.757	164	548274	20.000	ng	0.00
64) Phenanthrene-d10	11.239	188	994271	20.000	ng	0.00
76) Chrysene-d12	13.874	240	678828	20.000	ng	0.00
86) Perylene-d12	15.292	264	567141	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.345	112	1872348	116.467	ng	0.02
7) Phenol-d6	6.369	99	2277852	114.156	ng	0.00
23) Nitrobenzene-d5	7.292	82	1413066	75.397	ng	0.00
42) 2,4,6-Tribromophenol	10.551	330	569304	103.248	ng	0.00
45) 2-Fluorobiphenyl	9.086	172	2265471	69.128	ng	0.00
79) Terphenyl-d14	12.833	244	2659799	67.576	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133310.D
Acq On : 09 May 2023 10:46
Operator : CG\JU
Sample : PB152628BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB152628BL

Quant Time: May 10 01:44:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration




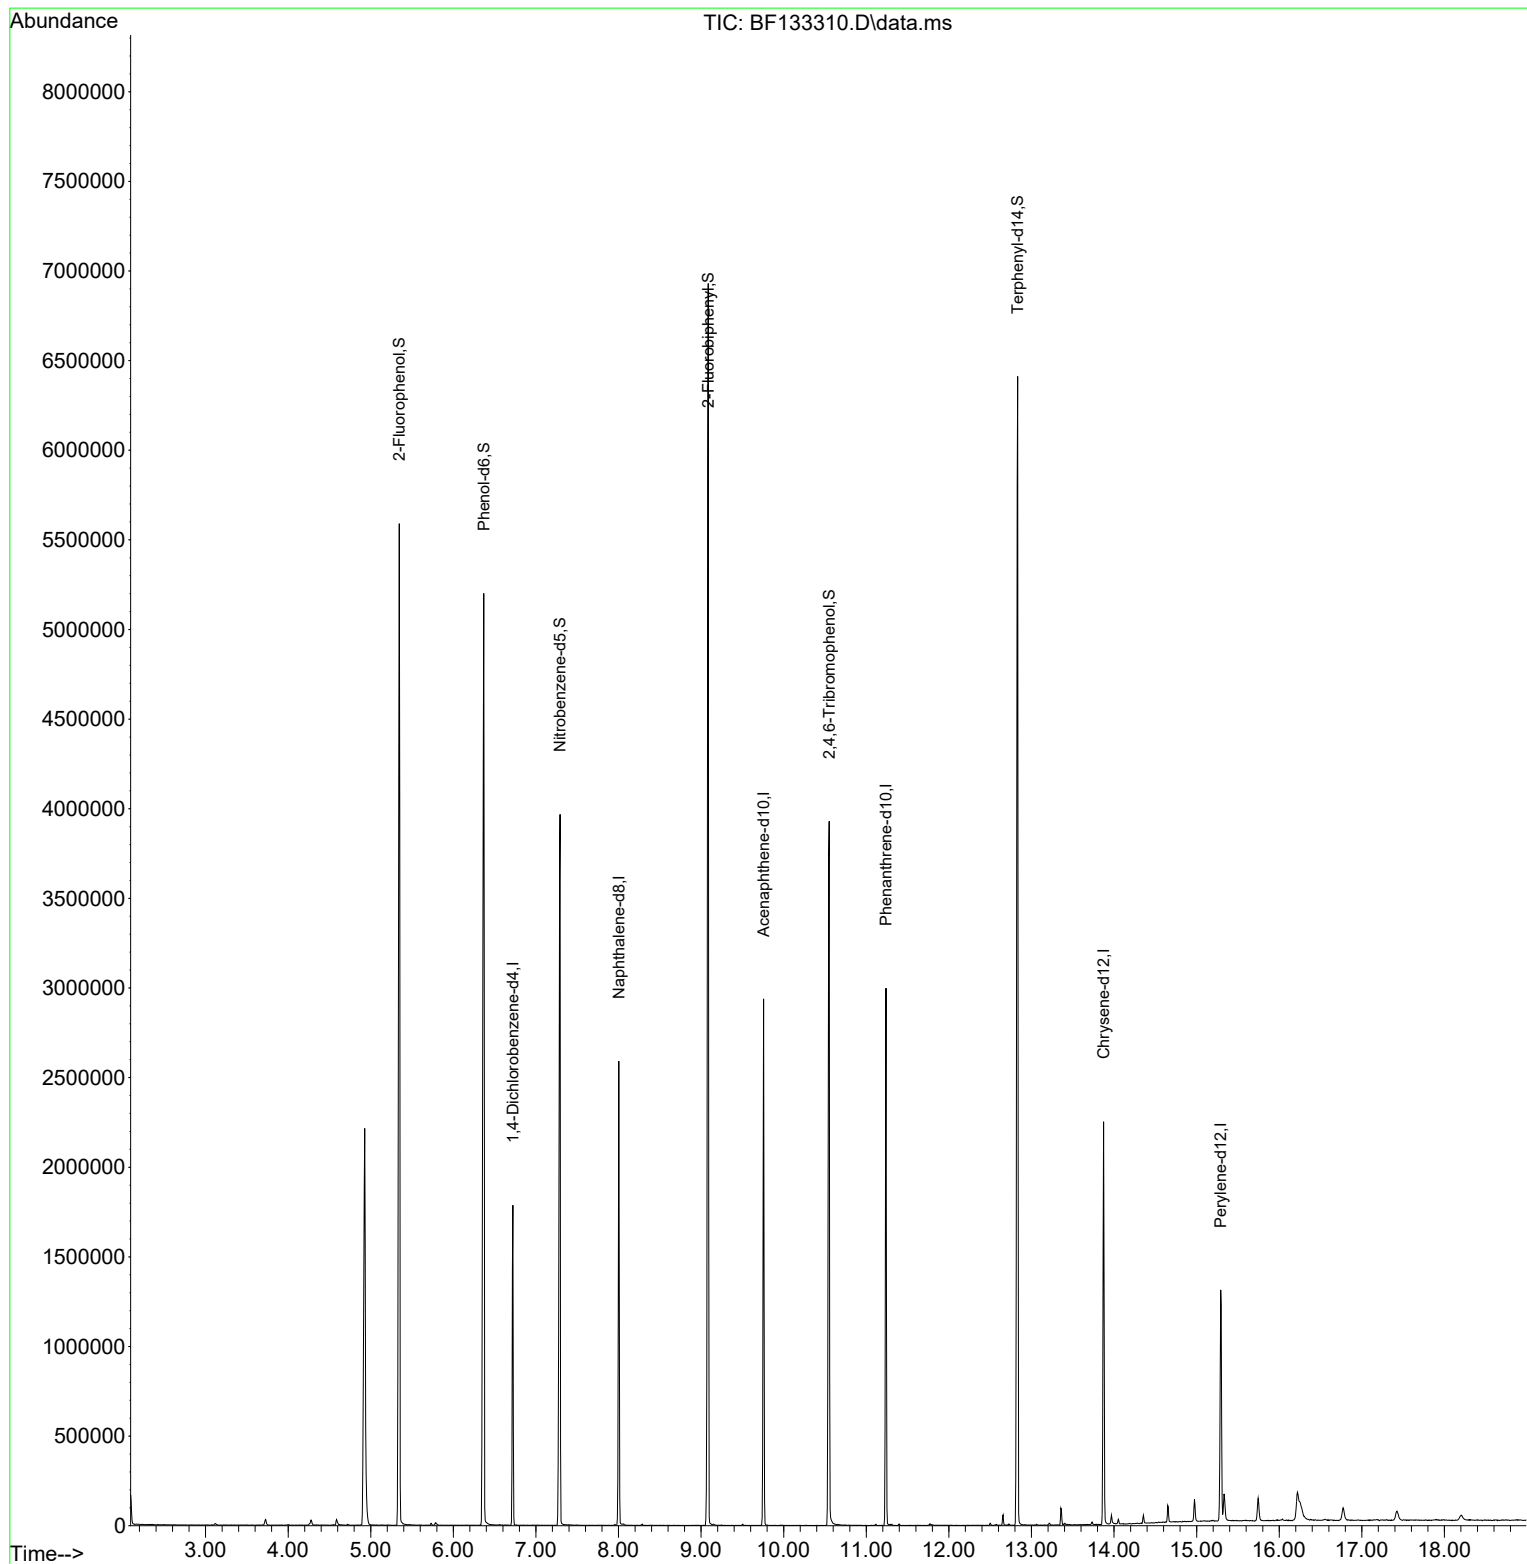


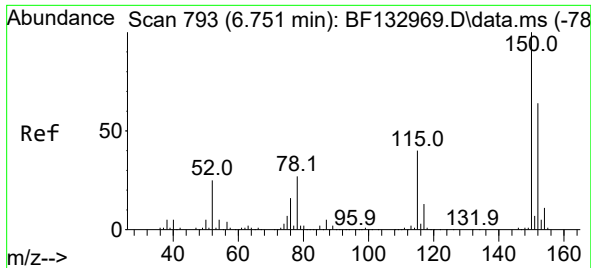

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.722 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46




Instrument :
BNA_F
ClientSampleId :
PB152628BL

Tgt Ion:152 Resp: 242848
Ion Ratio Lower Upper
152 100
150 155.3 124.8 187.2
115 59.8 49.9 74.9

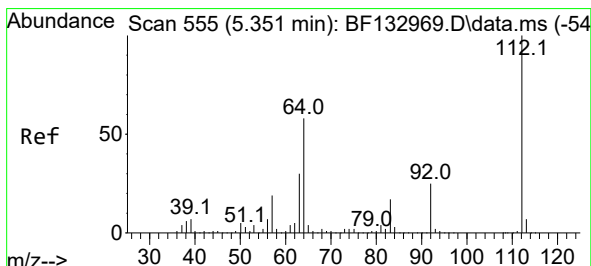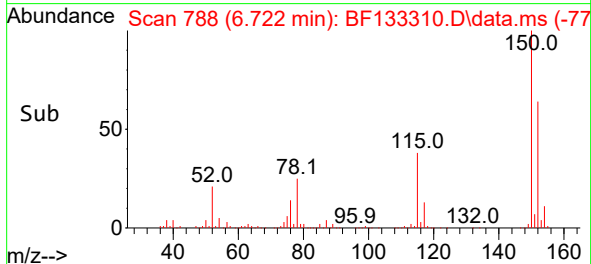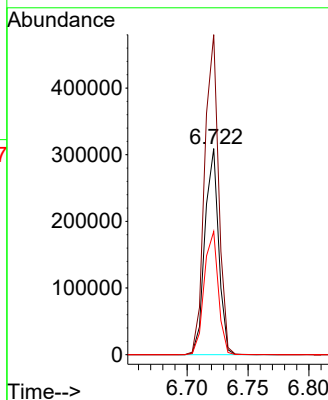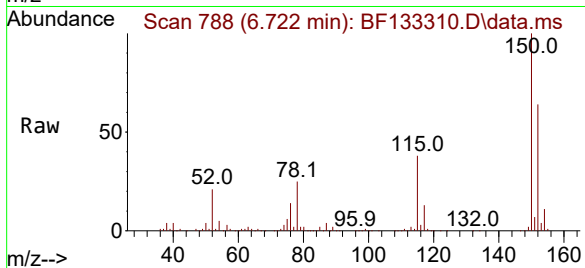

#5
2-Fluorophenol
Concen: 116.467 ng
RT: 5.345 min Scan# 554
Delta R.T. 0.018 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46

Tgt Ion:112 Resp: 1872348
Ion Ratio Lower Upper
112 100
64 55.2 46.8 70.2
63 29.3 23.8 35.8


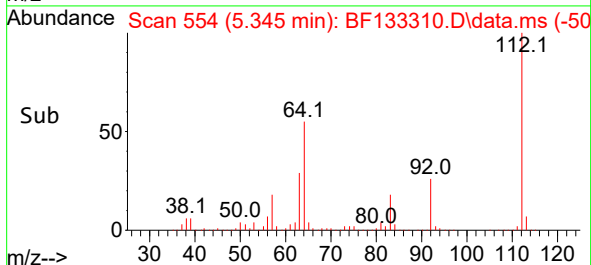
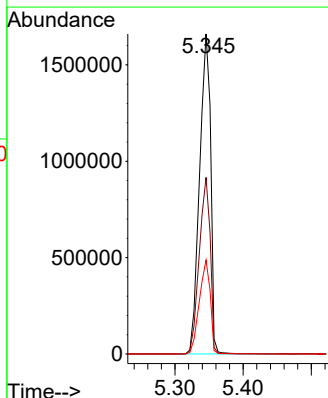
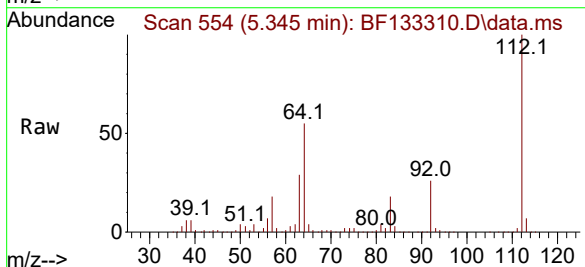




#7
Phenol-d6
Concen: 114.156 ng
RT: 6.369 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46




Instrument :
BNA_F
ClientSampleId :
PB152628BL


Tgt Ion: 99 Resp: 2277852
Ion Ratio Lower Upper
99 100
42 18.5 16.3 24.5
71 32.0 25.6 38.4

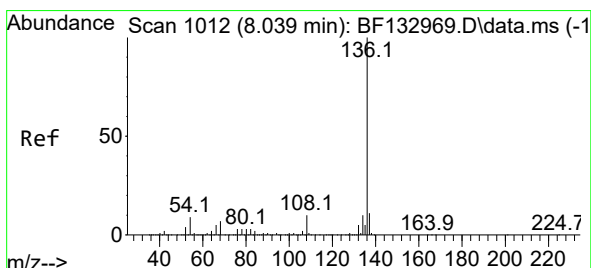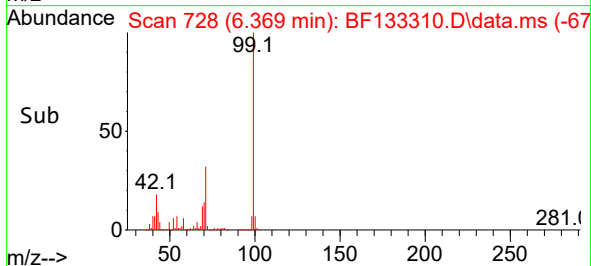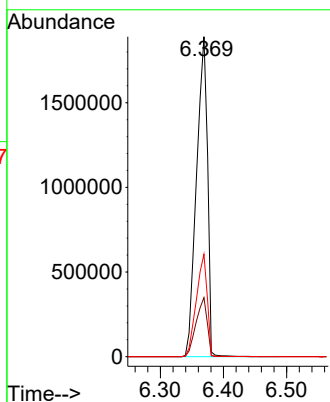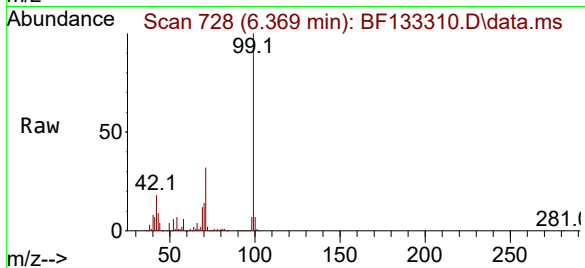

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46

Tgt Ion: 136 Resp: 1011619
Ion Ratio Lower Upper
136 100
137 11.4 8.6 13.0
54 9.0 7.0 10.4
68 7.0 5.4 8.2


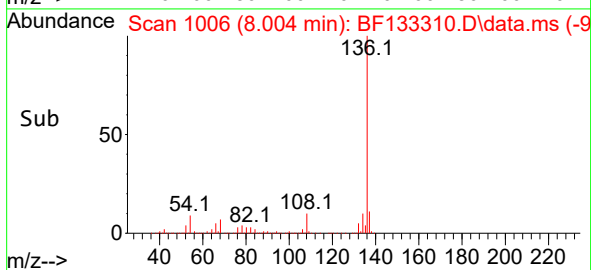
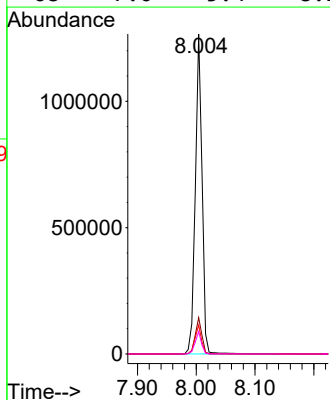
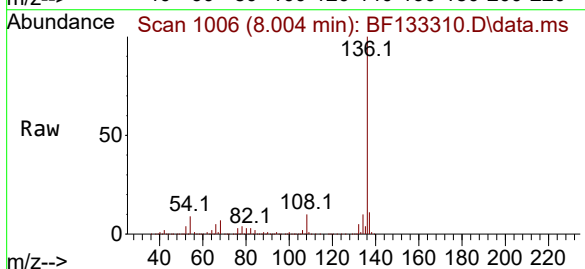


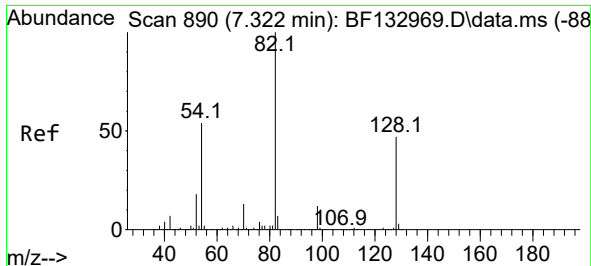

#23
Nitrobenzene-d5
Concen: 75.397 ng
RT: 7.292 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46




Instrument :
BNA_F
ClientSampleId :
PB152628BL


Tgt Ion: 82 Resp: 1413066
Ion Ratio Lower Upper
82 100
128 51.1 37.7 56.5
54 50.1 43.0 64.4

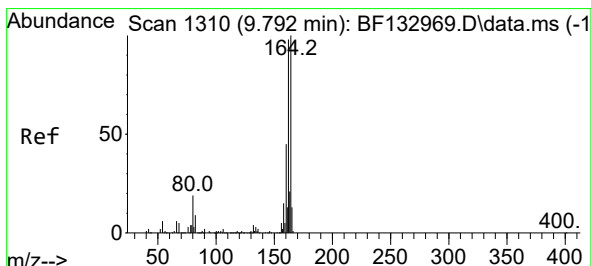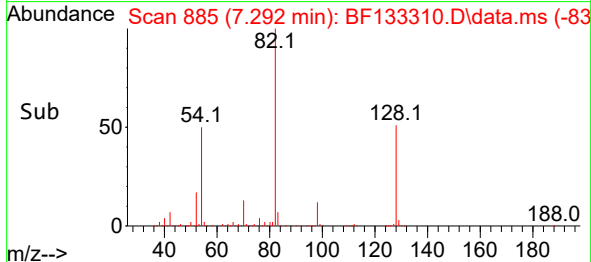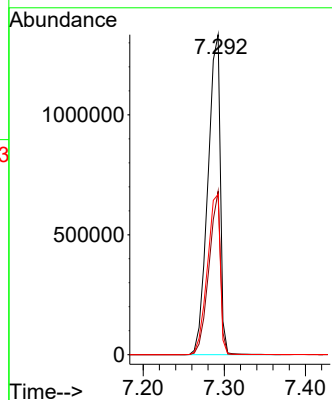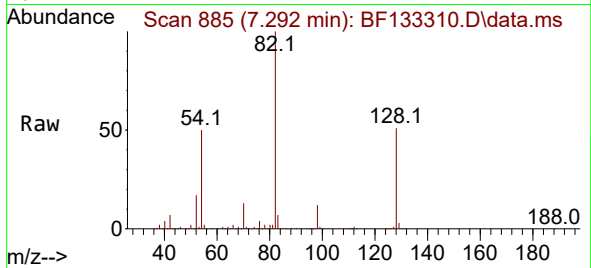

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.757 min Scan# 1304
Delta R.T. -0.006 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46

Tgt Ion: 164 Resp: 548274
Ion Ratio Lower Upper
164 100
162 99.6 78.7 118.1
160 44.3 35.8 53.6

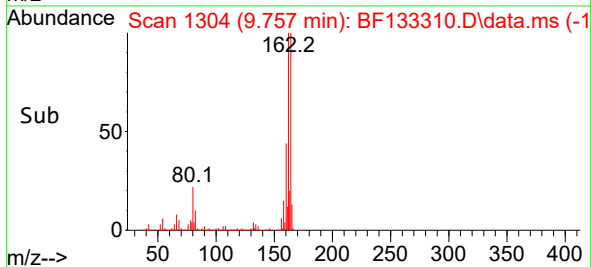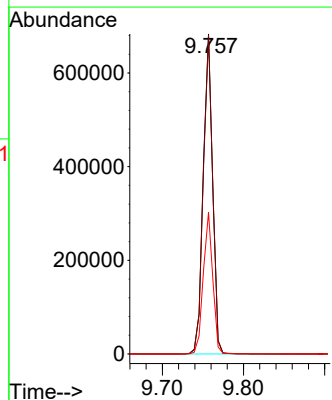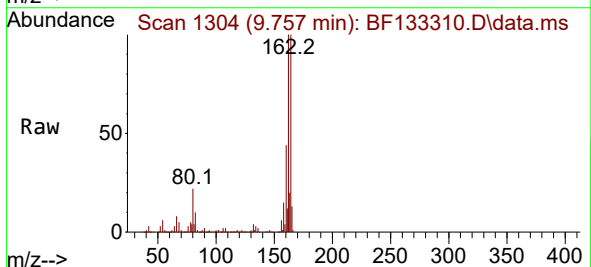

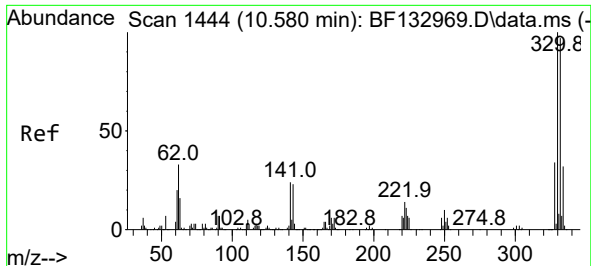

#42

2,4,6-Tribromophenol

Concen: 103.248 ng

RT: 10.551 min Scan# 1444

Delta R.T. 0.000 min

Lab File: BF133310.D

Acq: 09 May 2023 10:46

Instrument :

BNA_F

ClientSampleId :

PB152628BL





Tgt Ion:330 Resp: 569304

Ion Ratio Lower Upper

330 100

332 97.0 77.1 115.7

141 30.6 25.8 38.8

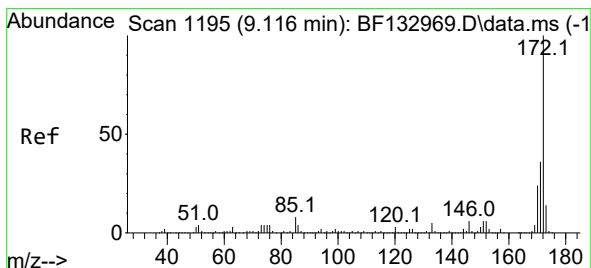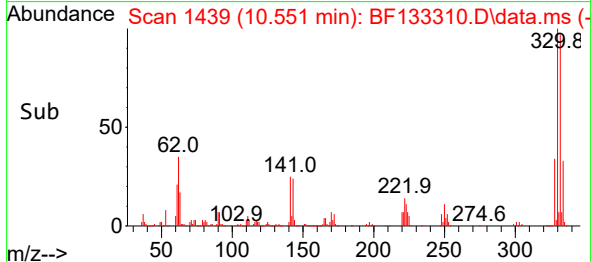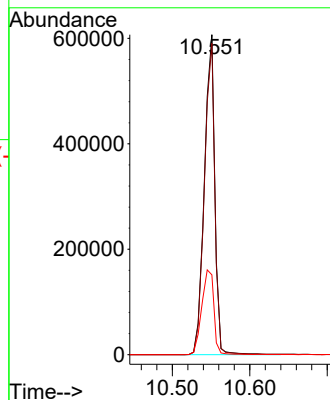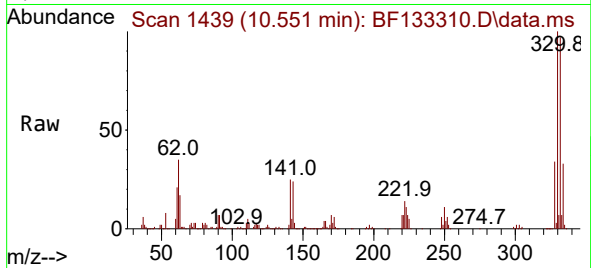

#45

2-Fluorobiphenyl

Concen: 69.128 ng

RT: 9.086 min Scan# 1190

Delta R.T. 0.000 min

Lab File: BF133310.D

Acq: 09 May 2023 10:46




Tgt Ion:172 Resp: 2265471


Ion Ratio Lower Upper

172 100

171 36.4 28.8 43.2

170 24.5 19.4 29.2


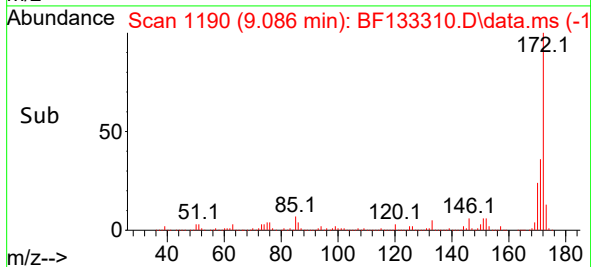
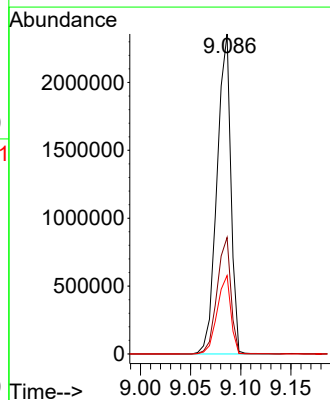
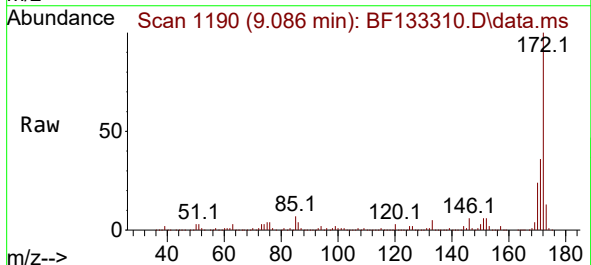


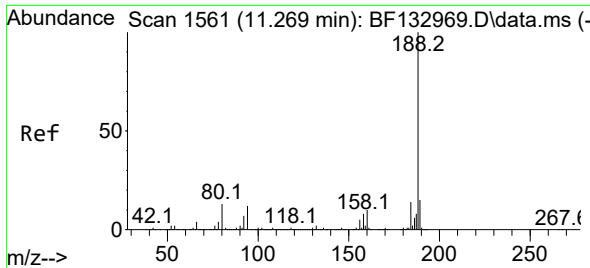

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.239 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46




Instrument :
BNA_F
ClientSampleId :
PB152628BL


Tgt Ion:188 Resp: 994271
Ion Ratio Lower Upper
188 100
94 10.9 9.7 14.5
80 11.6 10.4 15.6

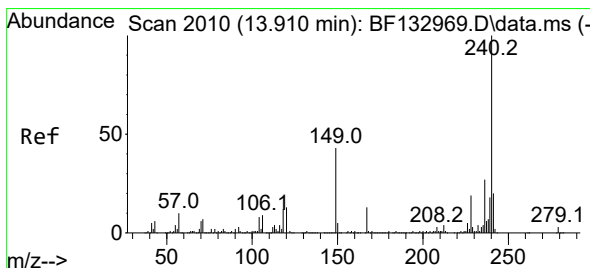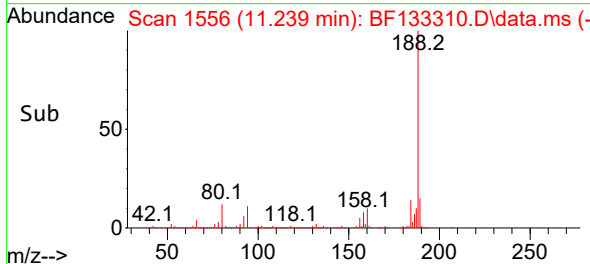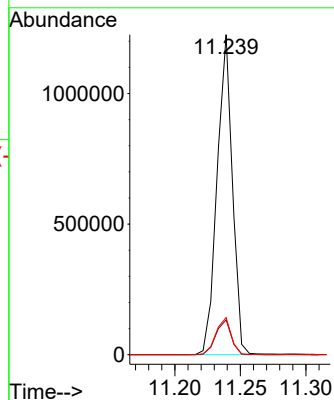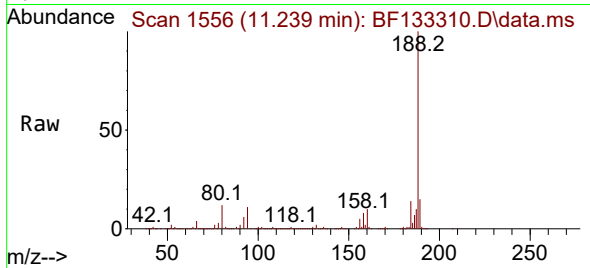

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.874 min Scan# 2004
Delta R.T. -0.006 min
Lab File: BF133310.D
Acq: 09 May 2023 10:46

Tgt Ion:240 Resp: 678828
Ion Ratio Lower Upper
240 100
120 13.1 10.5 15.7
236 26.5 21.5 32.3


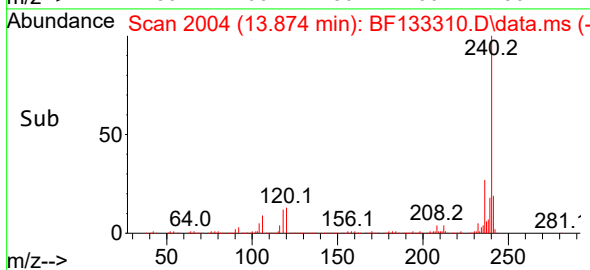
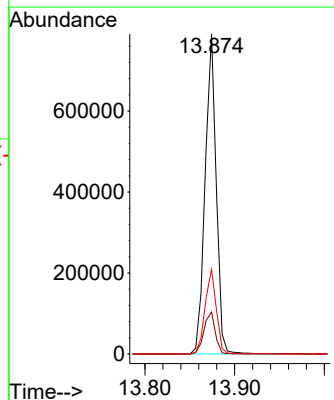
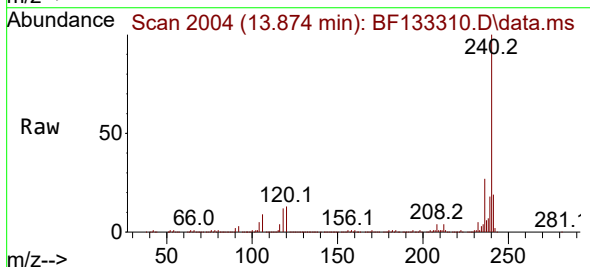


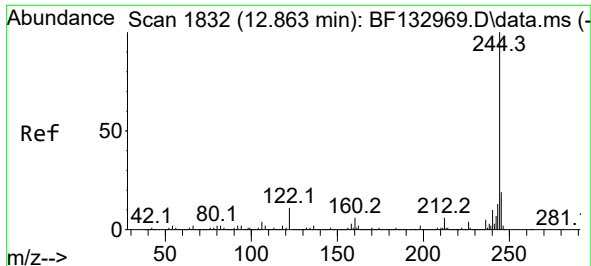

#79
 Terphenyl-d14
 Concen: 67.576 ng
 RT: 12.833 min Scan# 1827
 Delta R.T. 0.000 min
 Lab File: BF133310.D
 Acq: 09 May 2023 10:46

Instrument :
 BNA_F
 ClientSampleId :
 PB152628BL

Tgt Ion:244 Resp: 2659799
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.1 7.7
 122 11.3 8.6 13.0

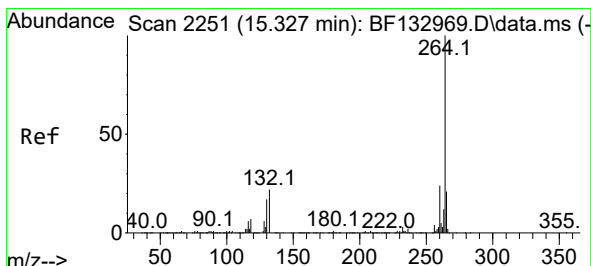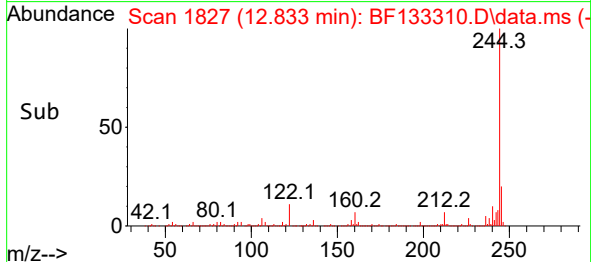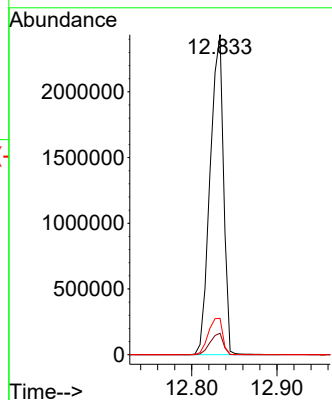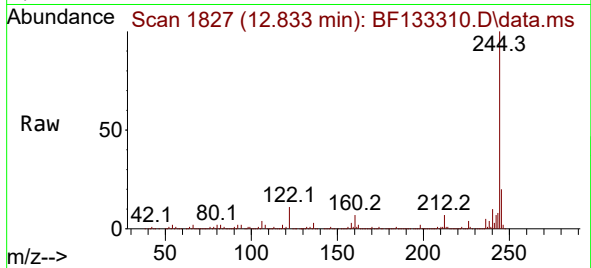

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.292 min Scan# 2245
 Delta R.T. 0.000 min
 Lab File: BF133310.D
 Acq: 09 May 2023 10:46

Tgt Ion:264 Resp: 567141
 Ion Ratio Lower Upper
 264 100
 260 24.4 18.8 28.2
 265 21.7 17.0 25.4

