
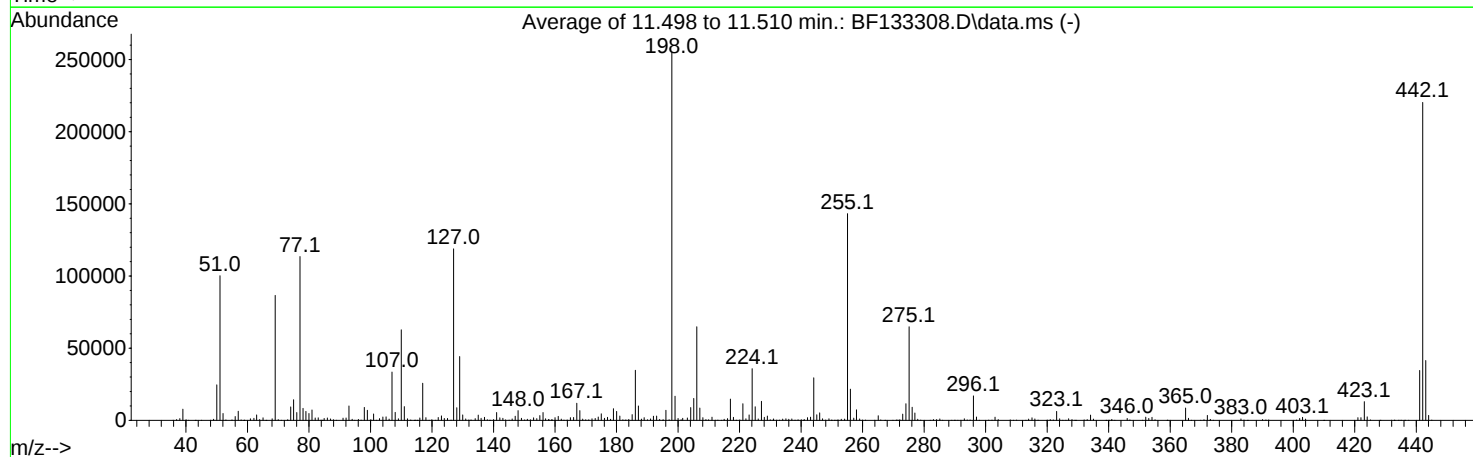


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133308.D
Acq On : 09 May 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 09 04:59:36 2023

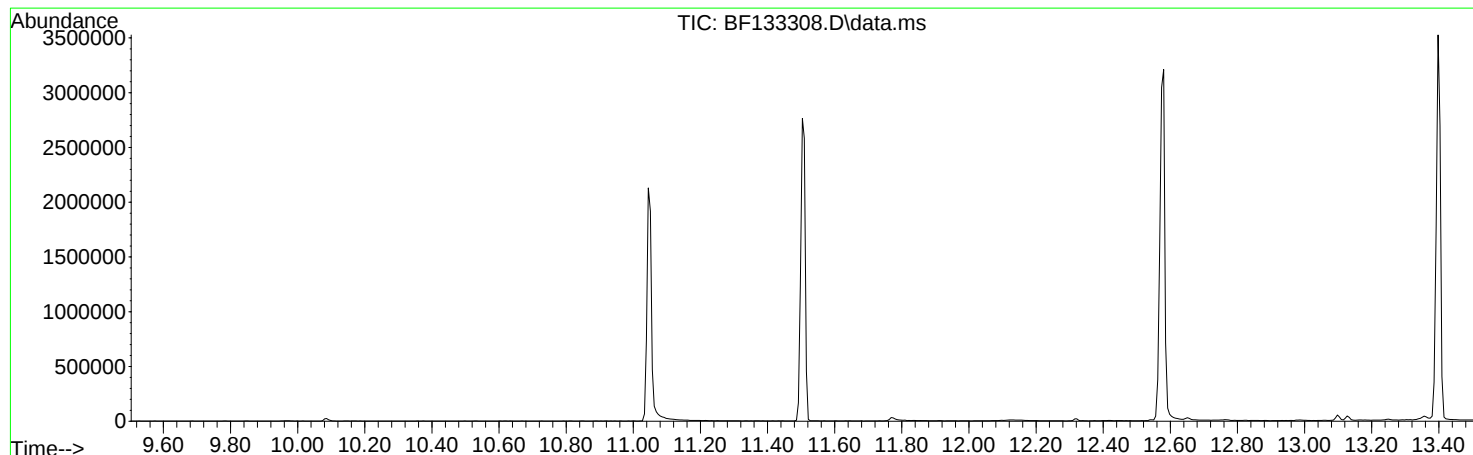

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	100211	PASS
68	69	0.00	2	1.3	1104	PASS
69	198	0.00	100	34.0	86565	PASS
70	69	0.00	2	0.7	590	PASS
127	198	10	80	46.6	118821	PASS
197	198	0.00	2	0.2	504	PASS
198	198	100	100	100.0	254869	PASS
199	198	5	9	6.6	16697	PASS
275	198	10	60	25.5	64896	PASS
365	198	1	100	3.4	8592	PASS
441	198	0.01	100	13.6	34562	PASS
442	442	50	100	100.0	220299	PASS
443	442	15	24	18.8	41479	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/9/2023	BNA_F	<u>BF133308.D</u>
Compound Name	Response	Retention Time
DDT	606590	13.398
DDD	13212	13.098
DDE	1274	12.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14486	621076	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133308.D
Acq On : 09 May 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 05:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

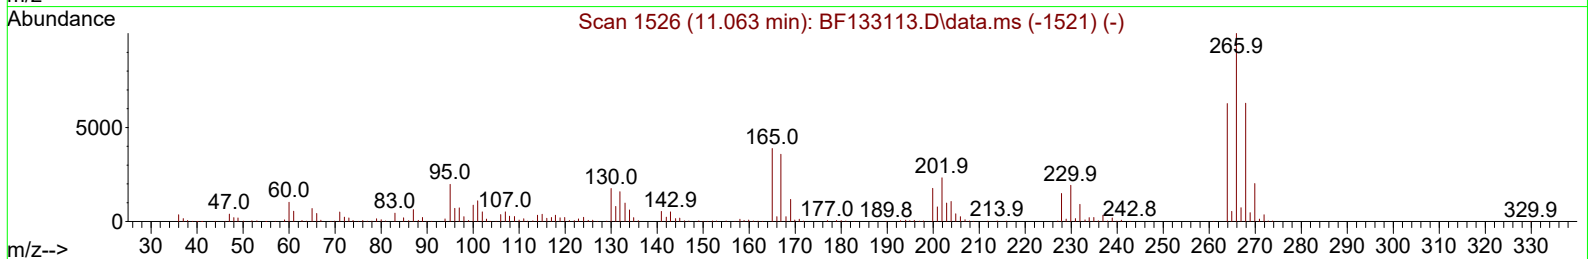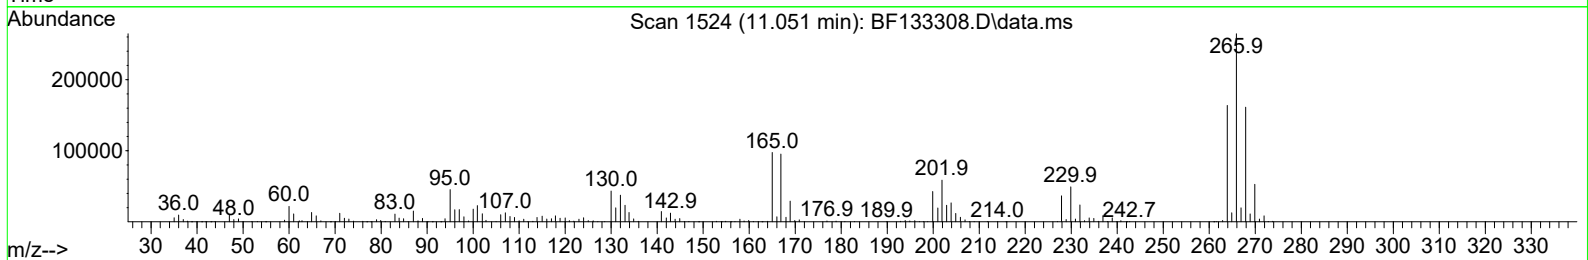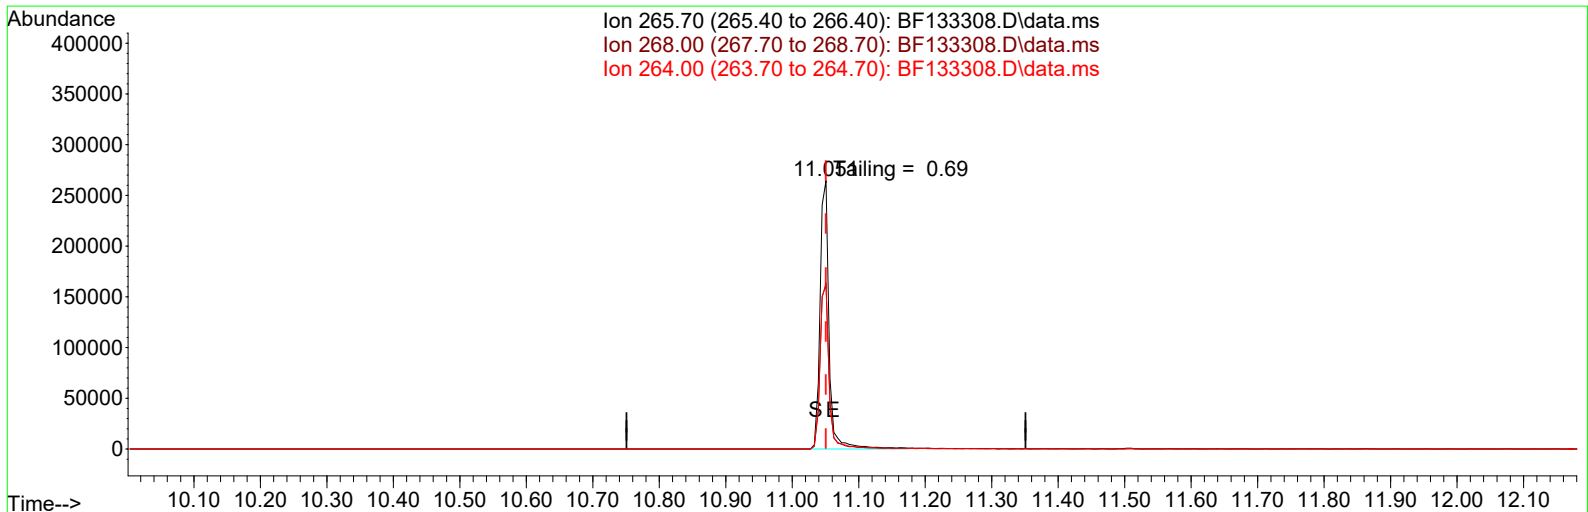

TIC: BF133308.D\data.ms

(70) Pentachlorophenol (C)

11.051min (-0.000) 497745.26 ng




response 252133

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	60.93
264.00	63.30	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050923\
Data File : BF133308.D
Acq On : 09 May 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 05:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

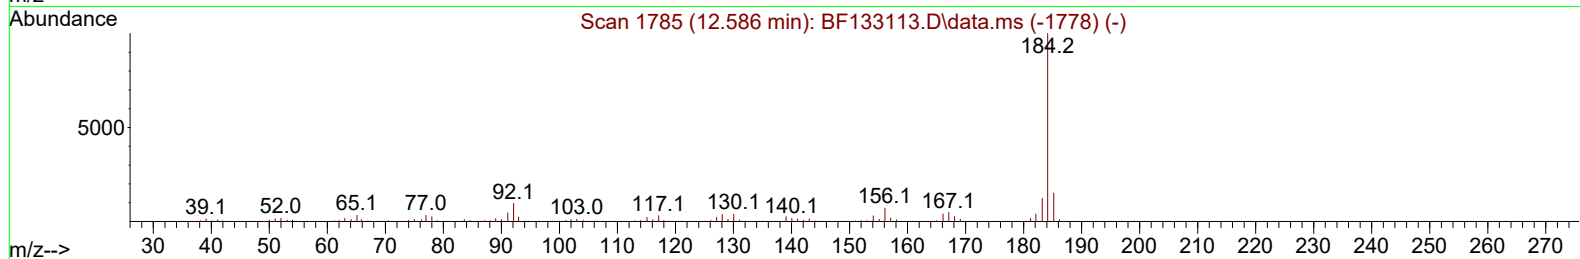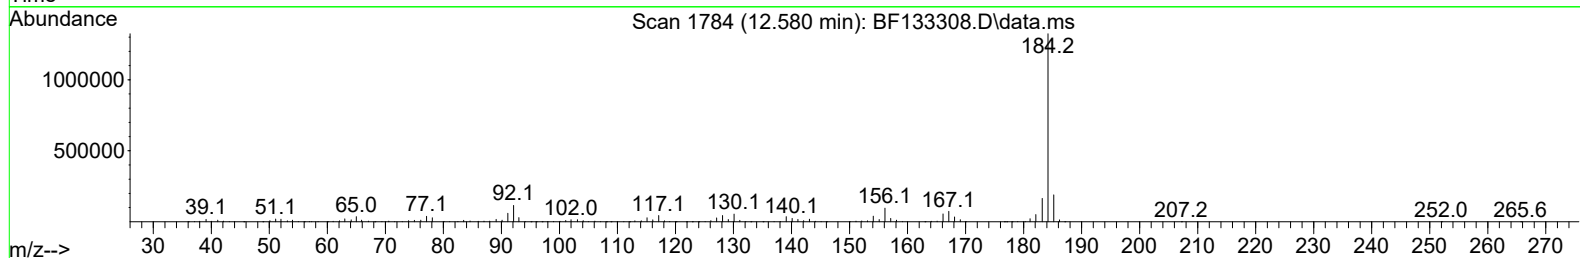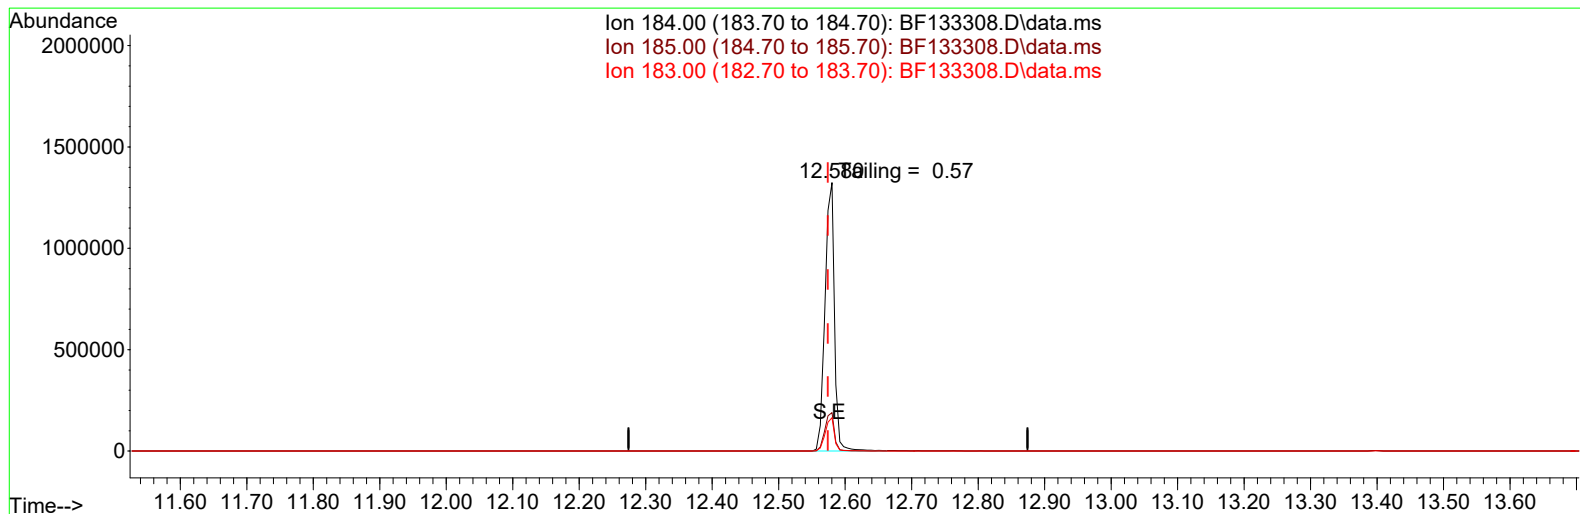

TIC: BF133308.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 0.00 ng

response 1313324

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.34#
183.00	11.70	12.40
0.00	0.00	0.00