


Data Path : Z:\HPCHEM1\BNA F\Data\BF051016\
 Data File : BF086852.D
 Acq On : 10 May 2016 10:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 16:04:56 2016

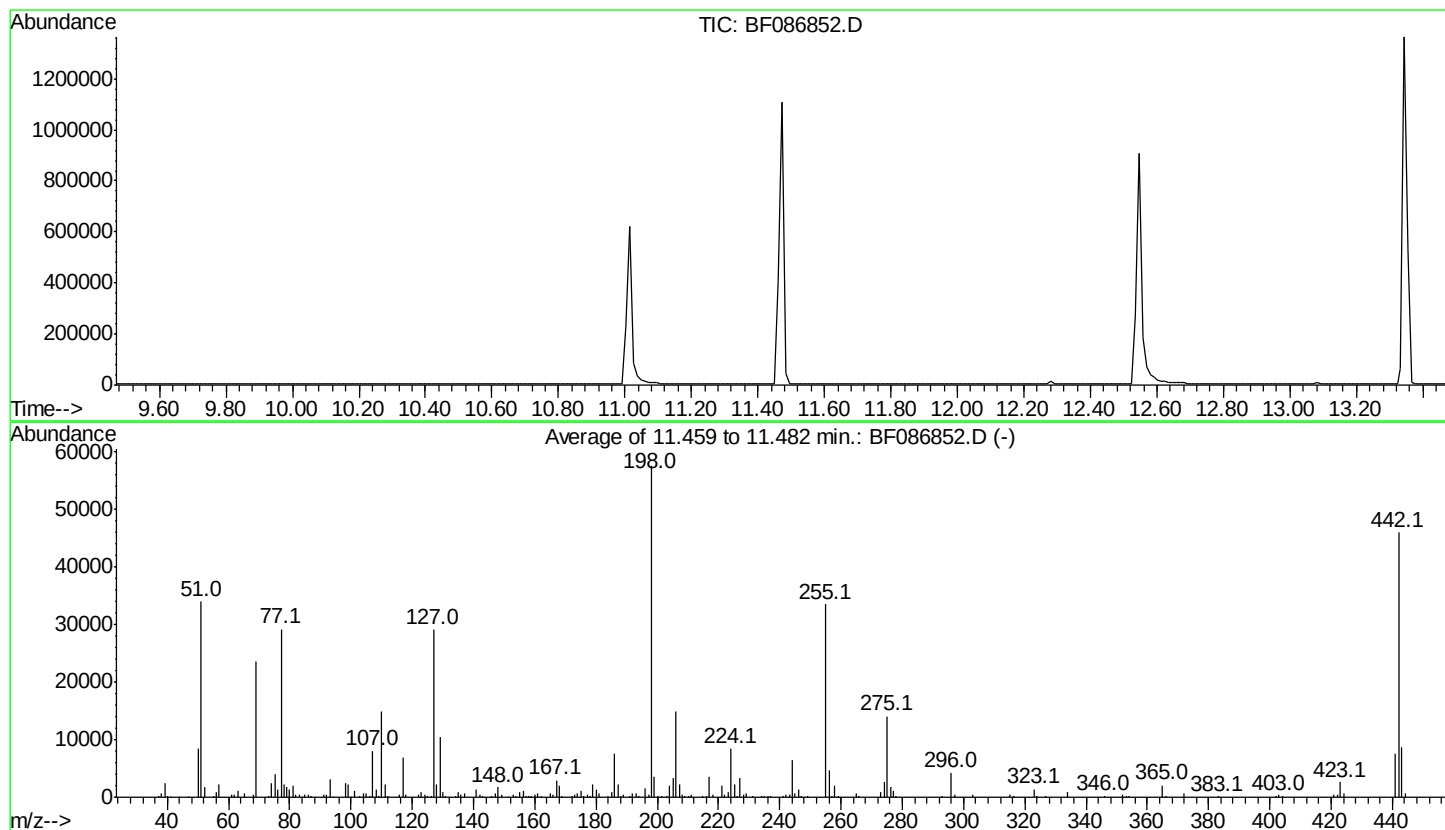

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	33898	PASS
68	69	0.00	2	1.9	446	PASS
69	198	0.00	100	41.1	23647	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	29026	PASS
197	198	0.00	2	0.6	362	PASS
198	198	100	100	100.0	57513	PASS
199	198	5	9	6.3	3616	PASS
275	198	10	60	24.4	14049	PASS
365	198	1	100	3.5	2018	PASS
441	442	0.01	24	16.4	7519	PASS
442	198	50	100	79.7	45866	PASS
443	442	15	24	18.7	8561	PASS