


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051016\
 Data File : BF086875.D
 Acq On : 11 May 2016 1:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 16:04:56 2016

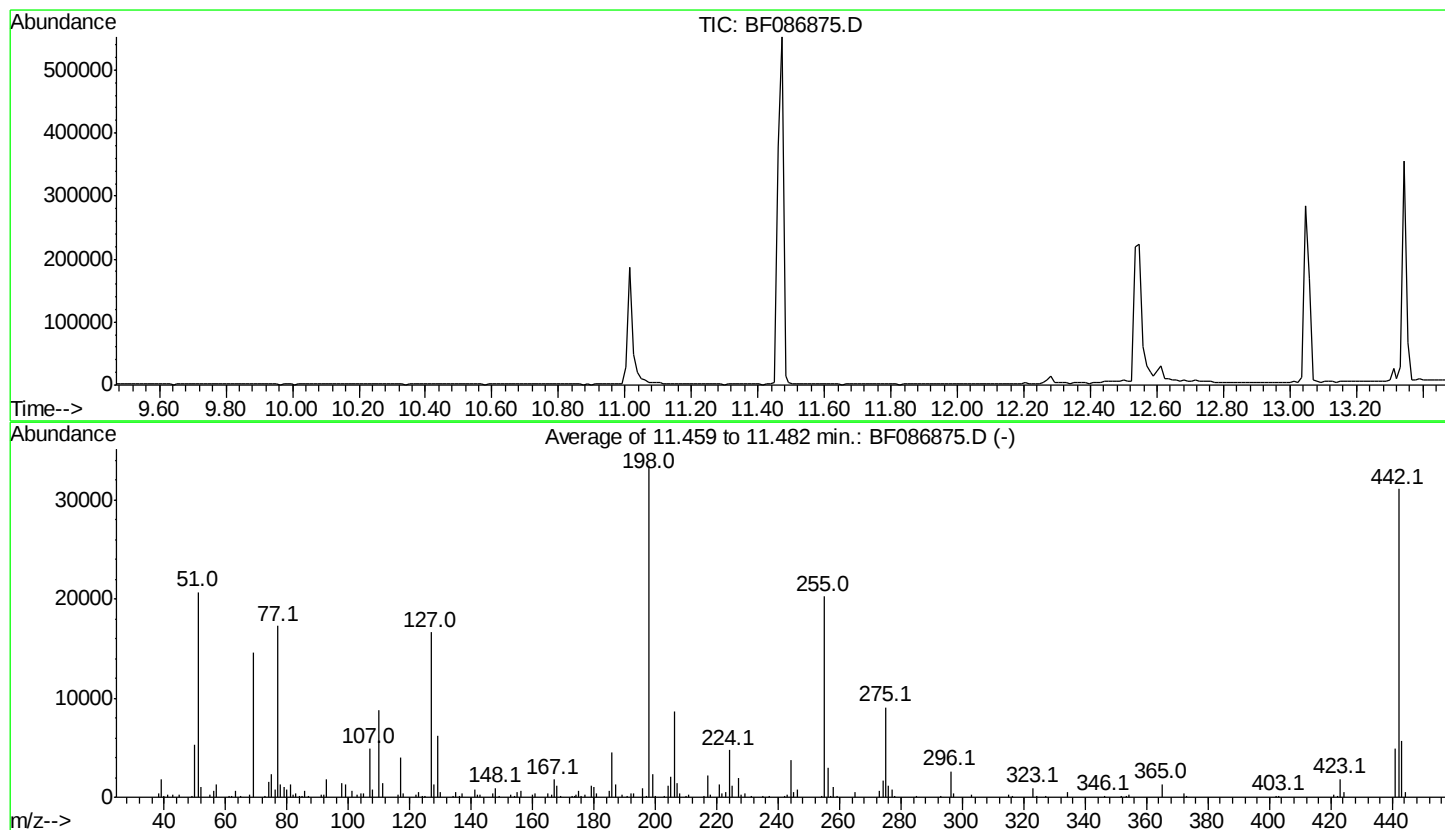

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.8	20663	PASS
68	69	0.00	2	1.4	210	PASS
69	198	0.00	100	43.5	14535	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	16616	PASS
197	198	0.00	2	0.5	180	PASS
198	198	100	100	100.0	33444	PASS
199	198	5	9	6.9	2296	PASS
275	198	10	60	27.0	9044	PASS
365	198	1	100	4.0	1331	PASS
441	442	0.01	24	15.8	4904	PASS
442	198	50	100	93.0	31103	PASS
443	442	15	24	18.4	5734	PASS