
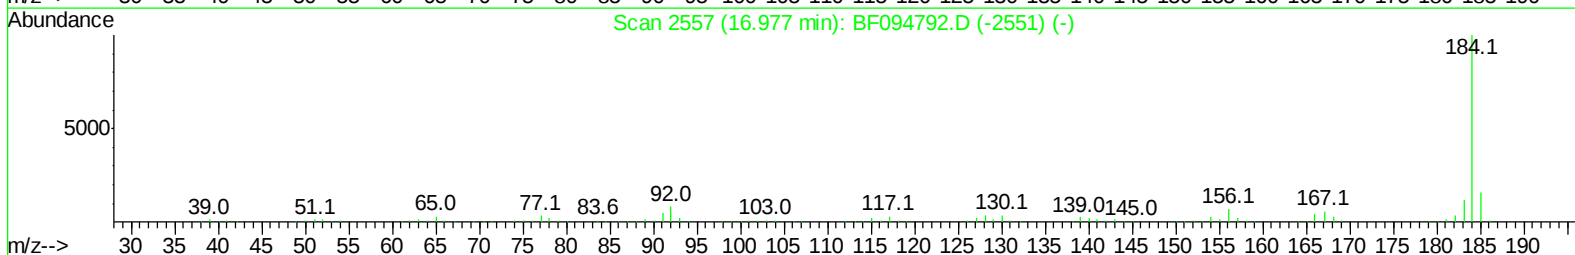
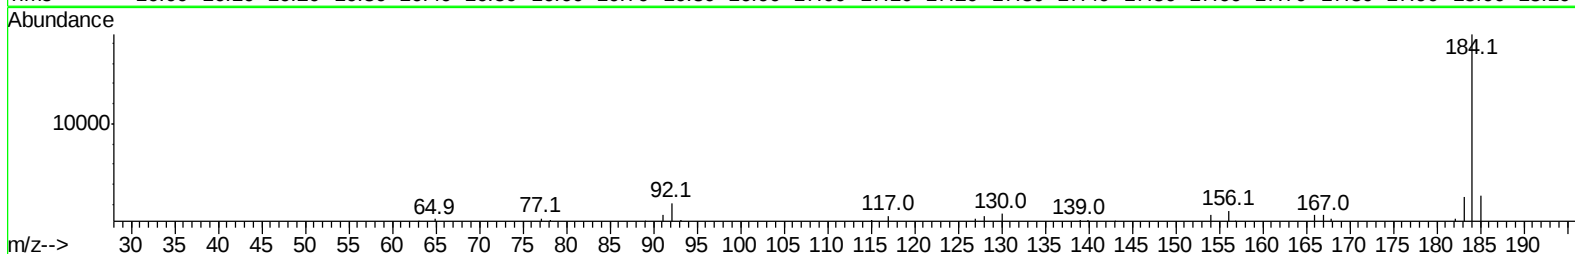


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051017\
Data File : BF095055.D
Acq On : 10 May 2017 14:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 18:20:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

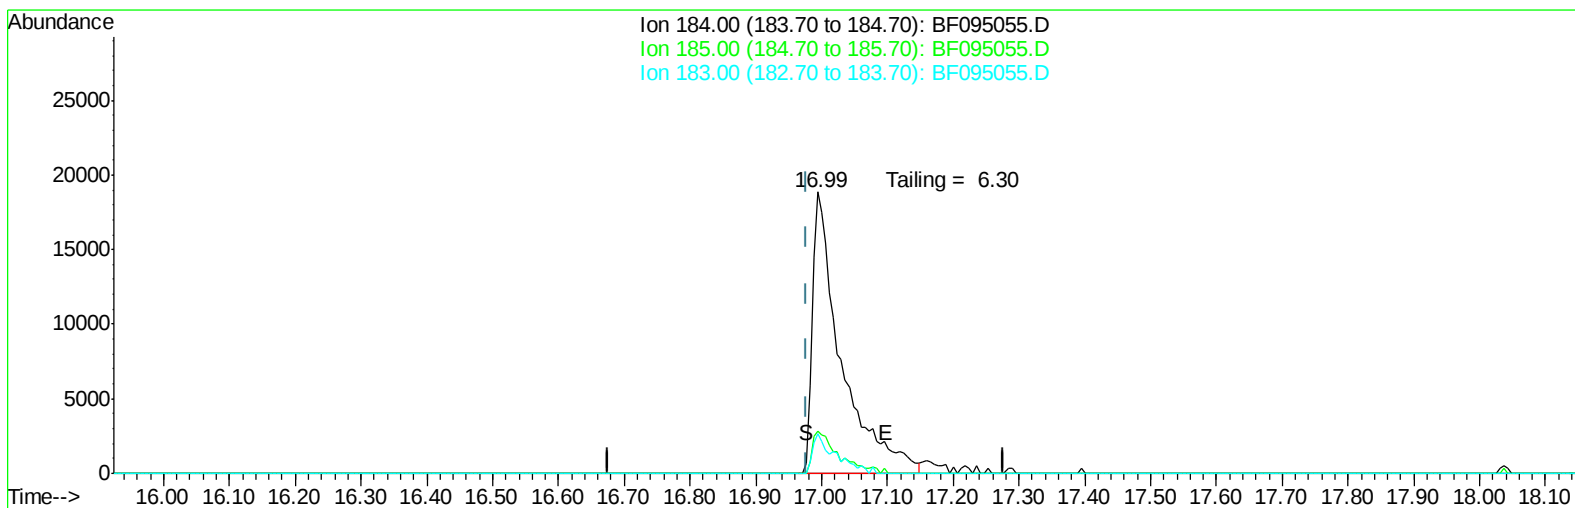

TIC: BF095055.D

(76) Benzidine




16.995min (+0.018) 0.00ng

response 56724

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.11#
183.00	12.20	14.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051017\
Data File : BF095055.D
Acq On : 10 May 2017 14:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 18:20:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

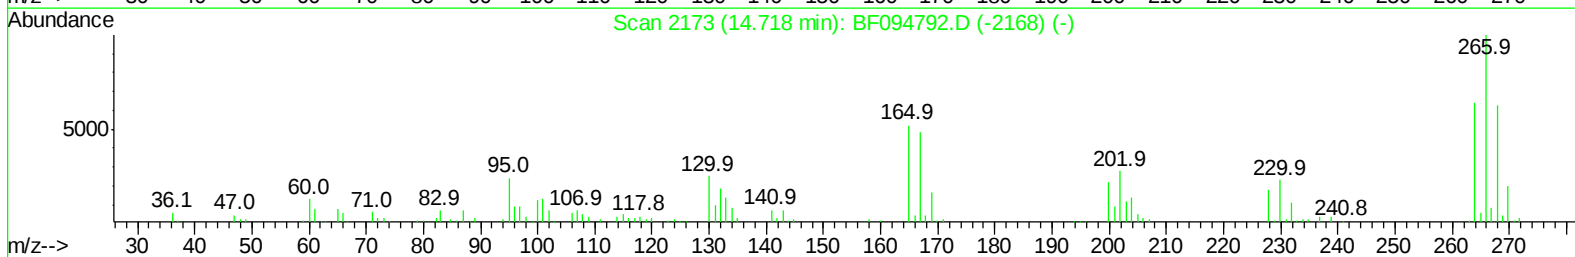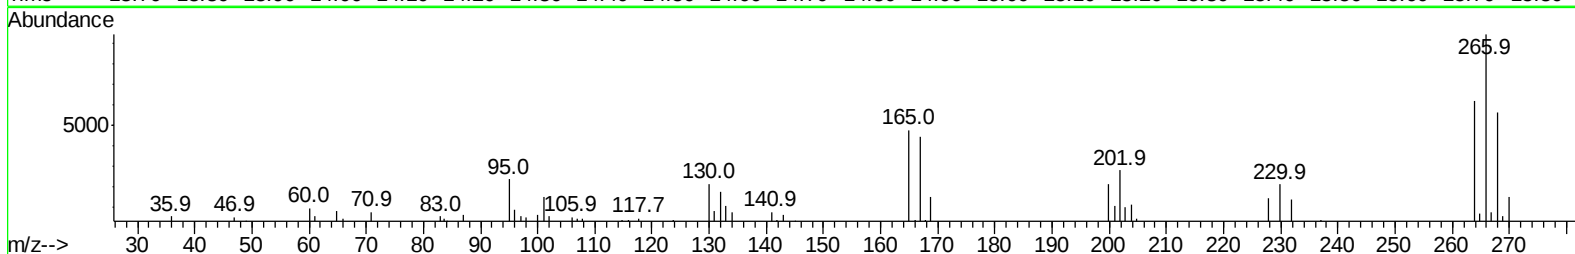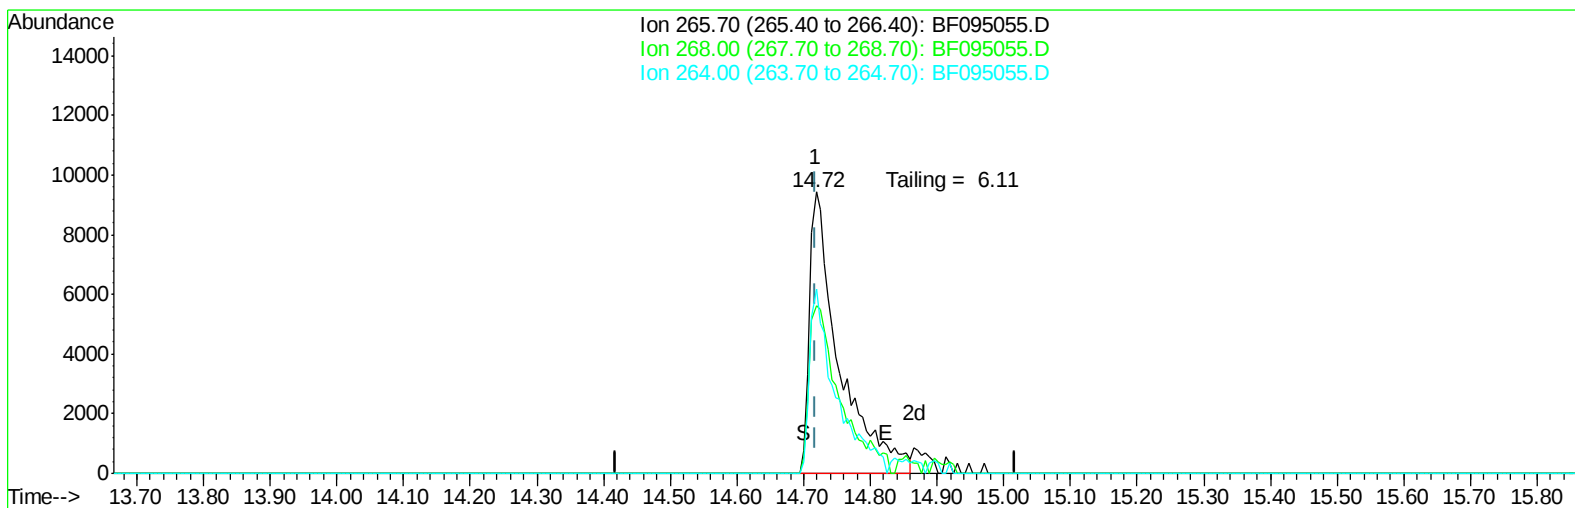

TIC: BF095055.D

(69) Pentachlorophenol (C)

14.718min (+0.000) 0.00ng m

response 28645

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.69
264.00	64.60	65.25
0.00	0.00	0.00