

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051017\
 Data File : BF095061.D
 Acq On : 10 May 2017 17:58
 Operator : SJ/MA
 Sample : I3055-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EFF-WW

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.101	23	28	44	rBV	744743	1026092	2.38%	0.220%
2	4.048	353	359	370	rBV	731628	1358735	3.15%	0.292%
3	4.342	404	409	420	rVB	439806	700382	1.62%	0.150%
4	5.054	522	530	536	rBV	884349	1594519	3.70%	0.342%
5	5.566	612	617	622	rBV2	818333	1578513	3.66%	0.339%
6	5.842	622	664	667	rVV2	3829370	36927583	85.59%	7.928%
7	5.889	669	672	684	rVV2	511517	1244017	2.88%	0.267%
8	6.042	693	698	713	rVB	832770	1396198	3.24%	0.300%
9	6.284	719	739	741	rBV	5375079	22144983	51.33%	4.754%
10	6.966	850	855	860	rBV	752376	847347	1.96%	0.182%
11	7.172	884	890	901	rBV	399877	1239191	2.87%	0.266%
12	7.325	913	916	921	rVB	636573	742454	1.72%	0.159%
13	7.431	930	934	943	rVV	712840	1235665	2.86%	0.265%
14	7.707	977	981	988	rBV	436545	627376	1.45%	0.135%
15	7.925	1008	1018	1019	rBV	2757048	6089250	14.11%	1.307%
16	7.948	1019	1022	1026	rVV2	1226318	2757582	6.39%	0.592%
17	8.295	1070	1081	1087	rVB2	442468	1043338	2.42%	0.224%
18	8.525	1107	1120	1123	rVV	3483020	9440200	21.88%	2.027%
19	8.625	1132	1137	1141	rBV	840345	1506061	3.49%	0.323%
20	8.854	1158	1176	1179	rVV	5924095	26013437	60.29%	5.585%
21	9.036	1205	1207	1209	rVB	1179114	821836	1.90%	0.176%
22	9.207	1225	1236	1239	rBV2	410494	895329	2.08%	0.192%
23	9.272	1239	1247	1249	rBV3	328979	725894	1.68%	0.156%
24	9.736	1321	1326	1329	rBV	771676	1052864	2.44%	0.226%
25	9.813	1334	1339	1341	rBV2	492646	725418	1.68%	0.156%
26	9.895	1350	1353	1356	rBV2	578139	739242	1.71%	0.159%
27	10.172	1396	1400	1408	rVB	1001684	1153346	2.67%	0.248%
28	10.601	1465	1473	1477	rBV2	578487	1450050	3.36%	0.311%
29	10.848	1503	1515	1517	rBV	5483571	12174892	28.22%	2.614%
30	11.513	1611	1628	1631	rBV	2757574	5075075	11.76%	1.090%
31	11.683	1655	1657	1659	rVB	1748330	1272731	2.95%	0.273%
32	11.842	1667	1684	1692	rVB3	4082161	9114041	21.12%	1.957%
33	12.354	1761	1771	1777	rBV5	504489	1804873	4.18%	0.387%
34	12.601	1802	1813	1816	rBV2	4148498	7378296	17.10%	1.584%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051017\
 Data File : BF095061.D
 Acq On : 10 May 2017 17:58
 Operator : SJ/MA
 Sample : I3055-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EFF-WW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.330	1895	1937	1940	rBV2	2933251	22053290	51.11%	4.735%
36	13.454	1953	1958	1966	rBV	564803	924196	2.14%	0.198%
37	13.530	1966	1971	1978	rVV	757860	1268905	2.94%	0.272%
38	13.877	2024	2030	2042	rBV5	326886	1209714	2.80%	0.260%
39	14.183	2074	2082	2091	rVB	3709123	6436139	14.92%	1.382%
40	14.354	2105	2111	2114	rVV	1037697	2214338	5.13%	0.475%
41	14.401	2114	2119	2123	rVV	2337130	5271449	12.22%	1.132%
42	14.442	2123	2126	2150	rVV	1567362	3821311	8.86%	0.820%
43	14.689	2153	2168	2180	rVV3	1149775	4924374	11.41%	1.057%
44	15.054	2224	2230	2241	rVB	403935	785201	1.82%	0.169%
45	15.371	2279	2284	2292	rBV	387253	819779	1.90%	0.176%
46	15.565	2311	2317	2326	rVB	2285464	3693773	8.56%	0.793%
47	15.995	2376	2390	2399	rBV6	1167265	5527919	12.81%	1.187%
48	16.295	2436	2441	2447	rVB3	323468	753726	1.75%	0.162%
49	16.659	2499	2503	2507	rBV6	365166	690812	1.60%	0.148%
50	16.712	2507	2512	2518	rBV	1787760	3032256	7.03%	0.651%
51	16.959	2544	2554	2556	rBV6	1257651	3632777	8.42%	0.780%
52	17.236	2594	2601	2605	rBV2	1840008	4191846	9.72%	0.900%
53	17.289	2605	2610	2619	rVB3	2219697	5245815	12.16%	1.126%
54	17.424	2630	2633	2640	rVB4	447166	833802	1.93%	0.179%
55	17.600	2659	2663	2669	rVB2	407146	769748	1.78%	0.165%
56	17.718	2669	2683	2687	rBV	5293277	15824408	36.68%	3.397%
57	17.789	2687	2695	2697	rBV	2087750	4418566	10.24%	0.949%
58	17.818	2697	2700	2710	rVV	1973579	5544613	12.85%	1.190%
59	17.936	2711	2720	2729	rVV2	3505522	12068475	27.97%	2.591%
60	18.018	2729	2734	2739	rVV	1871831	2988539	6.93%	0.642%
61	18.153	2750	2757	2765	rBV3	3082656	9898873	22.94%	2.125%
62	18.218	2765	2768	2771	rVV3	590453	951472	2.21%	0.204%
63	18.365	2788	2793	2801	rVB2	1055629	2553343	5.92%	0.548%
64	18.659	2820	2843	2846	rBV2	6236209	43145286	100.00%	9.263%
65	18.730	2852	2855	2857	rVB	1355177	1235232	2.86%	0.265%
66	18.765	2857	2861	2864	rVV	2746844	4641354	10.76%	0.996%
67	18.794	2864	2866	2870	rVB	3089241	3154290	7.31%	0.677%
68	18.853	2870	2876	2880	rVB	1529125	2107953	4.89%	0.453%
69	18.930	2885	2889	2891	rBV	960168	1338279	3.10%	0.287%
70	18.994	2897	2900	2903	rVB	1427579	1654819	3.84%	0.355%
71	19.030	2903	2906	2913	rVB2	1302150	2112251	4.90%	0.453%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051017\
 Data File : BF095061.D
 Acq On : 10 May 2017 17:58
 Operator : SJ/MA
 Sample : I3055-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EFF-WW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	19.089	2913	2916	2925	rBV7	443788	1395527	3.23%	0.300%
73	19.165	2925	2929	2936	rVB	1852792	2489954	5.77%	0.535%
74	19.412	2955	2971	2980	rBV5	5586176	29204741	67.69%	6.270%
75	19.477	2980	2982	2983	rVV	789305	779309	1.81%	0.167%
76	19.506	2983	2987	2990	rVV	2642095	4662649	10.81%	1.001%
77	19.541	2990	2993	2998	rVB	2408670	2868043	6.65%	0.616%
78	19.600	3001	3003	3006	rBV2	720306	641011	1.49%	0.138%
79	19.636	3006	3009	3014	rVB	1264074	2033119	4.71%	0.436%
80	19.677	3014	3016	3019	rVB	708555	685130	1.59%	0.147%
81	19.718	3019	3023	3025	rBV	651370	981027	2.27%	0.211%
82	19.894	3049	3053	3060	rVB	1587787	1957459	4.54%	0.420%
83	20.106	3078	3089	3099	rBV3	5354325	19561551	45.34%	4.200%
84	20.189	3099	3103	3108	rVV	2302151	4537228	10.52%	0.974%
85	20.236	3108	3111	3117	rVV2	1527799	2224483	5.16%	0.478%
86	20.300	3117	3122	3135	rVB2	1894235	5094749	11.81%	1.094%
87	20.412	3135	3141	3144	rBV3	391196	890320	2.06%	0.191%
88	20.588	3167	3171	3178	rVB	998175	1659265	3.85%	0.356%
89	20.812	3201	3209	3216	rBV2	4027631	9730665	22.55%	2.089%
90	20.906	3220	3225	3233	rVB	1315445	2854540	6.62%	0.613%
91	20.977	3233	3237	3241	rBV2	495169	883874	2.05%	0.190%
92	21.030	3242	3246	3249	rBV	523266	865594	2.01%	0.186%
93	21.441	3311	3316	3322	rVB2	381266	777110	1.80%	0.167%
94	21.730	3357	3365	3373	rBV	1866005	3962627	9.18%	0.851%
95	21.847	3378	3385	3396	rVB	661707	1887199	4.37%	0.405%
96	21.977	3398	3407	3416	rVV	431763	1549171	3.59%	0.333%
97	22.088	3419	3426	3443	rVB4	610719	2219318	5.14%	0.476%
98	22.977	3571	3577	3591	rVB2	459418	1418715	3.29%	0.305%
99	23.118	3594	3601	3613	rVB2	205916	672004	1.56%	0.144%
100	23.418	3643	3652	3657	rBV3	496308	1673930	3.88%	0.359%


Sum of corrected areas: 465796045

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051017\
Data File : BF095061.D
Acq On : 10 May 2017 17:58
Operator : SJ/MA
Sample : I3055-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
EFF-WW

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

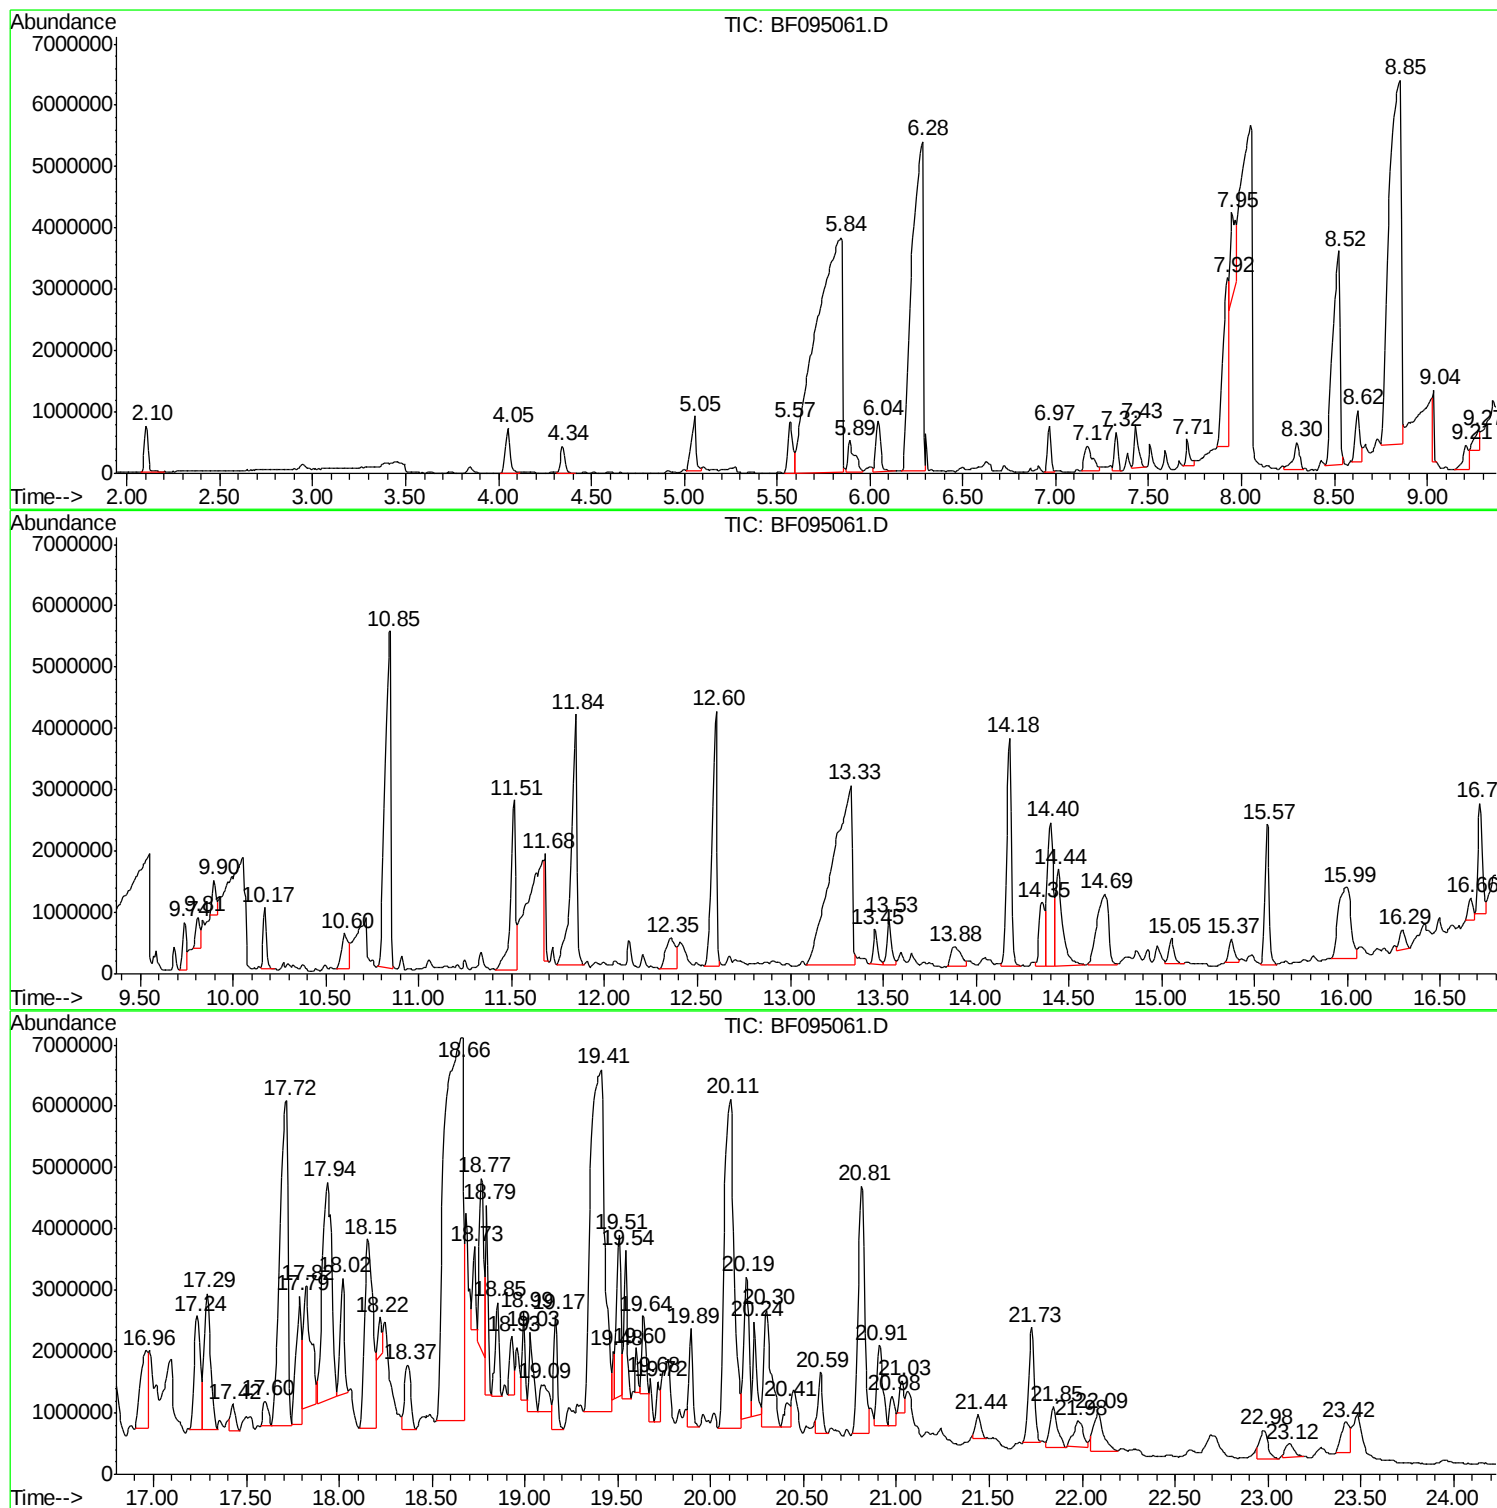

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF051017\
Data_File : BF095061.D
Acq_On : 10 May, 2017 17:588
Operator : SJ/MAA
Sample : I3055-022
Misc :
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
EFF-WW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
