
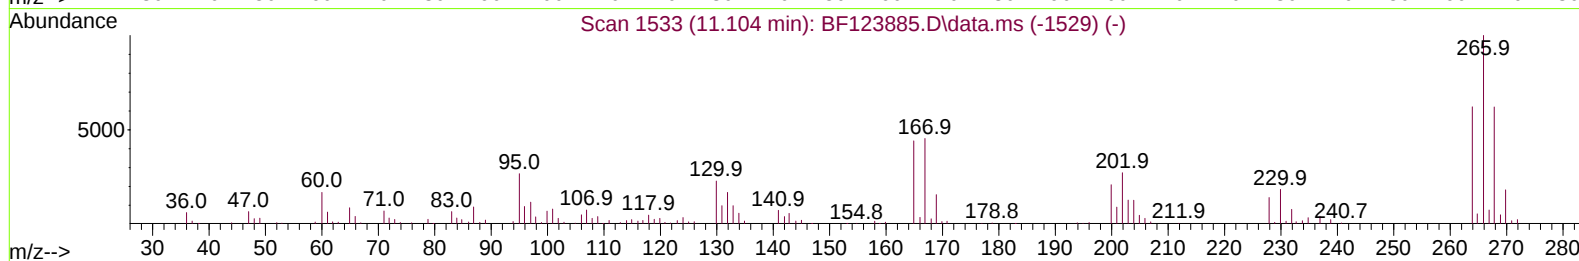
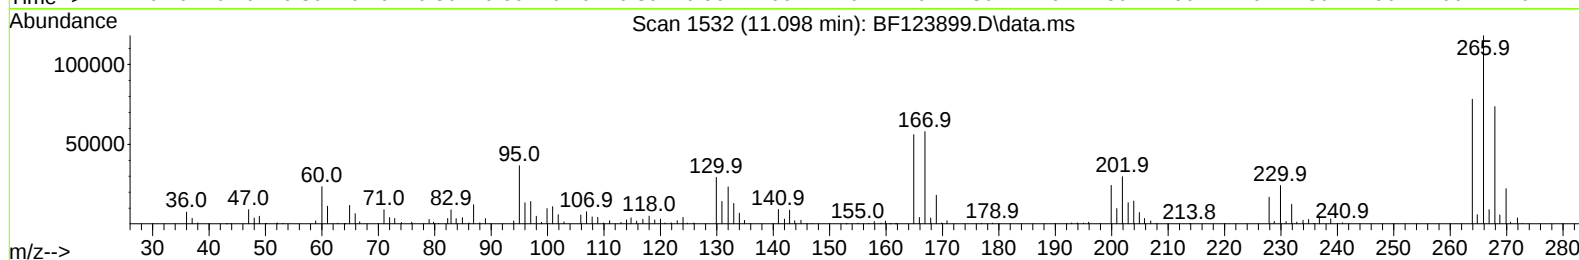


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123899.D
Acq On : 11 May 2021 00:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 05:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 10 16:46:01 2021
Response via : Initial Calibration

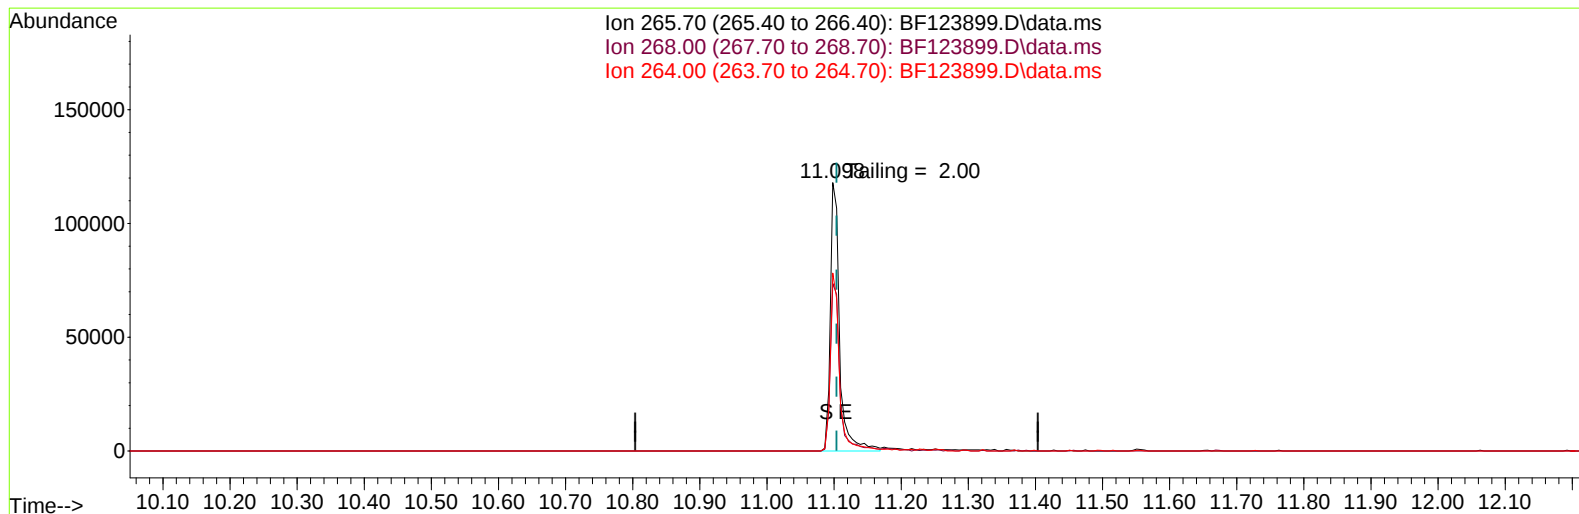

TIC: BF123899.D\data.ms

(70) Pentachlorophenol (C)




11.098min (-0.006) 27460.95 ng

response 116708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.43
264.00	65.70	66.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123899.D
Acq On : 11 May 2021 00:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 05:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 10 16:46:01 2021
Response via : Initial Calibration

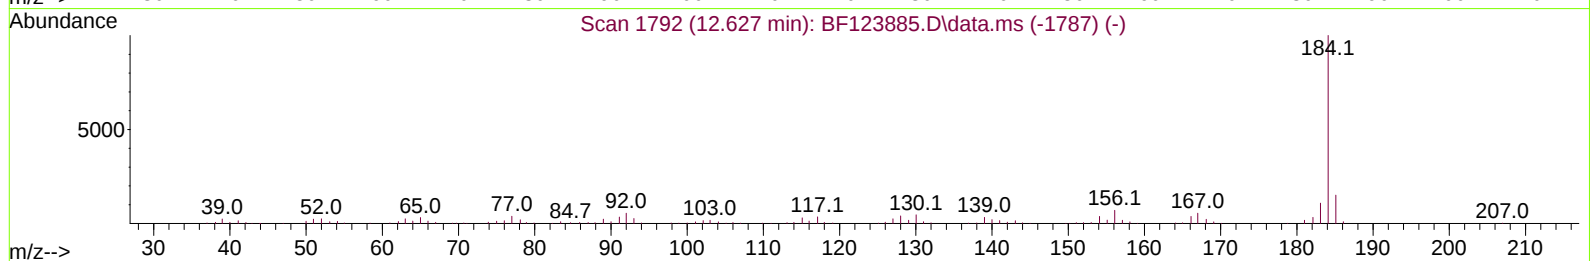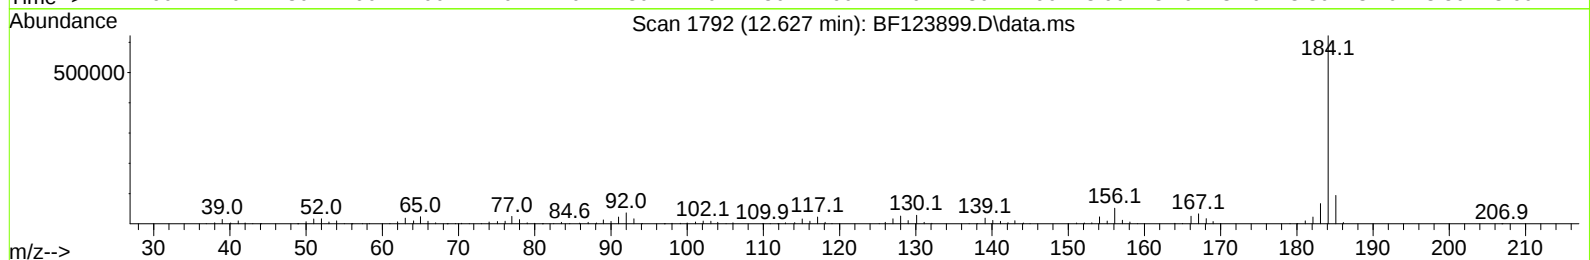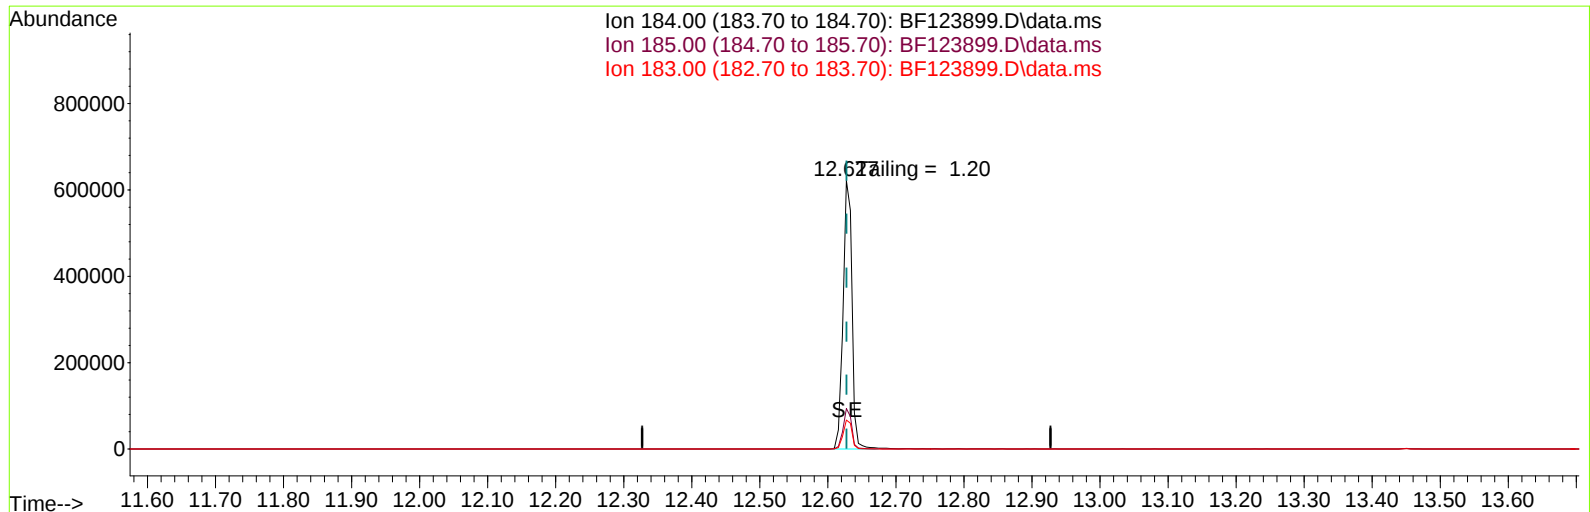

TIC: BF123899.D\data.ms

(77) Benzidine

12.627min (+ 0.000) 0.00 ng

response 567305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.09
183.00	9.80	10.78
0.00	0.00	0.00