

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
 Data File : BF123898.D
 Acq On : 10 May 2021 22:39
 Operator : JU/CG
 Sample : M2322-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-20210505

Quant Time: May 11 03:38:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 10 16:46:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.769	152	113333	20.00	ng	0.00
21) Naphthalene-d8	8.051	136	479437	20.00	ng	0.00
39) Acenaphthene-d10	9.804	164	231874	20.00	ng	0.00
64) Phenanthrene-d10	11.292	188	389037	20.00	ng	# 0.00
76) Chrysene-d12	13.927	240	242621	20.00	ng	# 0.00
86) Perylene-d12	15.368	264	224798	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	781694	100.73	ng	0.01
7) Phenol-d6	6.416	99	901637	87.05	ng	0.00
23) Nitrobenzene-d5	7.333	82	965568	83.60	ng	0.00
42) 2,4,6-Tribromophenol	10.598	330	386402	113.13	ng	0.00
45) 2-Fluorobiphenyl	9.133	172	1331332	71.65	ng	0.00
79) Terphenyl-d14	12.880	244	1599934	107.77	ng	0.00
Target Compounds						
60) Diethylphthalate	10.227	149	89243	4.92	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123898.D
Acq On : 10 May 2021 22:39
Operator : JU/CG
Sample : M2322-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-20210505

Quant Time: May 11 03:38:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 10 16:46:01 2021
Response via : Initial Calibration




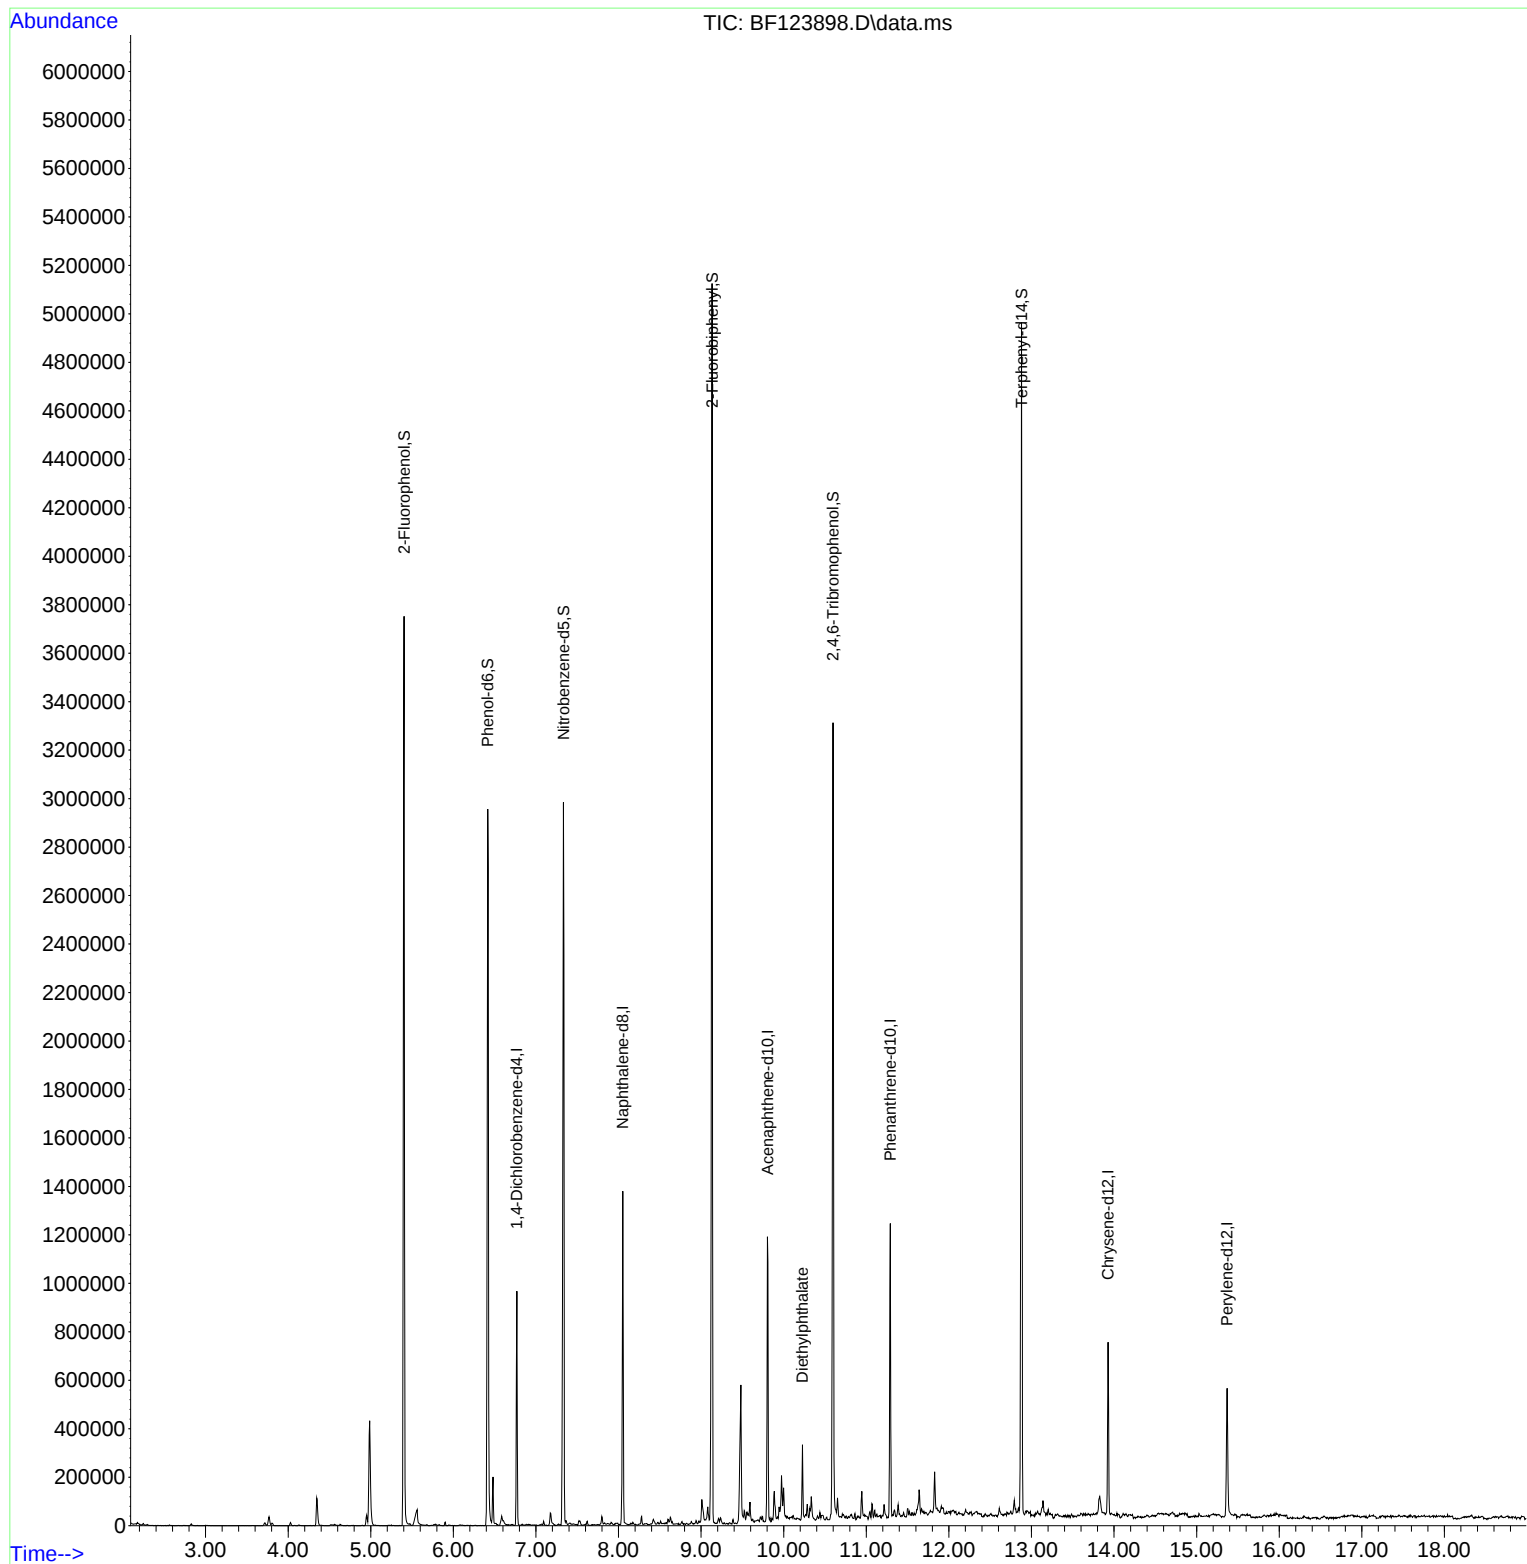


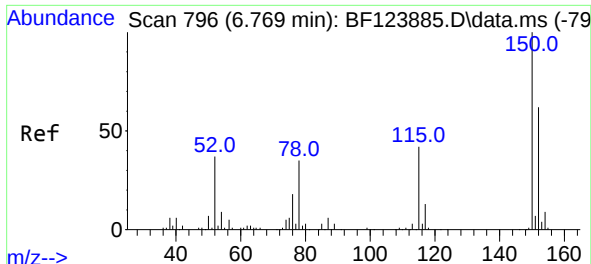

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.769 min Scan# 796
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion:152 Resp: 113333
Ion Ratio Lower Upper
152 100
150 151.5 127.0 190.6
115 62.6 54.3 81.5

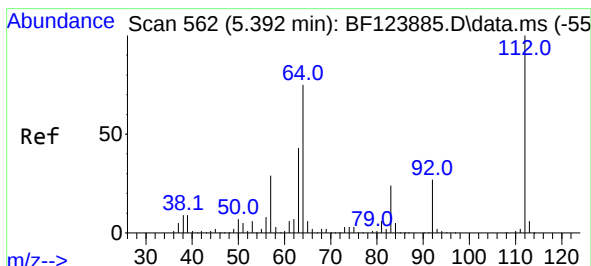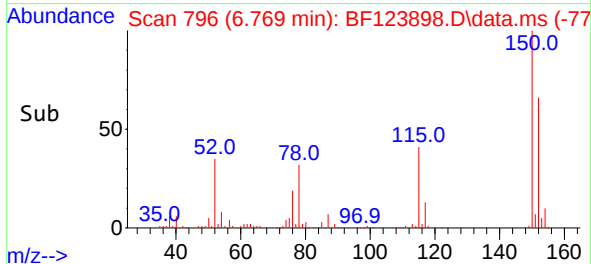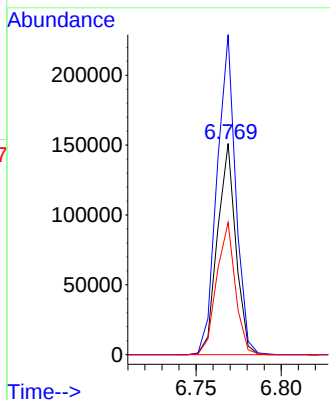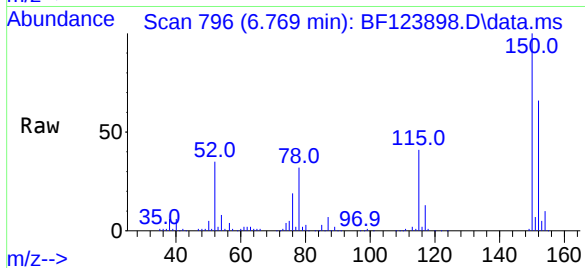

#5
2-Fluorophenol
Concen: 100.73 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.012 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion:112 Resp: 781694
Ion Ratio Lower Upper
112 100
64 78.0 61.4 92.0
63 45.1 33.0 49.4


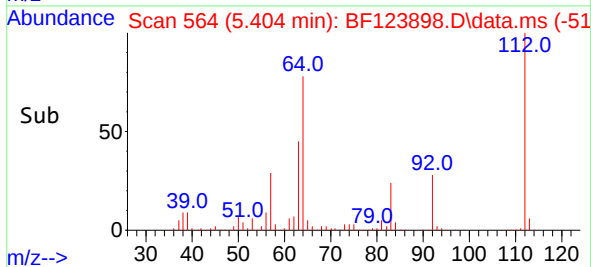
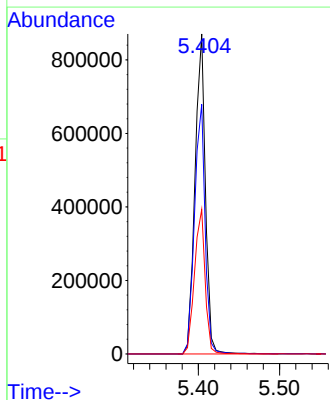
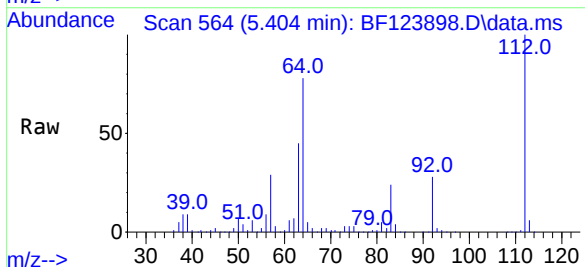


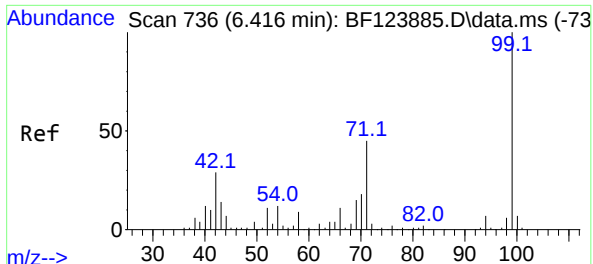

#7
Phenol-d6
Concen: 87.05 ng
RT: 6.416 min Scan# 736
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion: 99 Resp: 901637
Ion Ratio Lower Upper
99 100
42 29.2 19.8 29.8
71 44.8 31.1 46.7

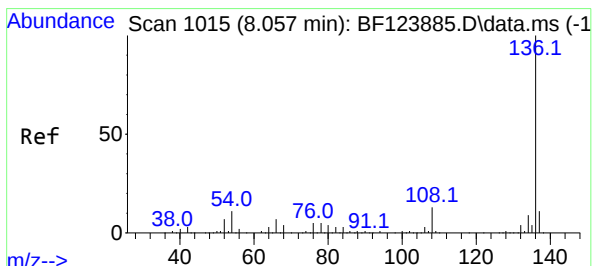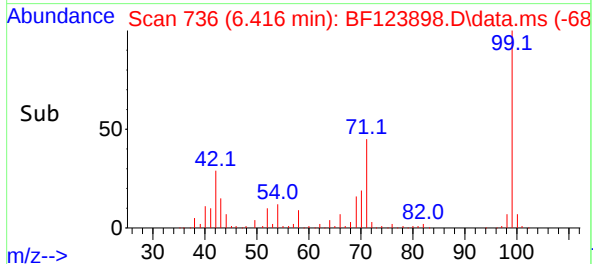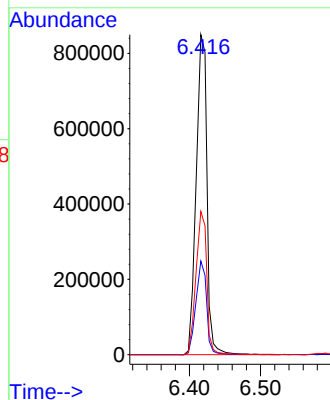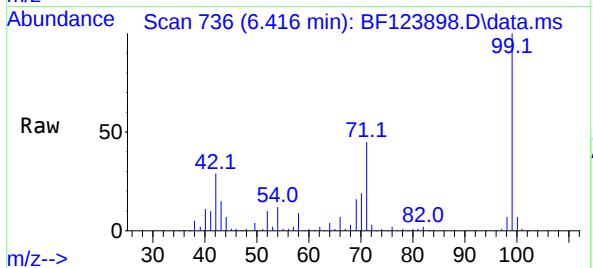

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.051 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion: 136 Resp: 479437
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 12.5 9.8 14.6
68 5.4 4.1 6.1


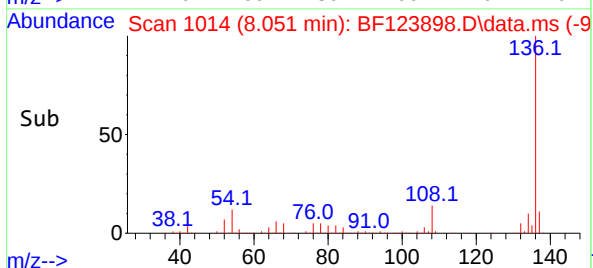
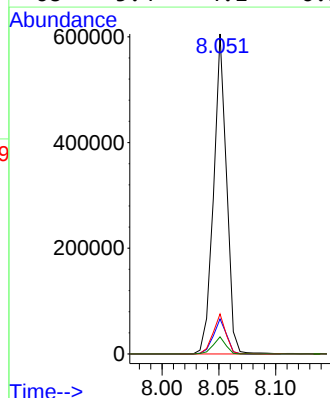
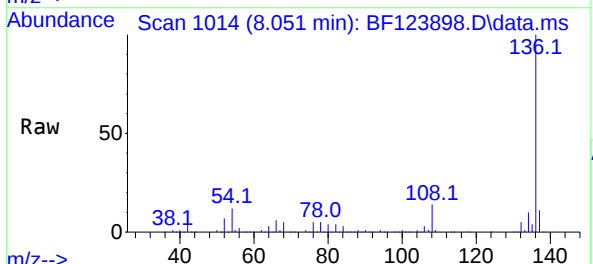


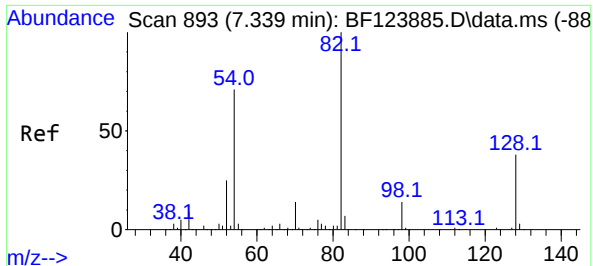

#23
Nitrobenzene-d5
Concen: 83.60 ng
RT: 7.333 min Scan# 892
Delta R.T. -0.006 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion: 82 Resp: 965568
Ion Ratio Lower Upper
82 100
128 36.0 29.4 44.2
54 70.0 54.1 81.1

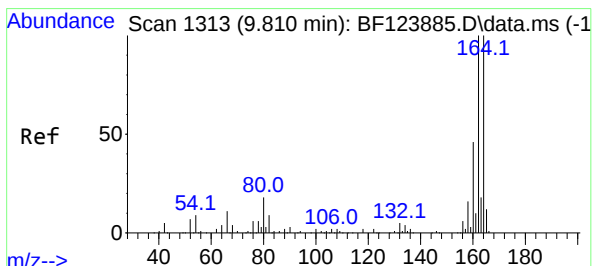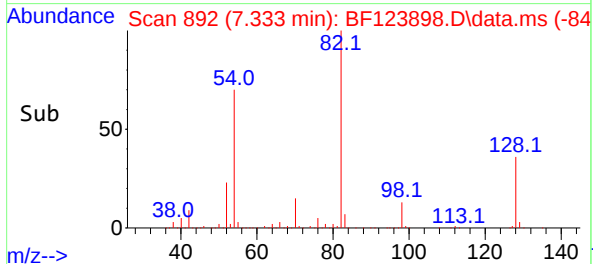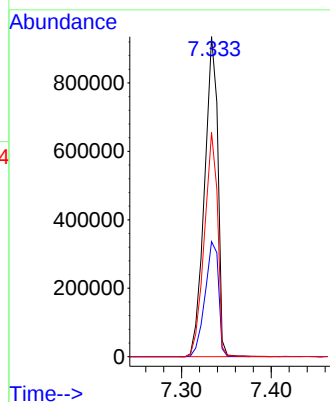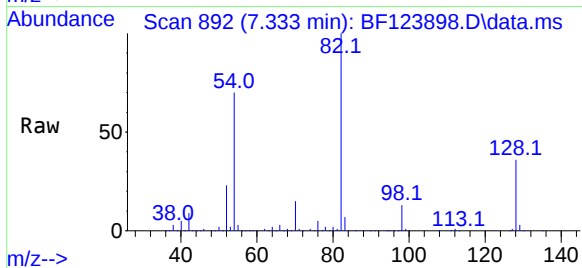

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.804 min Scan# 1312
Delta R.T. -0.006 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion:164 Resp: 231874
Ion Ratio Lower Upper
164 100
162 102.1 80.7 121.1
160 46.1 37.3 55.9


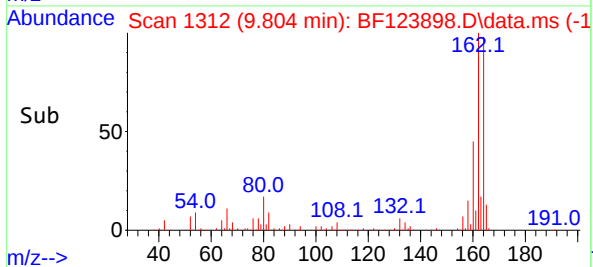
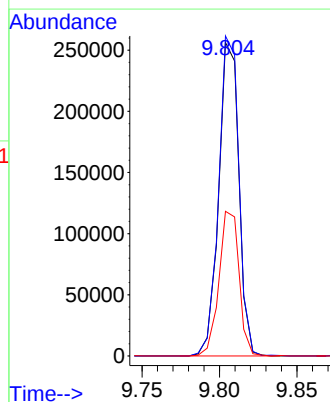
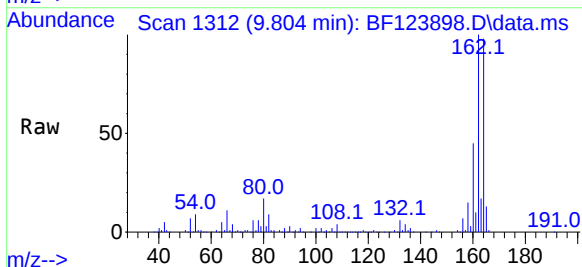


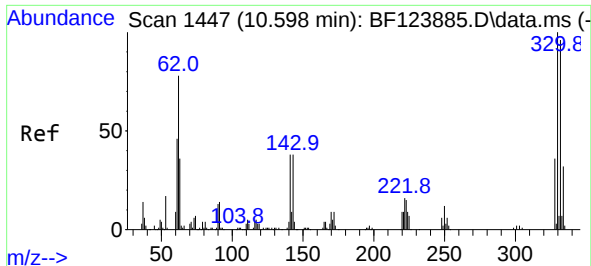

#42
2,4,6-Tribromophenol
Concen: 113.13 ng
RT: 10.598 min Scan# 1447
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion:330 Resp: 386402
Ion Ratio Lower Upper
330 100
332 95.8 77.1 115.7
141 31.8 27.9 41.9

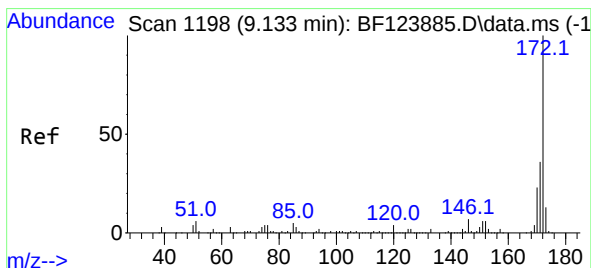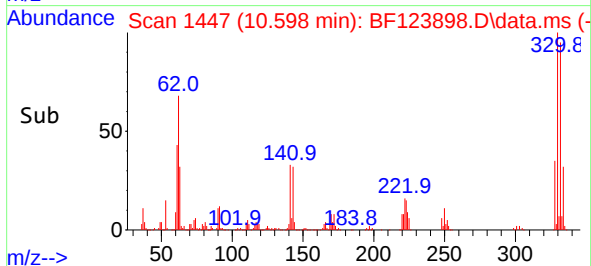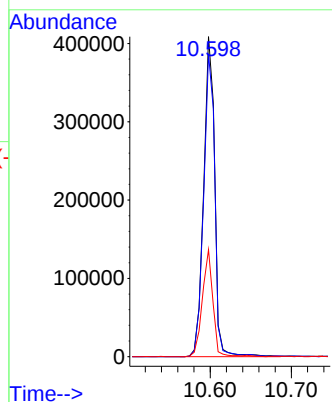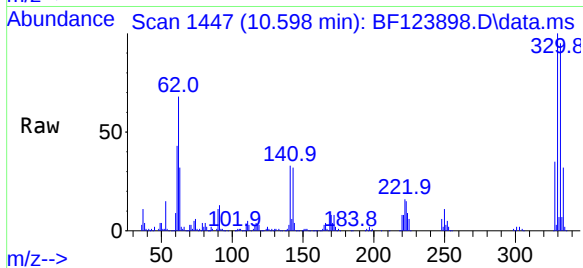

#45
2-Fluorobiphenyl
Concen: 71.65 ng
RT: 9.133 min Scan# 1198
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion:172 Resp: 1331332
Ion Ratio Lower Upper
172 100
171 35.0 28.1 42.1
170 23.1 19.2 28.8


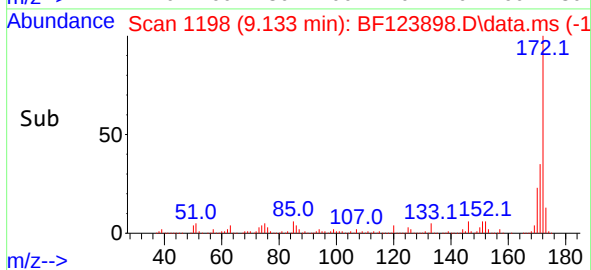
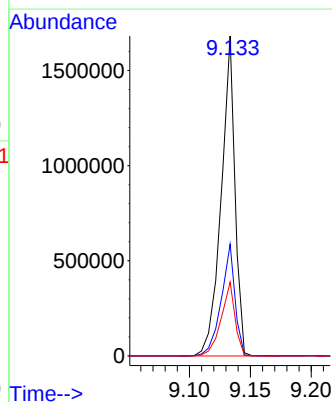
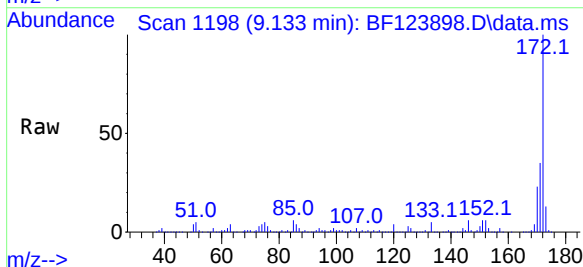


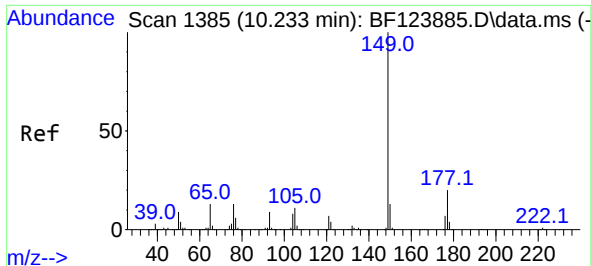

#60
Diethylphthalate
Concen: 4.92 ng
RT: 10.227 min Scan# 1384
Delta R.T. -0.006 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion:149 Resp: 89243
Ion Ratio Lower Upper
149 100
177 18.9 15.4 23.2
150 13.1 9.9 14.9

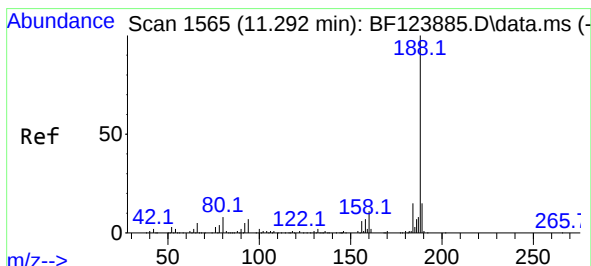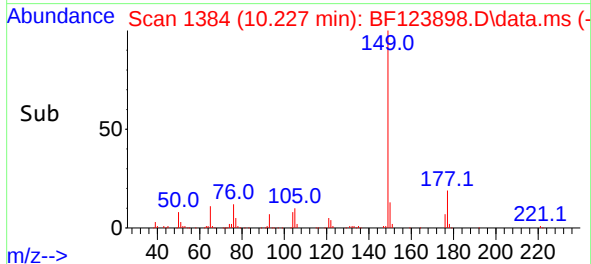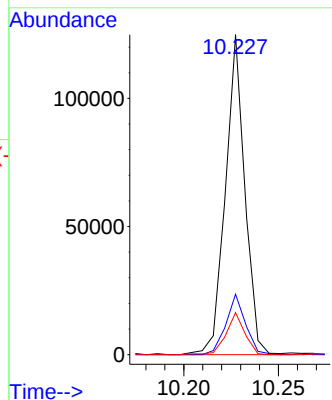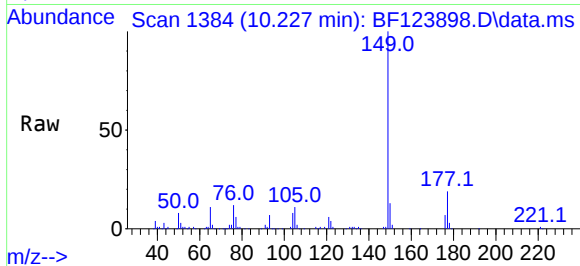

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.292 min Scan# 1565
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion:188 Resp: 389037
Ion Ratio Lower Upper
188 100
94 6.6 6.9 10.3#
80 7.4 8.2 12.2#


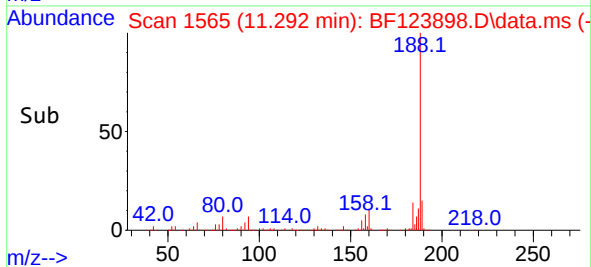
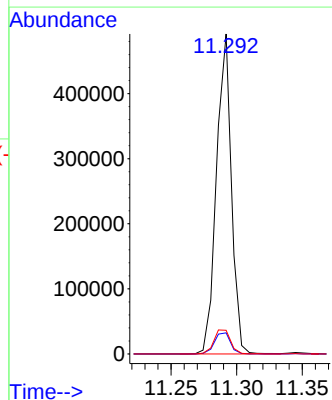
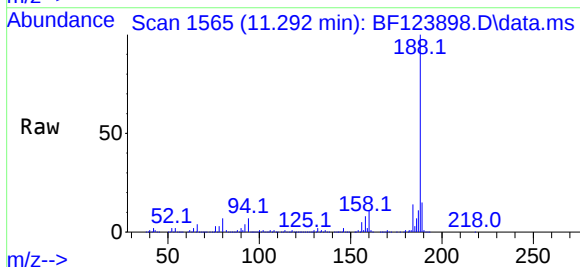


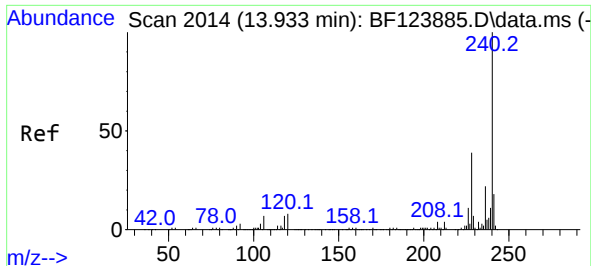

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.927 min Scan# 2013
Delta R.T. -0.006 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39




Instrument :
BNA_F
ClientSampleId :
WC-20210505


Tgt Ion:240 Resp: 242621
Ion Ratio Lower Upper
240 100
120 6.7 7.2 10.8#
236 22.3 19.0 28.4

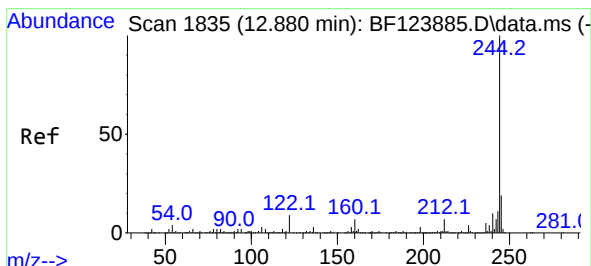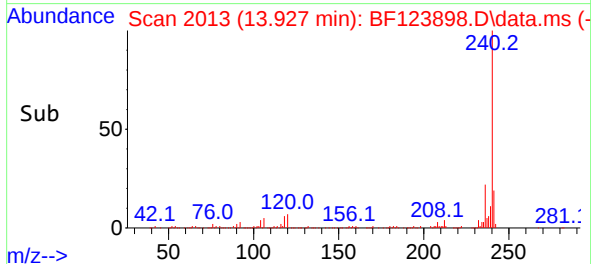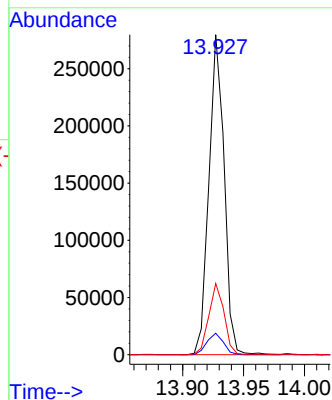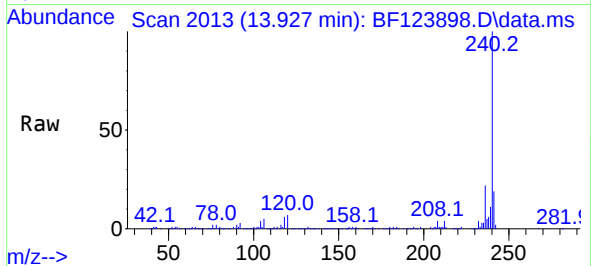

#79
Terphenyl-d14
Concen: 107.77 ng
RT: 12.880 min Scan# 1835
Delta R.T. -0.000 min
Lab File: BF123898.D
Acq: 10 May 2021 22:39

Tgt Ion:244 Resp: 1599934
Ion Ratio Lower Upper
244 100
212 7.2 5.7 8.5
122 10.4 9.7 14.5

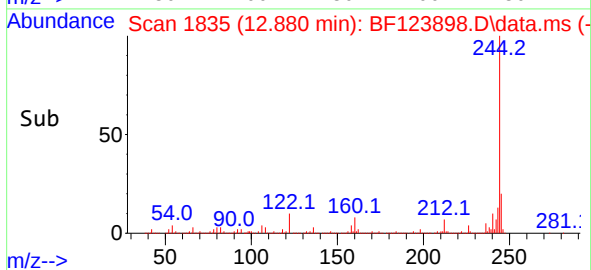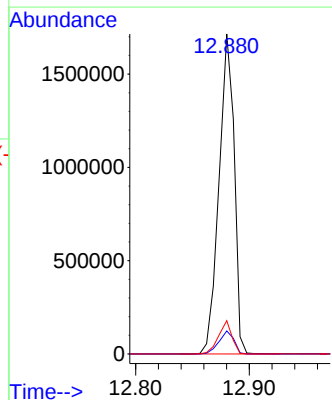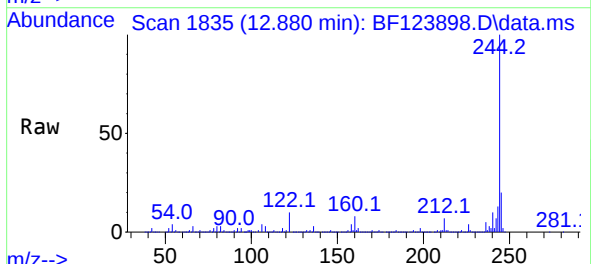

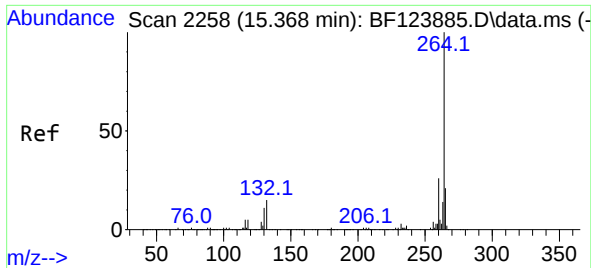

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.368 min Scan# 2258
 Delta R.T. 0.000 min
 Lab File: BF123898.D
 Acq: 10 May 2021 22:39

Instrument :
 BNA_F
 ClientSampleId :
 WC-20210505

Tgt Ion:264 Resp: 224798

Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.7	28.1
265	20.3	17.8	26.8

